

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
 Data File : BE094749.D
 Acq On : 6 Nov 2017 12:44
 Operator : SJ/JU
 Sample : PB103374BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK74

Quant Time: Nov 07 00:12:54 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 00:12:32 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1103	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	7036	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4108	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.44	240	8314	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	593600	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3441	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	9229	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	998	0.07	ng/ul#	24
17) Pyrene	19.65	202	1129	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Quant Time: Nov 07 00:12:54 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

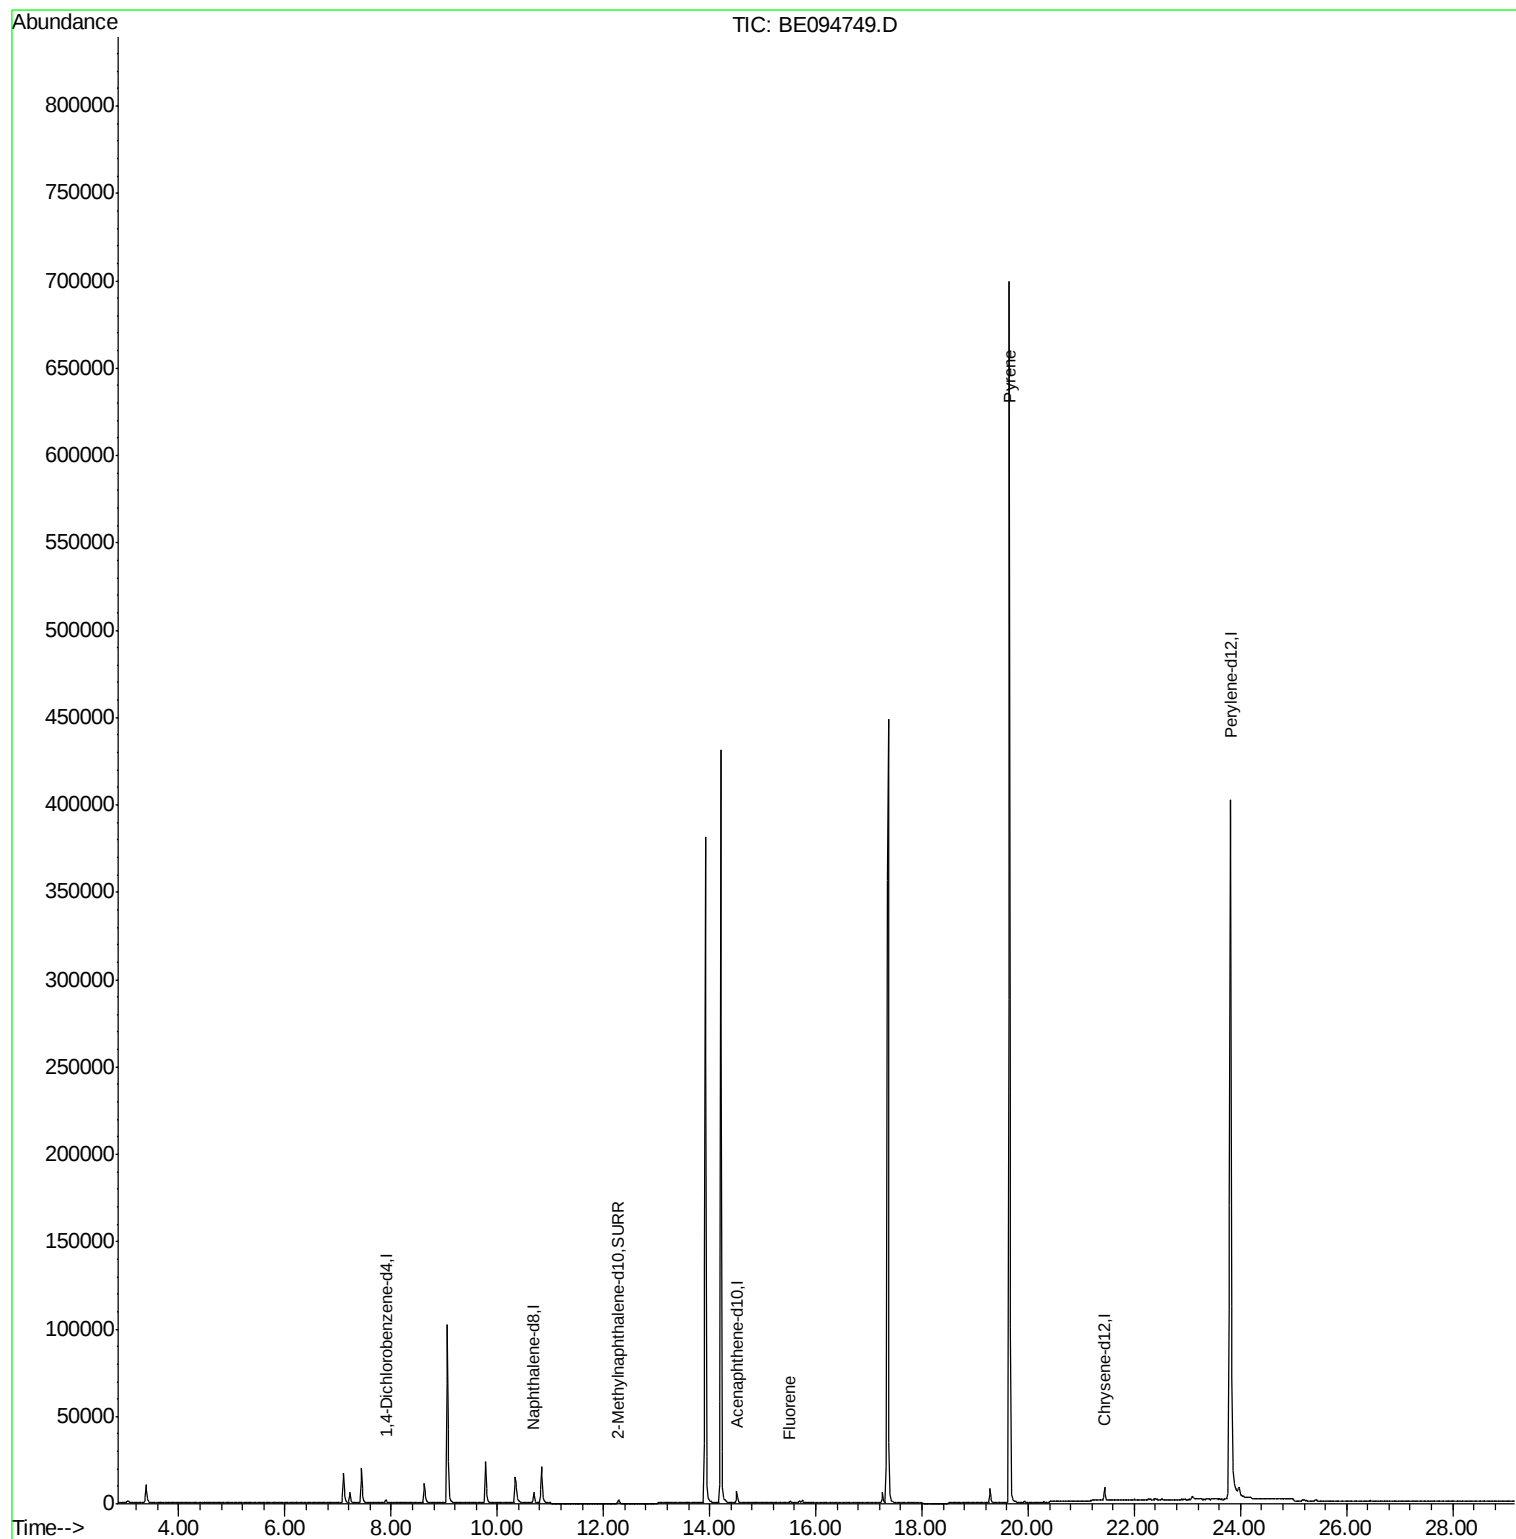

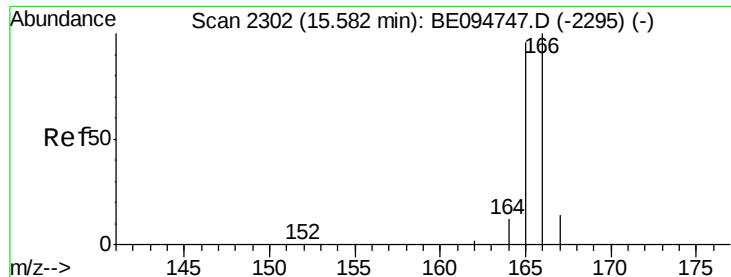

#9

Fluorene

Concen: 0.07 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.08 min

Lab File: BE094749.D

Acq: 6 Nov 2017 12:44

Instrument :

BNA_E

ClientSampleId :

SBLK74


Tot Ion:166 Resp: 998

Ion Ratio Lower Upper

166 100

165 11.8 73.4 110.2#

167 34.8 14.6 22.0#

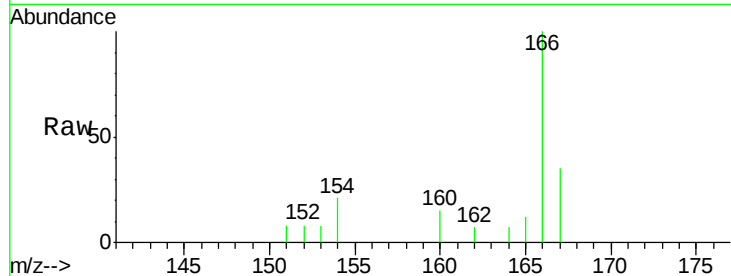

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.51

800

600

400



200

0

15.50

15.60

Time-->

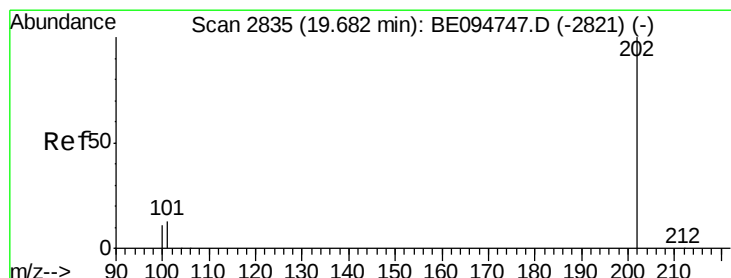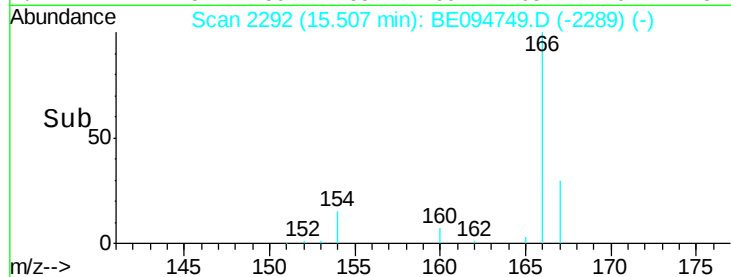

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.65 min Scan# 2827

Delta R.T. -0.03 min

Lab File: BE094749.D

Acq: 6 Nov 2017 12:44


Tgt Ion:202 Resp: 1129

Ion Ratio Lower Upper

202 100

101 146.8 18.2 27.4#

100 765.9 15.6 23.4#

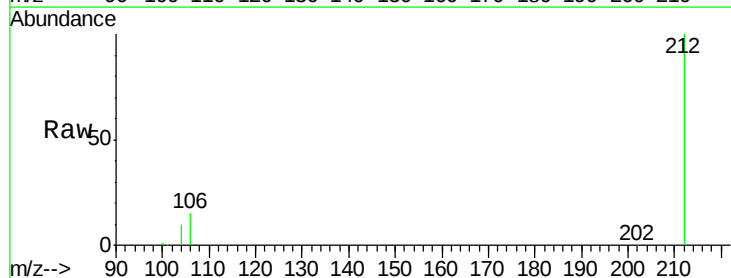

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

19.65

8000

6000

4000

2000

0

19.60

19.70

Time-->

