




Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

Sohil
11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:12:54 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

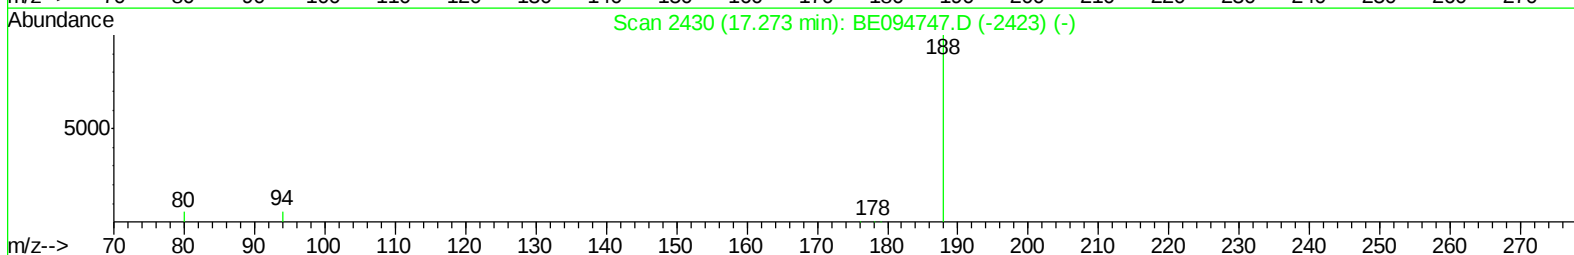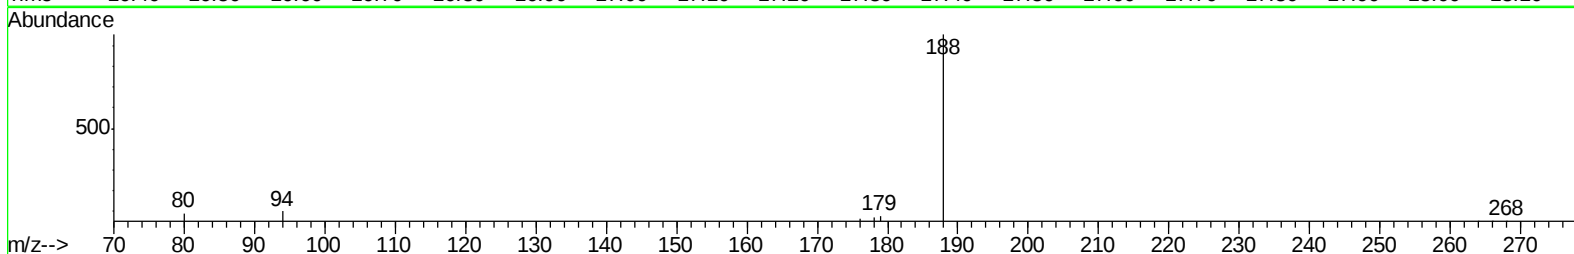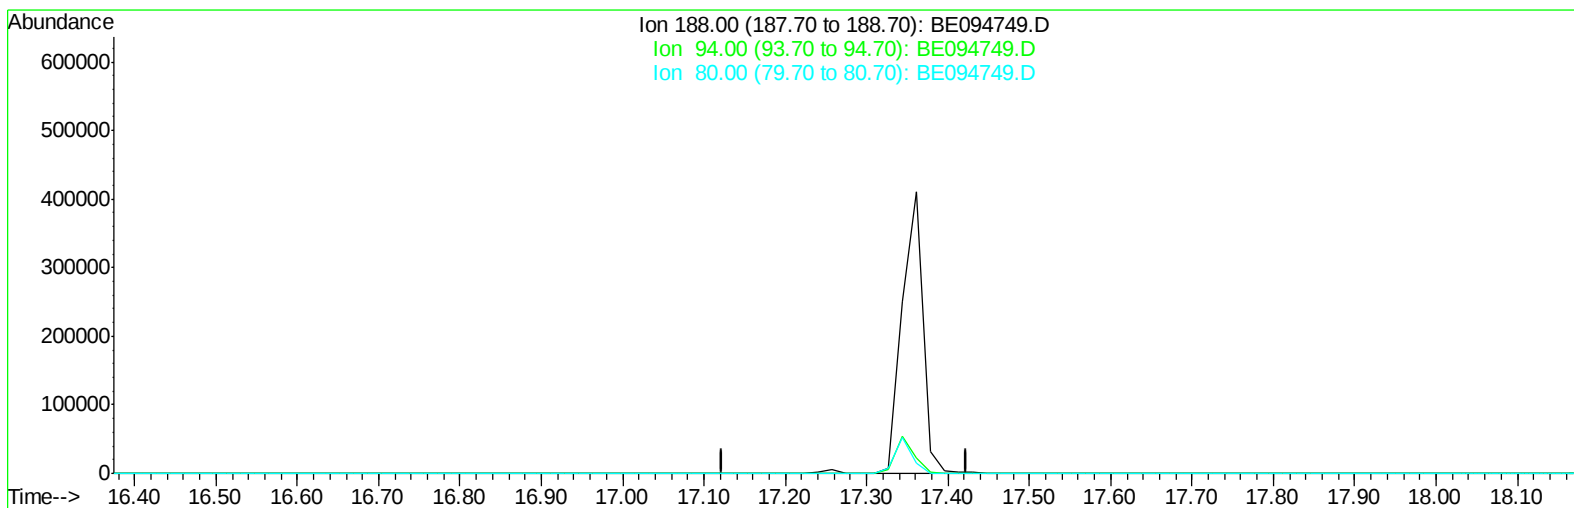

TIC: BE094749.D

(10) Phenanthrene-d10 (I)

17.273min (-17.273) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

Sohil
11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:12:54 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

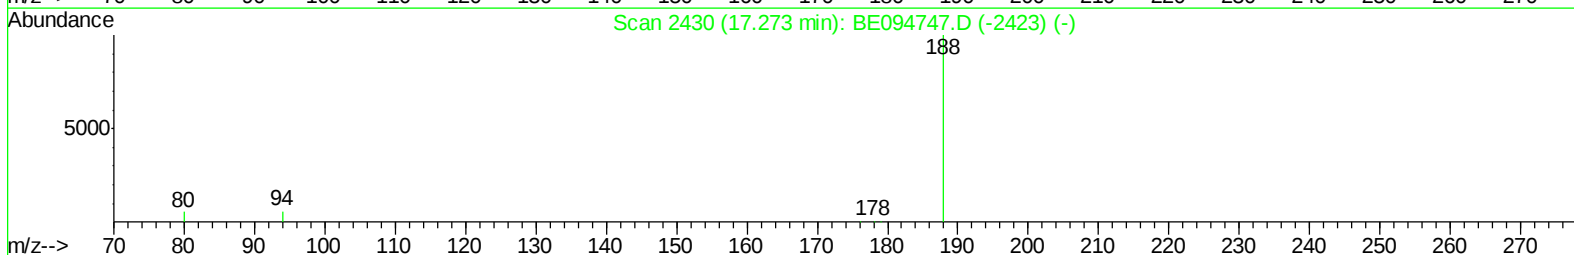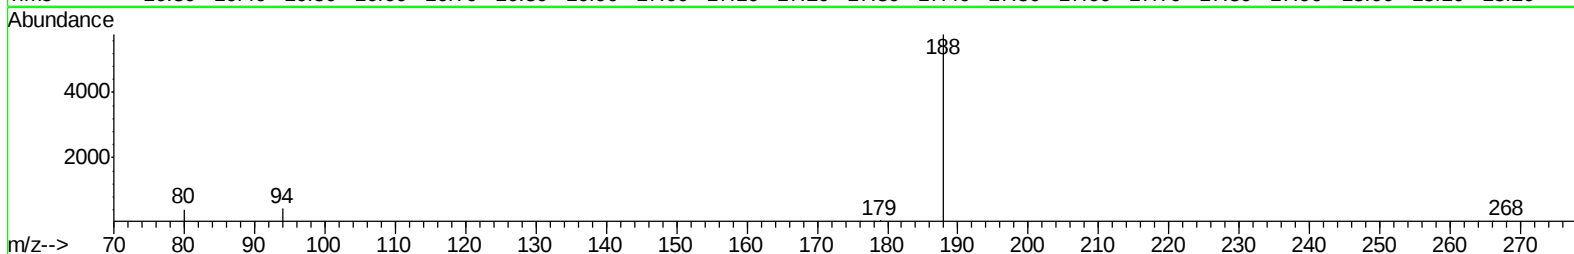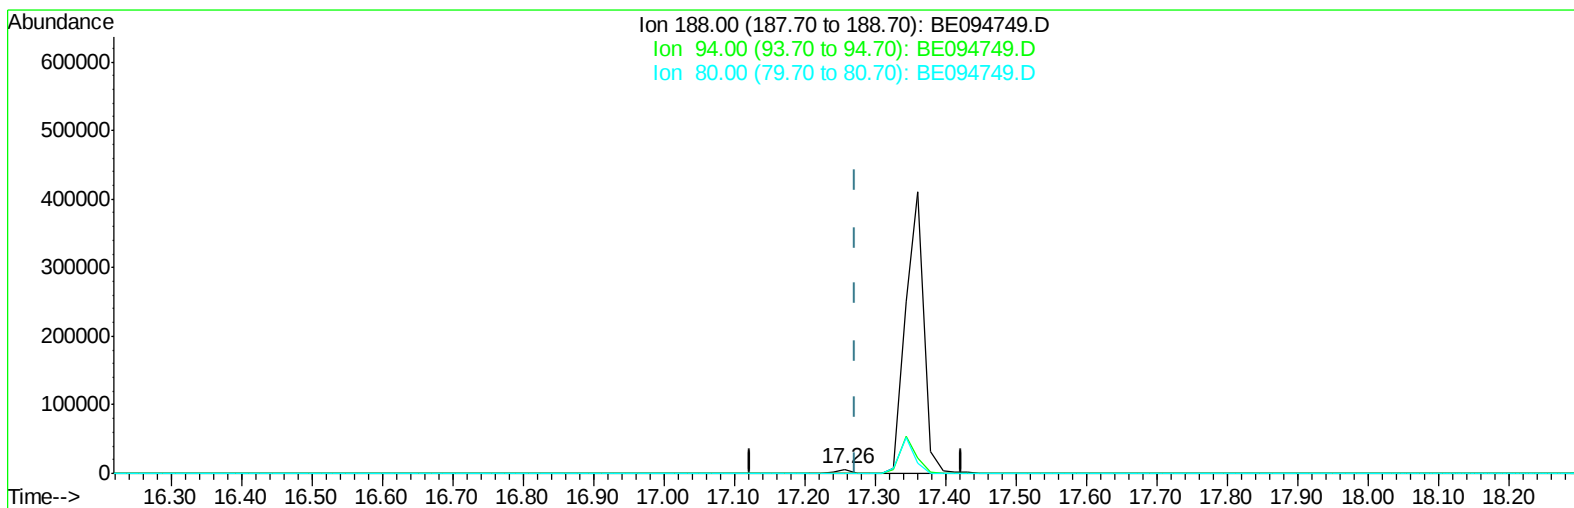

TIC: BE094749.D

(10) Phenanthrene-d10 (I)

17.257min (-0.016) 0.40ng/ul m

response 8728

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.51#
80.00	11.80	7.09#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

Sohil
11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:23:42 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

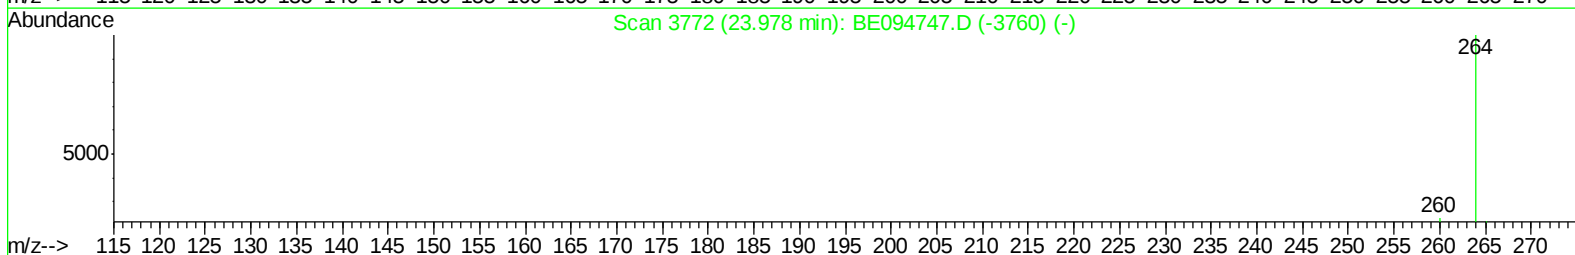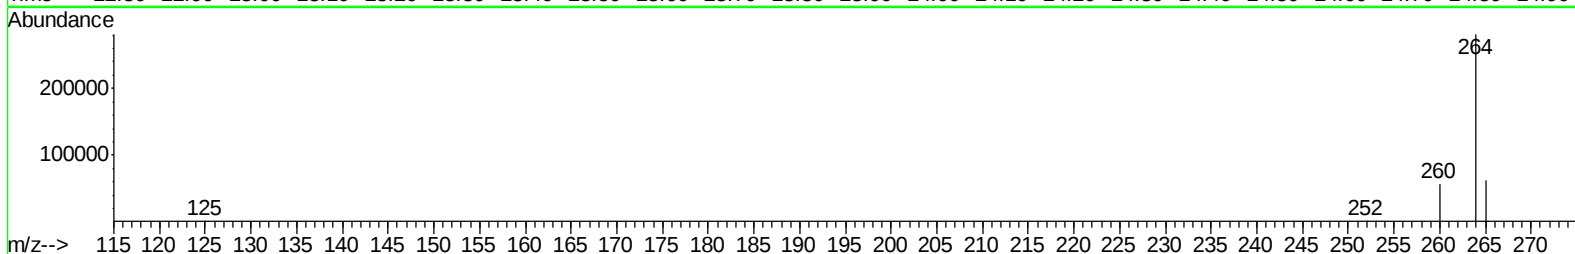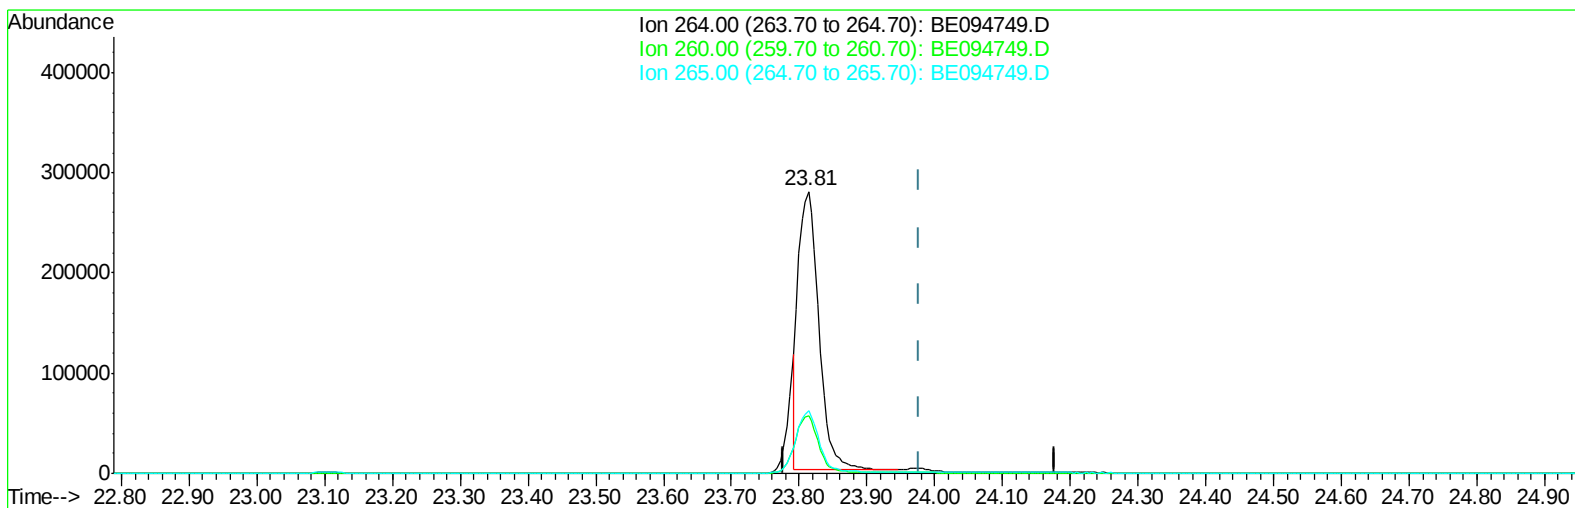

TIC: BE094749.D

(20) Perylene-d12 (I)

23.813min (-0.164) 0.40ng/ul

response 593600

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.28#
265.00	103.50	22.09#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

Sohil
11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:23:42 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

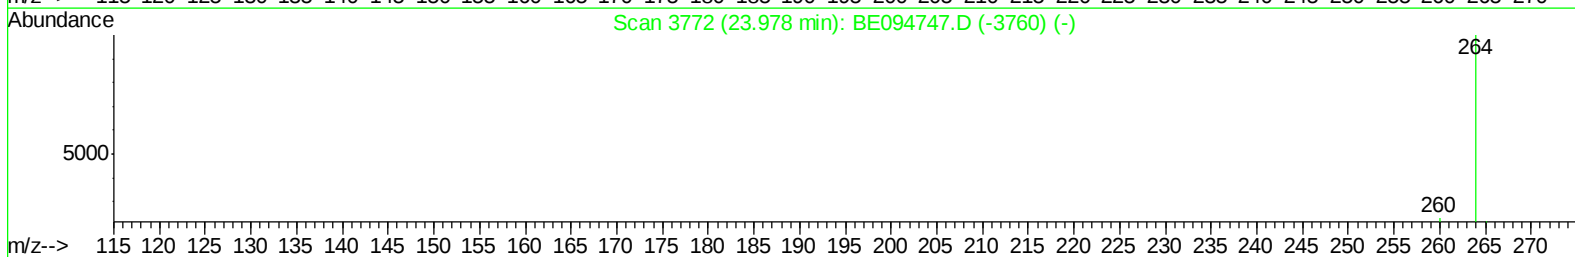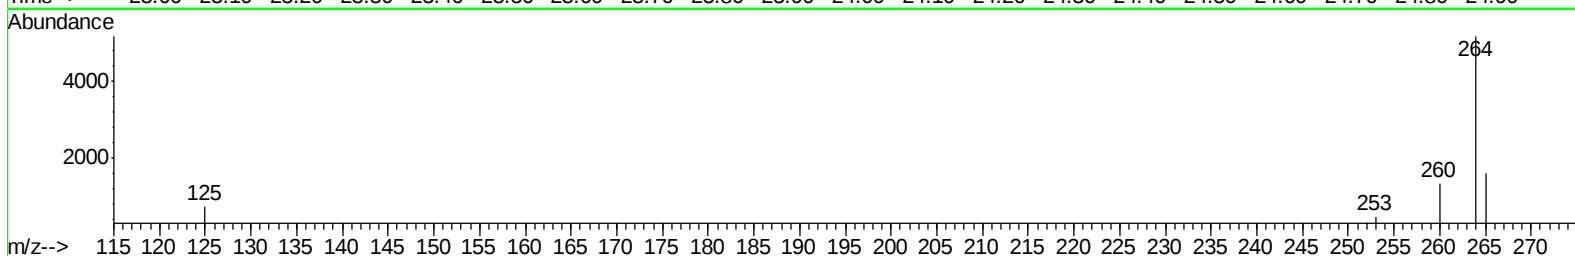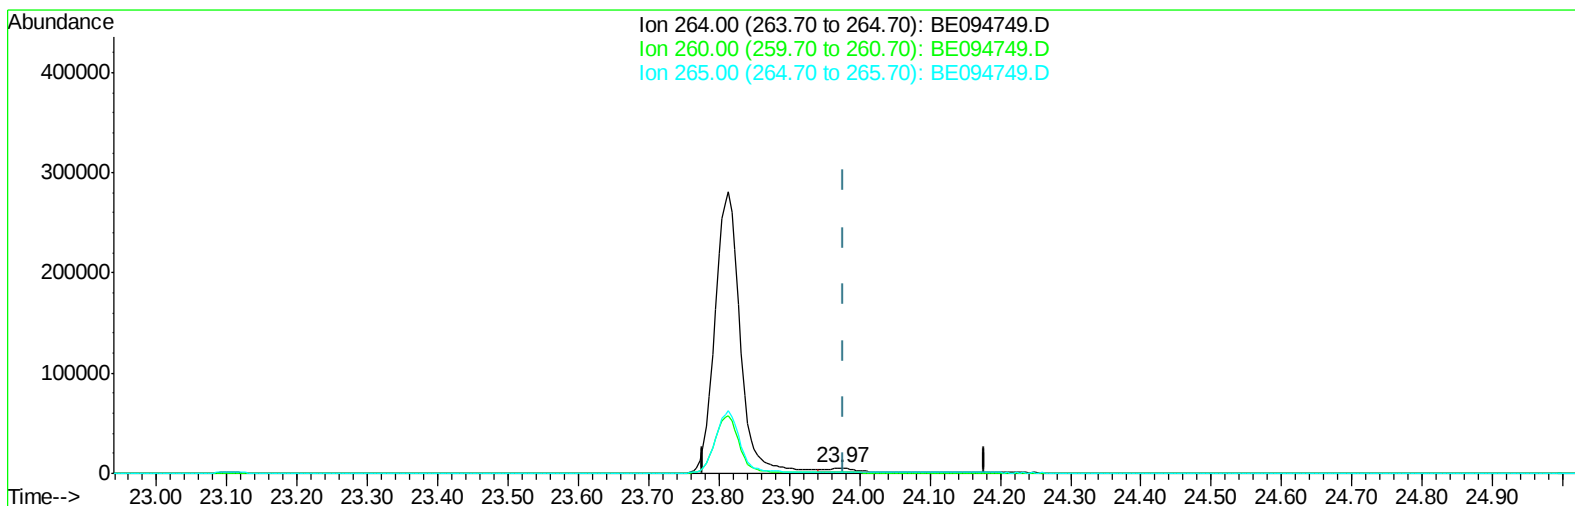

TIC: BE094749.D

(20) Perylene-d12 (I)

23.973min (-0.005) 0.40ng/ul m

response 10764

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.20
265.00	103.50	31.42#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
 Data File : BE094749.D
 Acq On : 6 Nov 2017 12:44
 Operator : SJ/JU
 Sample : PB103374BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK74

Manual Integrations
 APPROVED

Sohil
 11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:24:58 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 00:12:32 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1103	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	7036	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4108	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8728m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	8314	0.40	ng/ul	0.00
20) Perylene-d12	23.97	264	10764m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3441	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	9229	0.36	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094749.D
Acq On : 6 Nov 2017 12:44
Operator : SJ/JU
Sample : PB103374BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

Sohil
11/7/2017 5:41:23 PM

Quant Time: Nov 07 00:24:58 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

