

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101507.D
 Acq On : 6 Nov 2024 22:15
 Operator : RC/JU
 Sample : P4660-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 WC-CONCRETE-01-C

Quant Time: Nov 07 01:05:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	46975	20.000	ng	0.00
21) Naphthalene-d8	10.332	136	200241	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	139072	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	335687	20.000	ng	0.00
76) Chrysene-d12	21.066	240	438455	20.000	ng	-0.01
86) Perylene-d12	23.352	264	582677	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.314	112	467265	175.882	ng	0.00
7) Phenol-d6	6.942	99	558745	153.395	ng	0.00
23) Nitrobenzene-d5	8.769	82	374015	117.981	ng	0.00
42) 2,4,6-Tribromophenol	15.679	330	476724	182.170	ng	0.00
45) 2-Fluorobiphenyl	12.794	172	946514	111.127	ng	0.00
79) Terphenyl-d14	19.498	244	1719406	86.805	ng	0.00
Target Compounds						
31) Naphthalene	10.379	128	21474	2.124	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101507.D
Acq On : 6 Nov 2024 22:15
Operator : RC/JU
Sample : P4660-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-CONCRETE-01-C

Quant Time: Nov 07 01:05:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

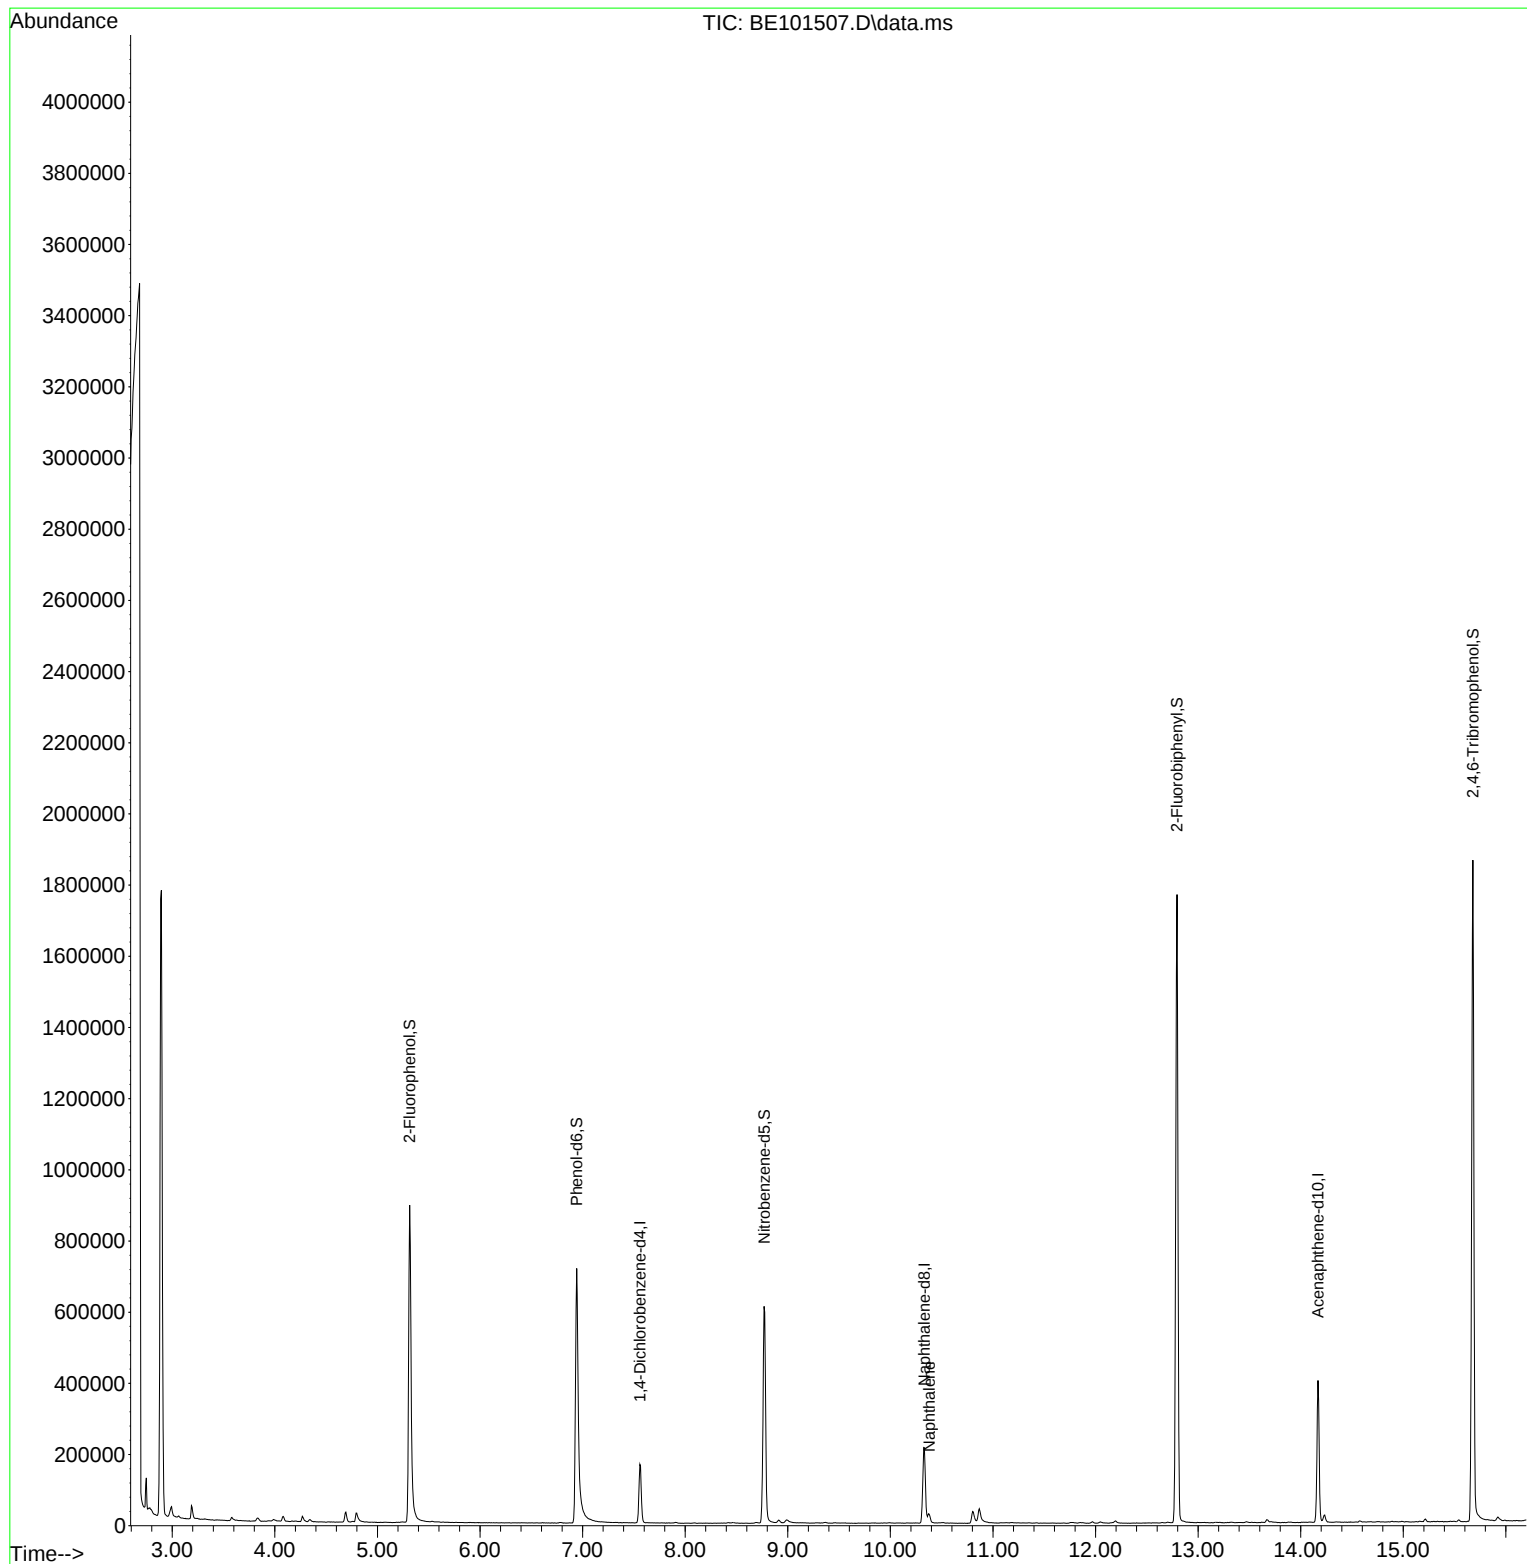

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101507.D
Acq On : 6 Nov 2024 22:15
Operator : RC/JU
Sample : P4660-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-CONCRETE-01-C

Quant Time: Nov 07 01:05:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

