

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101509.D
 Acq On : 6 Nov 2024 23:27
 Operator : RC/JU
 Sample : P4667-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F-5

Quant Time: Nov 07 01:06:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.564	152	43550	20.000	ng	0.00
21) Naphthalene-d8	10.331	136	182213	20.000	ng	0.00
39) Acenaphthene-d10	14.168	164	84237	20.000	ng	0.00
64) Phenanthrene-d10	16.906	188	273041	20.000	ng	0.00
76) Chrysene-d12	21.065	240	231938	20.000	ng	-0.01
86) Perylene-d12	23.351	264	21989	20.000	ng	# 0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.313	112	436598	177.263	ng	0.00
7) Phenol-d6	6.941	99	433493	128.368	ng	0.00
23) Nitrobenzene-d5	8.768	82	348924	120.956	ng	0.00
42) 2,4,6-Tribromophenol	15.678	330	409843	258.562	ng	0.00
45) 2-Fluorobiphenyl	12.793	172	864937	167.654	ng	0.00
79) Terphenyl-d14	19.503	244	1922421	183.471	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101509.D
Acq On : 6 Nov 2024 23:27
Operator : RC/JU
Sample : P4667-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-5

Quant Time: Nov 07 01:06:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

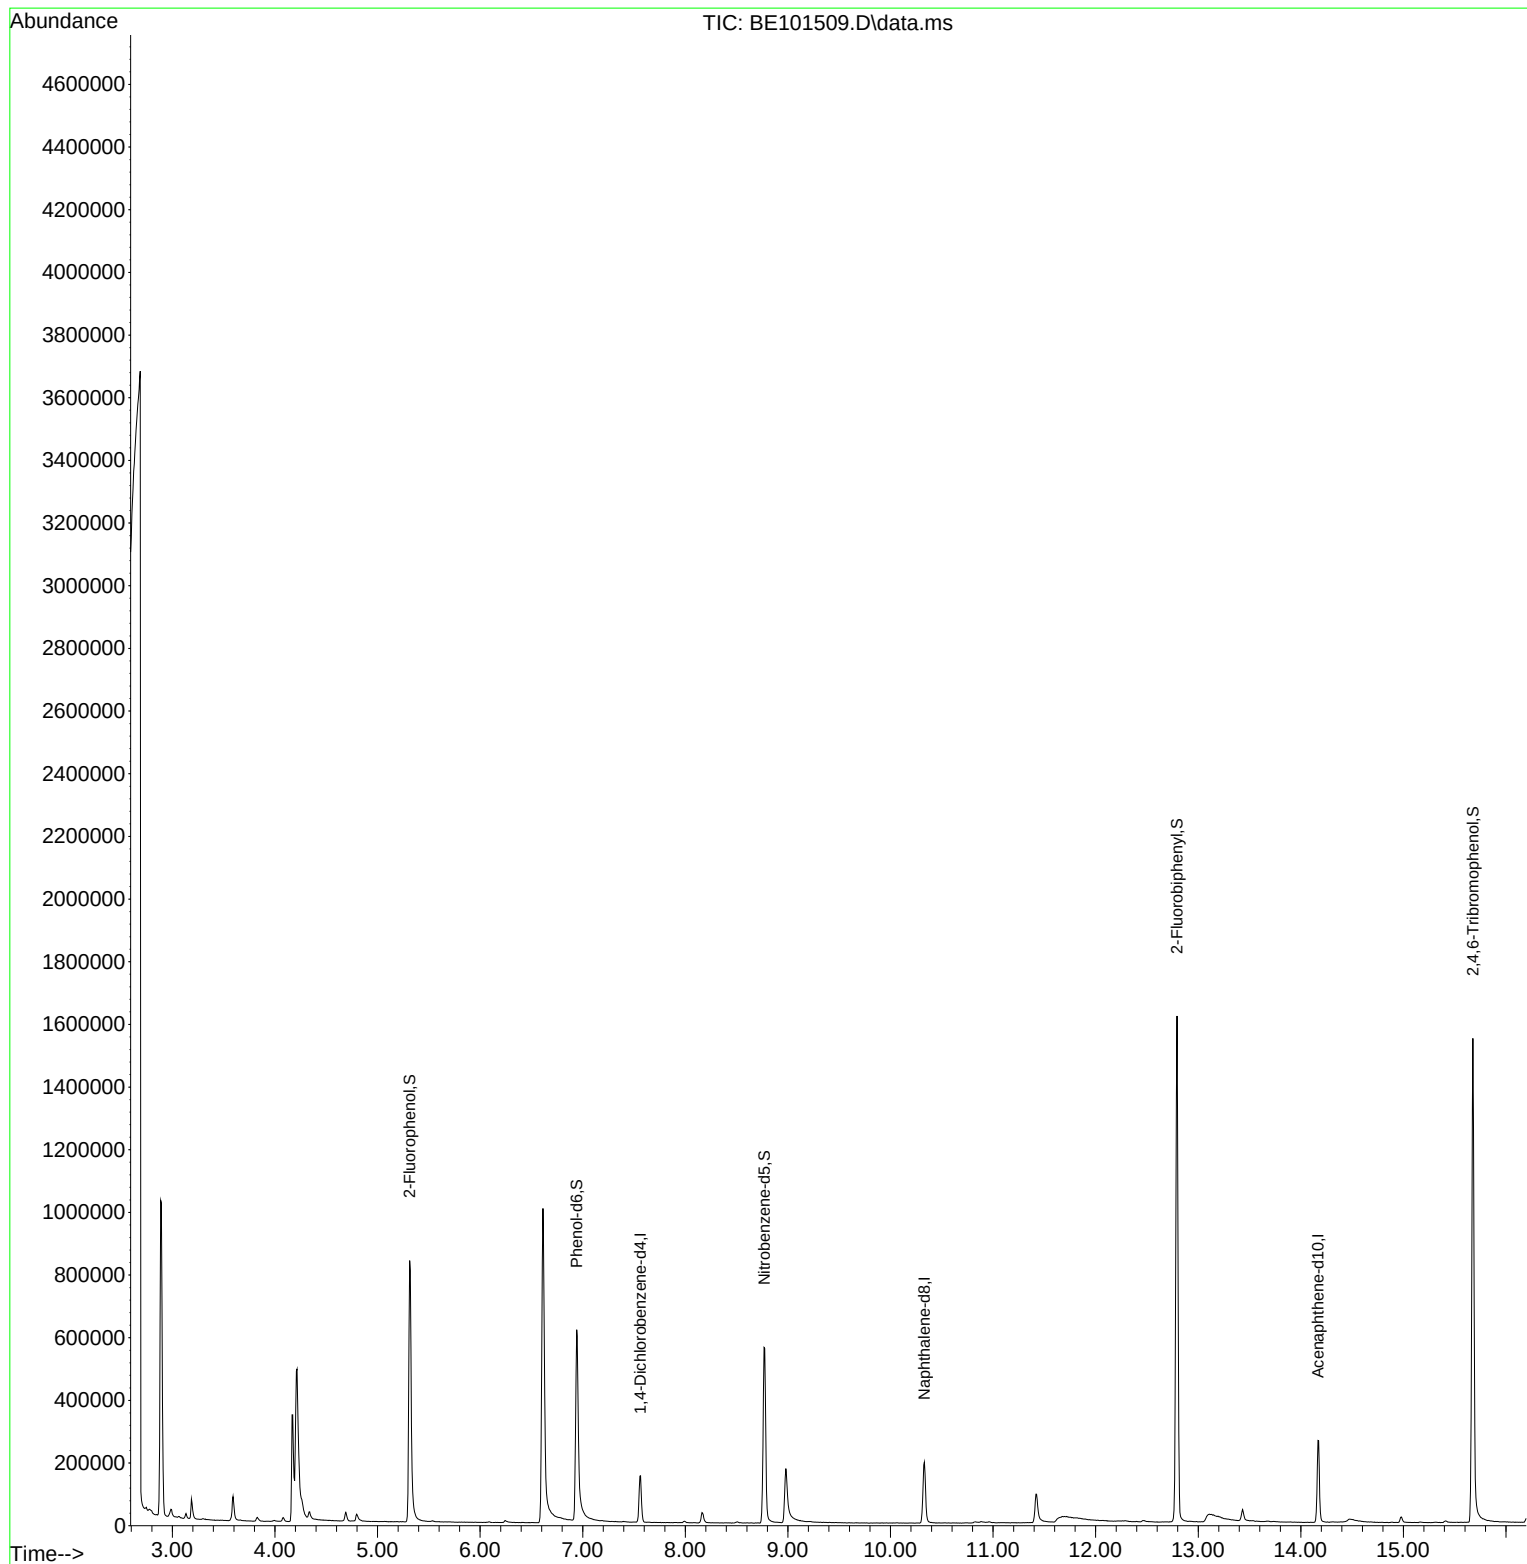

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101509.D
Acq On : 6 Nov 2024 23:27
Operator : RC/JU
Sample : P4667-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-5

Quant Time: Nov 07 01:06:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

