

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101514.D
 Acq On : 7 Nov 2024 2:26
 Operator : RC/JU
 Sample : P4680-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F26

Quant Time: Nov 07 02:20:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.557	152	40600	20.000	ng	0.00
21) Naphthalene-d8	10.324	136	164818	20.000	ng	0.00
39) Acenaphthene-d10	14.167	164	109250	20.000	ng	0.00
64) Phenanthrene-d10	16.905	188	268649	20.000	ng	0.00
76) Chrysene-d12	21.065	240	412444	20.000	ng	-0.01
86) Perylene-d12	23.350	264	561420	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.313	112	392043	170.739	ng	0.00
7) Phenol-d6	6.940	99	468128	148.697	ng	0.00
23) Nitrobenzene-d5	8.767	82	289191	110.830	ng	0.00
42) 2,4,6-Tribromophenol	15.677	330	349052	169.793	ng	0.00
45) 2-Fluorobiphenyl	12.792	172	712737	106.522	ng	0.00
79) Terphenyl-d14	19.502	244	2046205	109.819	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101514.D
Acq On : 7 Nov 2024 2:26
Operator : RC/JU
Sample : P4680-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F26

Quant Time: Nov 07 02:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

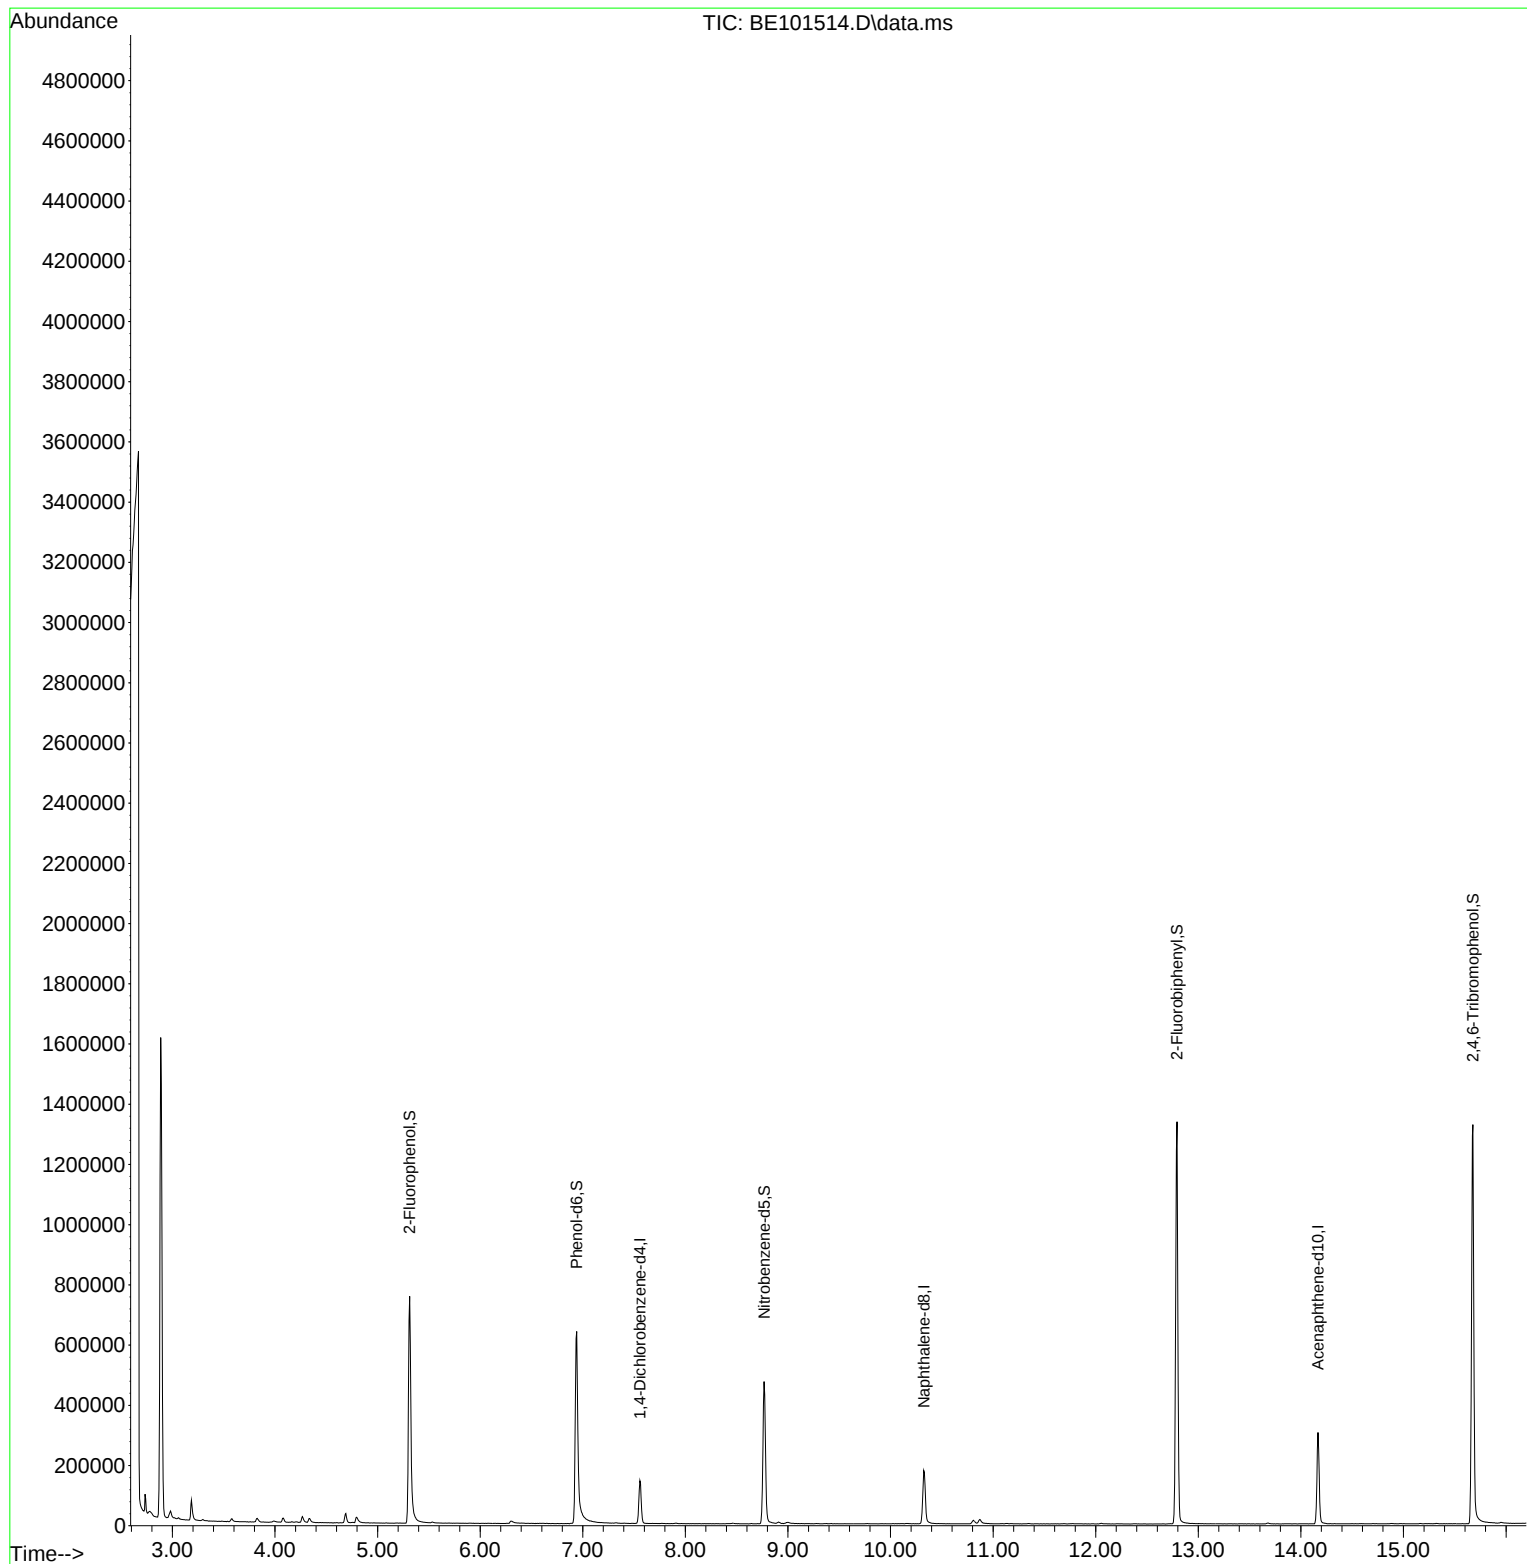

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101514.D
Acq On : 7 Nov 2024 2:26
Operator : RC/JU
Sample : P4680-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F26

Quant Time: Nov 07 02:20:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

