

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
 Data File : BE101515.D  
 Acq On : 7 Nov 2024 3:02  
 Operator : RC/JU  
 Sample : P4680-08  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 BP-F25

Quant Time: Nov 07 03:11:56 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 07 00:01:20 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.561  | 152  | 40987    | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.328 | 136  | 167334   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.171 | 164  | 110005   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 16.903 | 188  | 274287   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.063 | 240  | 392037   | 20.000  | ng    | -0.01    |
| 86) Perylene-d12            | 23.348 | 264  | 550173   | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.310  | 112  | 399613   | 172.393 | ng    | 0.00     |
| 7) Phenol-d6                | 6.938  | 99   | 465588   | 146.494 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.771  | 82   | 304136   | 114.805 | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.675 | 330  | 357025   | 172.479 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 12.790 | 172  | 770077   | 114.302 | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.500 | 244  | 1997749  | 112.799 | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
Data File : BE101515.D  
Acq On : 7 Nov 2024 3:02  
Operator : RC/JU  
Sample : P4680-08  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
BP-F25

Quant Time: Nov 07 03:11:56 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

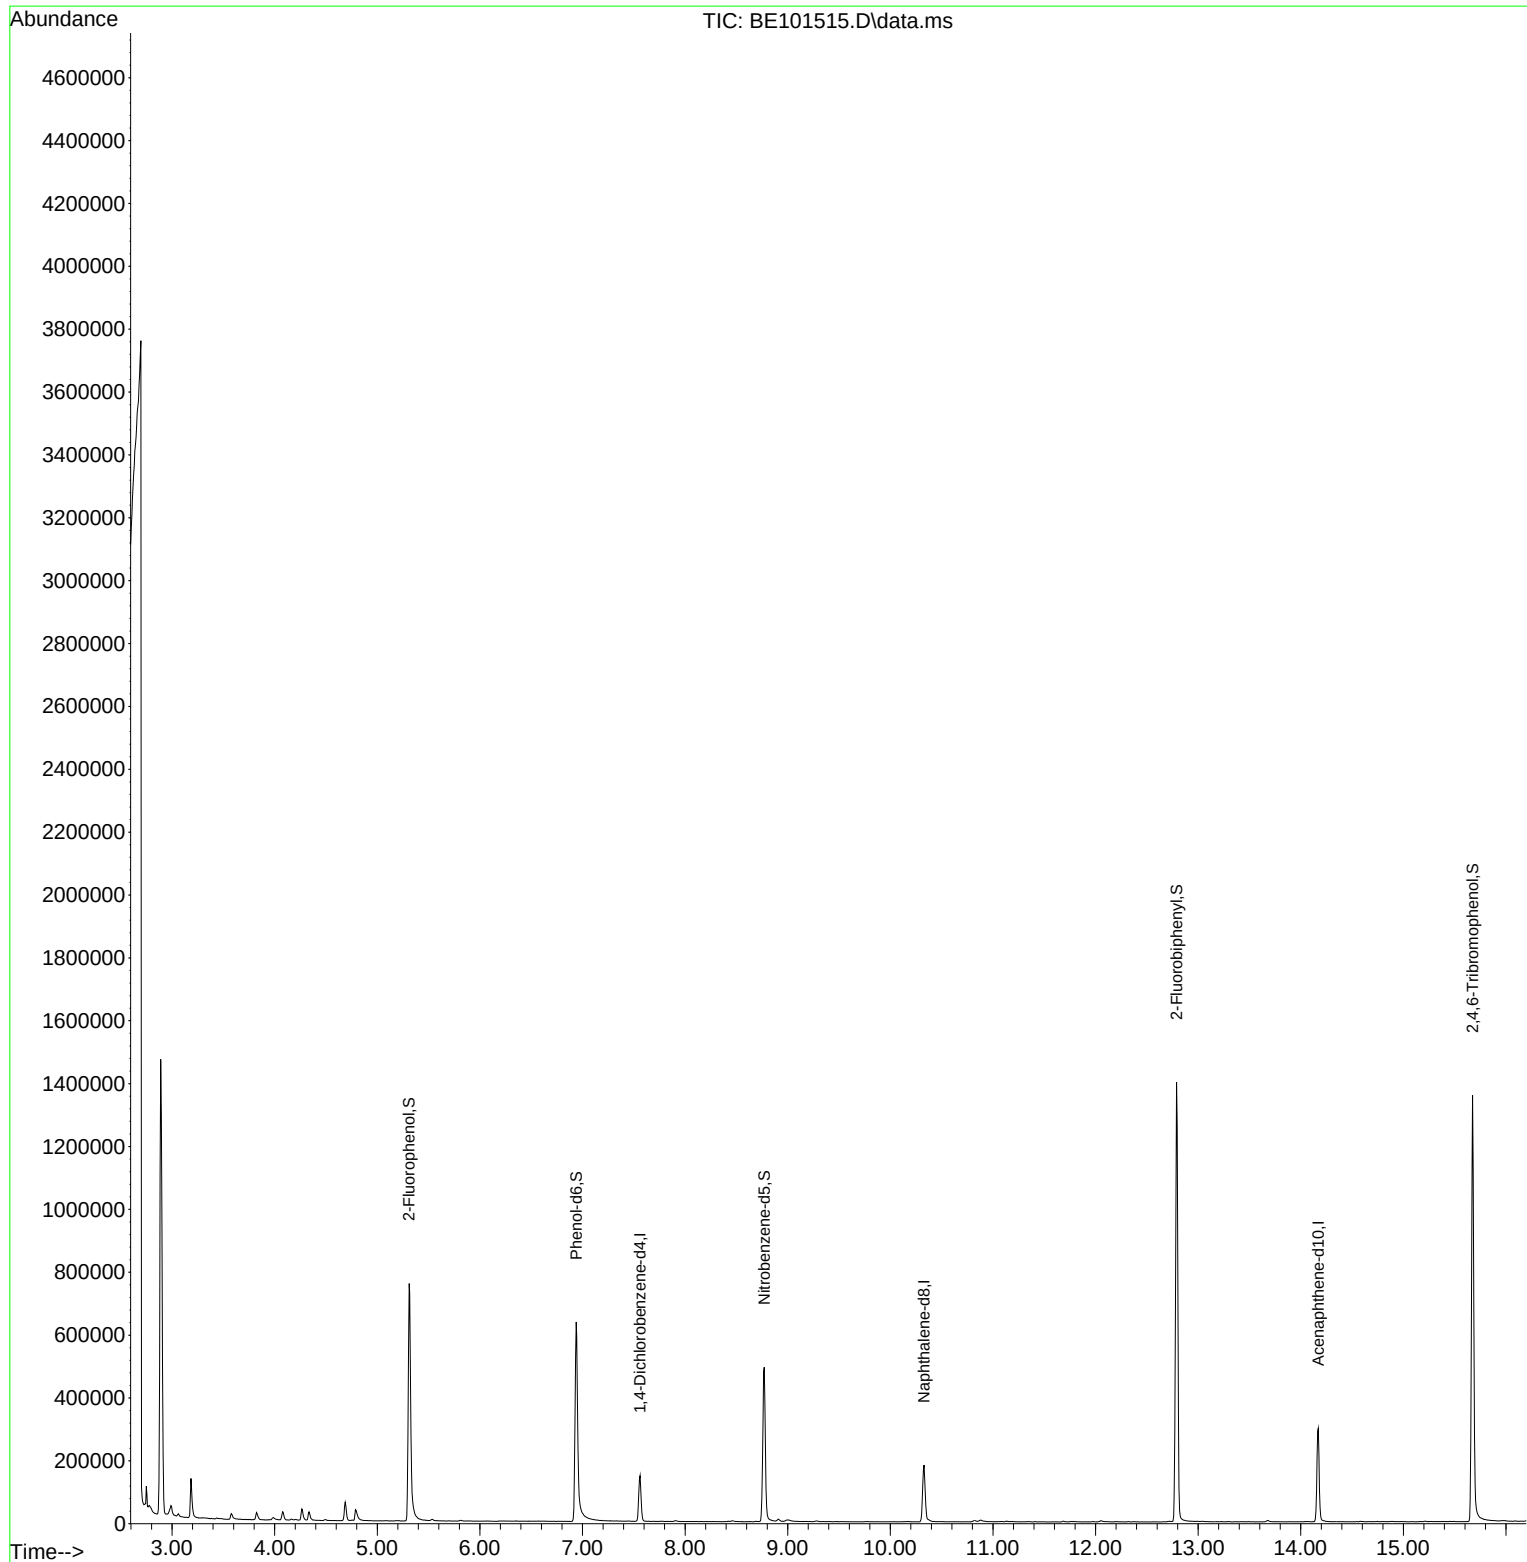

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
Data File : BE101515.D  
Acq On : 7 Nov 2024 3:02  
Operator : RC/JU  
Sample : P4680-08  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
BP-F25

Quant Time: Nov 07 03:11:56 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

