

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
 Data File : BE101518.D  
 Acq On : 7 Nov 2024 4:49  
 Operator : RC/JU  
 Sample : P4711-10  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 CF-613-COMP-17

Quant Time: Nov 07 04:41:54 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 07 00:01:20 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.561  | 152  | 41263    | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.328 | 136  | 167847   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.165 | 164  | 106709   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 16.903 | 188  | 273838   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.063 | 240  | 410570   | 20.000  | ng    | -0.01    |
| 86) Perylene-d12            | 23.348 | 264  | 266141   | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.311  | 112  | 347926   | 149.091 | ng    | 0.00     |
| 7) Phenol-d6                | 6.938  | 99   | 396341   | 123.872 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.765  | 82   | 281252   | 105.842 | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.675 | 330  | 327499   | 163.102 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 12.790 | 172  | 709156   | 108.511 | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.500 | 244  | 2027215  | 109.296 | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
Data File : BE101518.D  
Acq On : 7 Nov 2024 4:49  
Operator : RC/JU  
Sample : P4711-10  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
CF-613-COMP-17

Quant Time: Nov 07 04:41:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

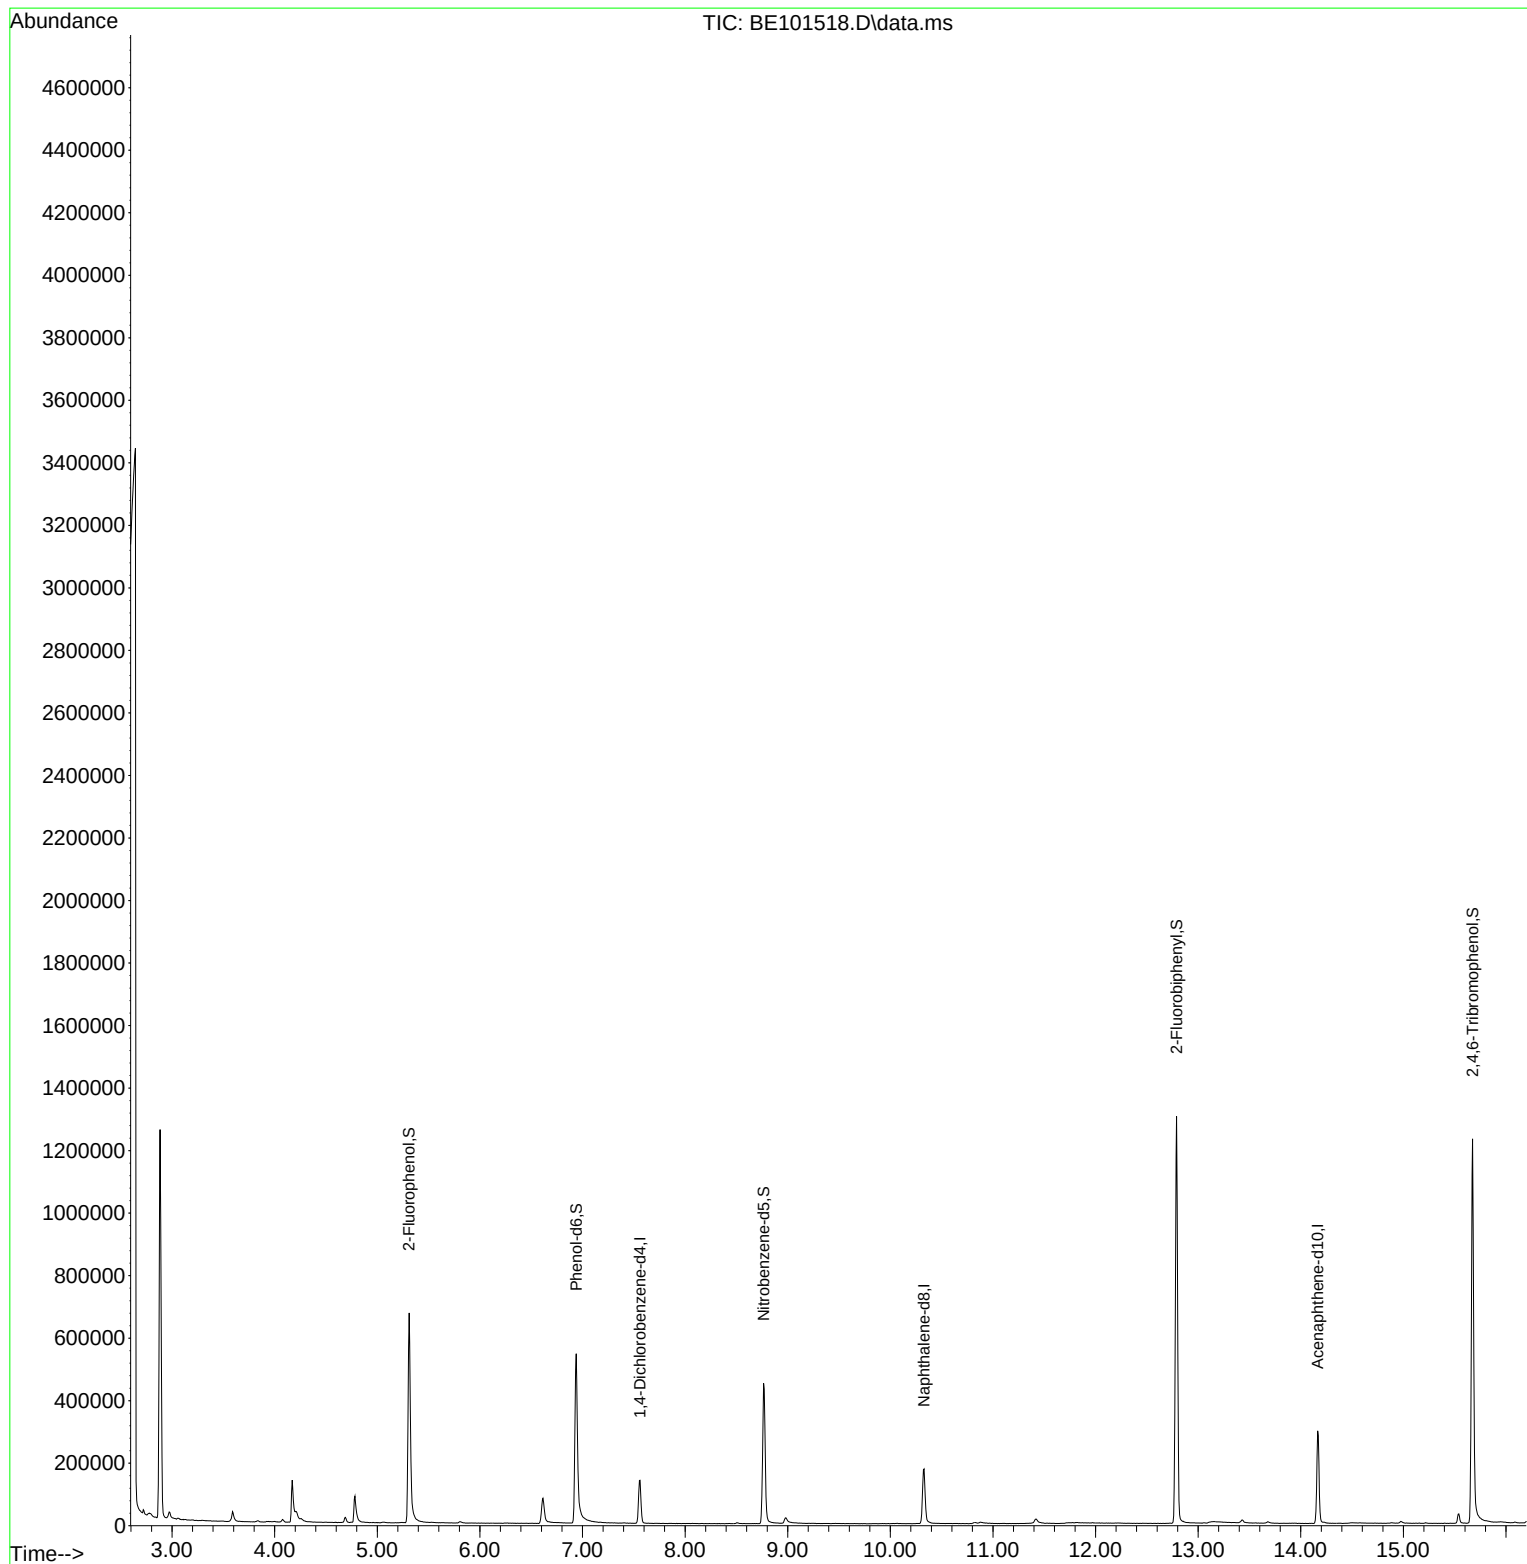

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110624\  
Data File : BE101518.D  
Acq On : 7 Nov 2024 4:49  
Operator : RC/JU  
Sample : P4711-10  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
CF-613-COMP-17

Quant Time: Nov 07 04:41:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

