
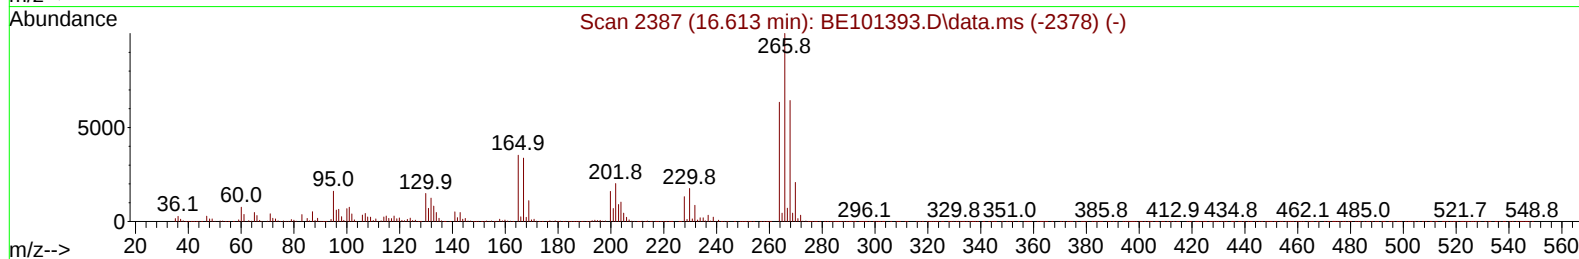
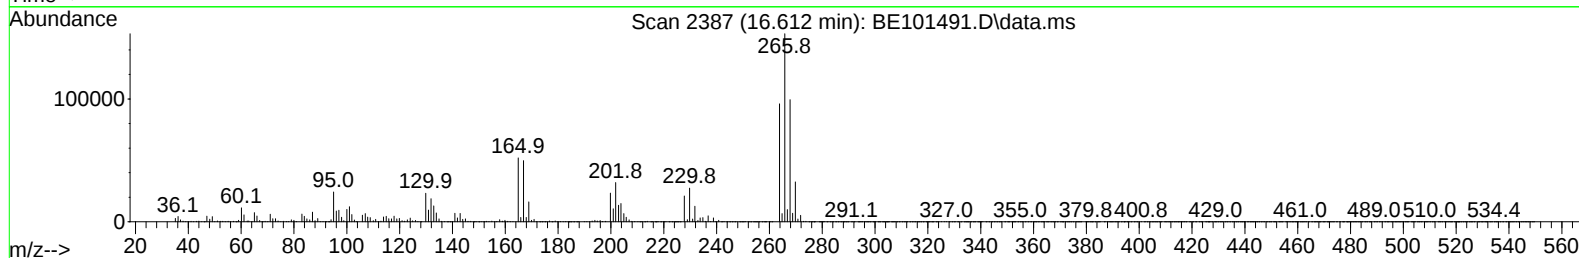


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101491.D
Acq On : 6 Nov 2024 11:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 14:00:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

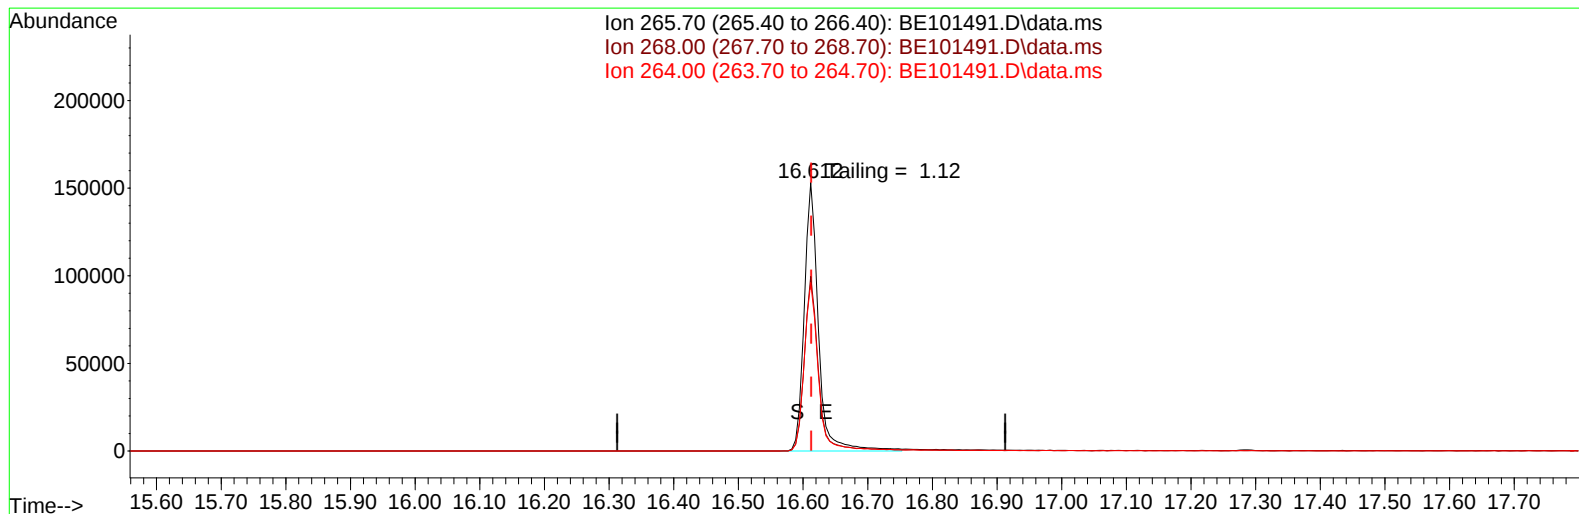

TIC: BE101491.D\data.ms

(70) Pentachlorophenol (C)




16.612min (-0.001) 879438.33 ng

response 237313

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.98
264.00	63.40	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101491.D
Acq On : 6 Nov 2024 11:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 14:00:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

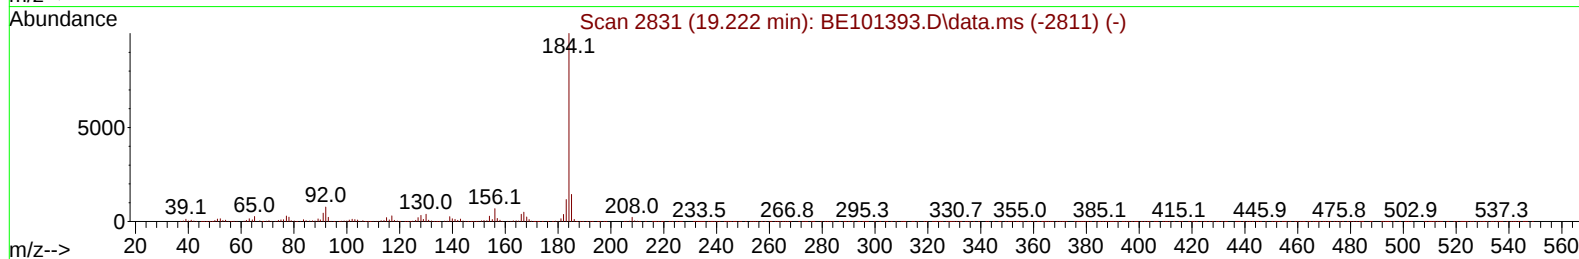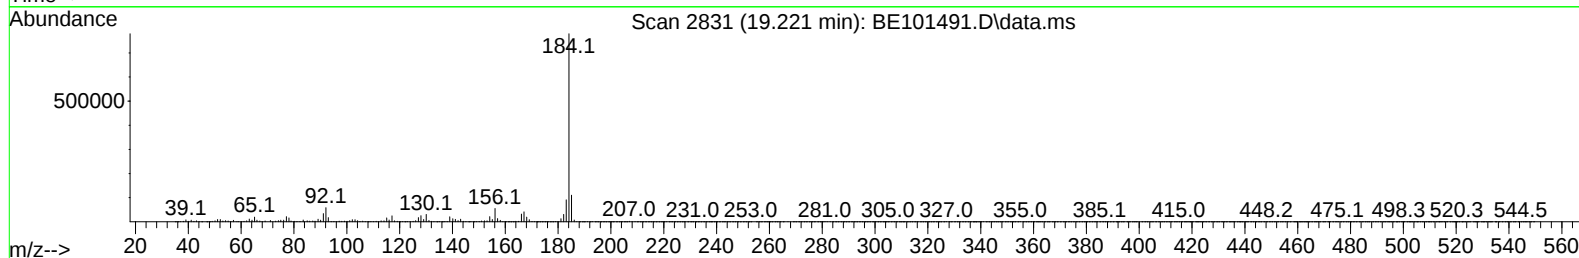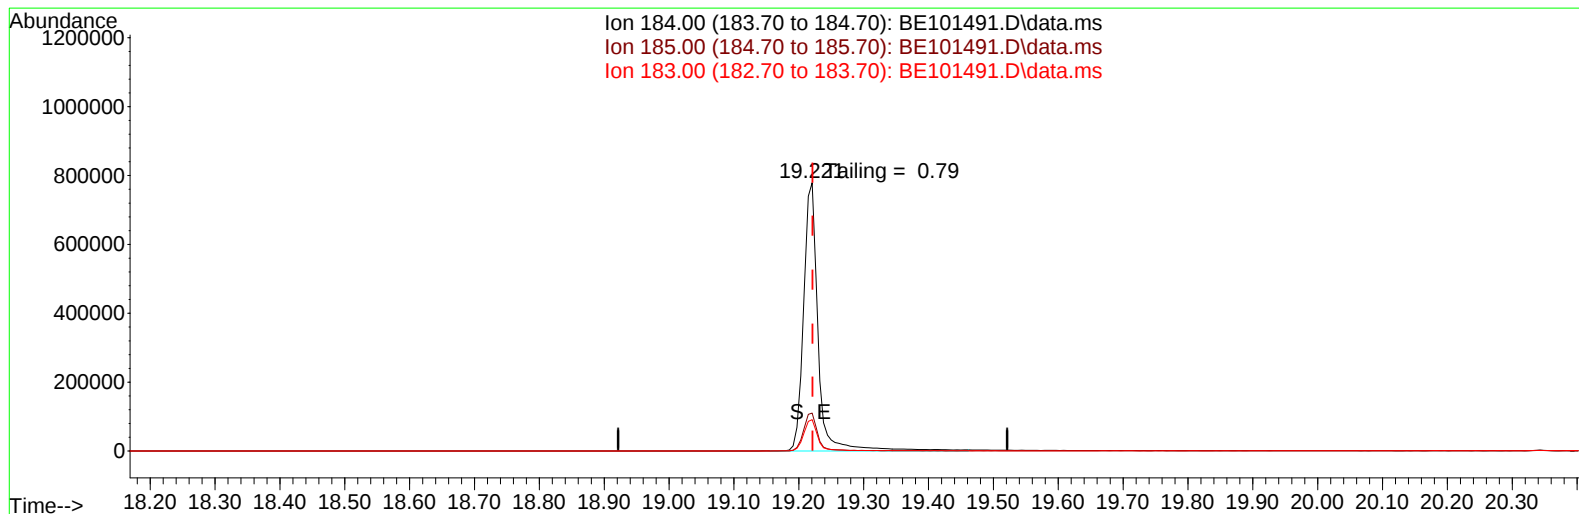

TIC: BE101491.D\data.ms

(77) Benzidine**19.221min (-0.001) 515869.86 ng****response 1191601**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.60	11.67
0.00	0.00	0.00