
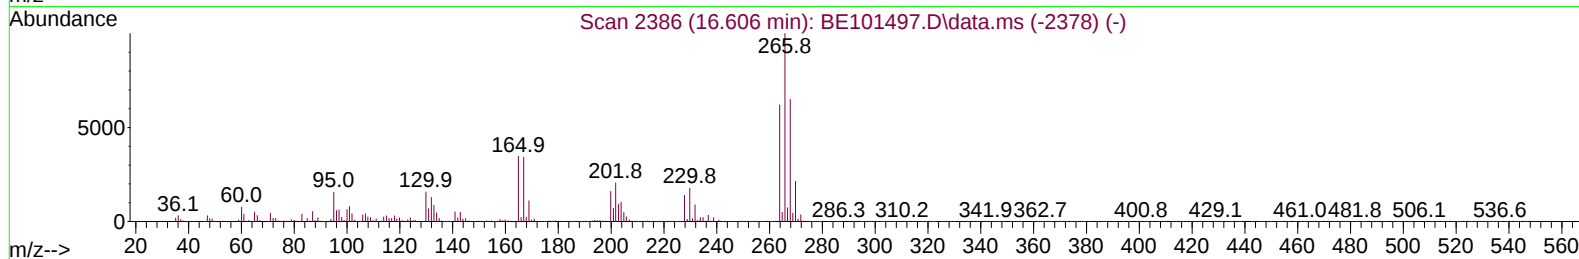
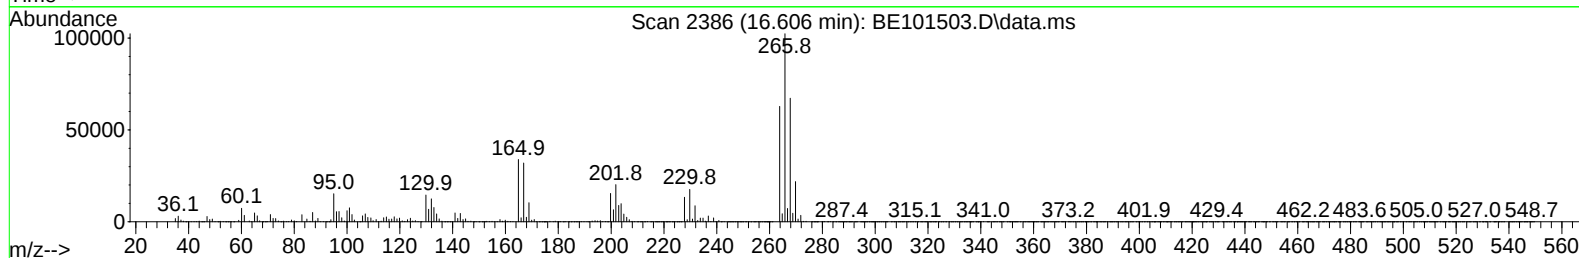


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101503.D
Acq On : 6 Nov 2024 19:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 00:16:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

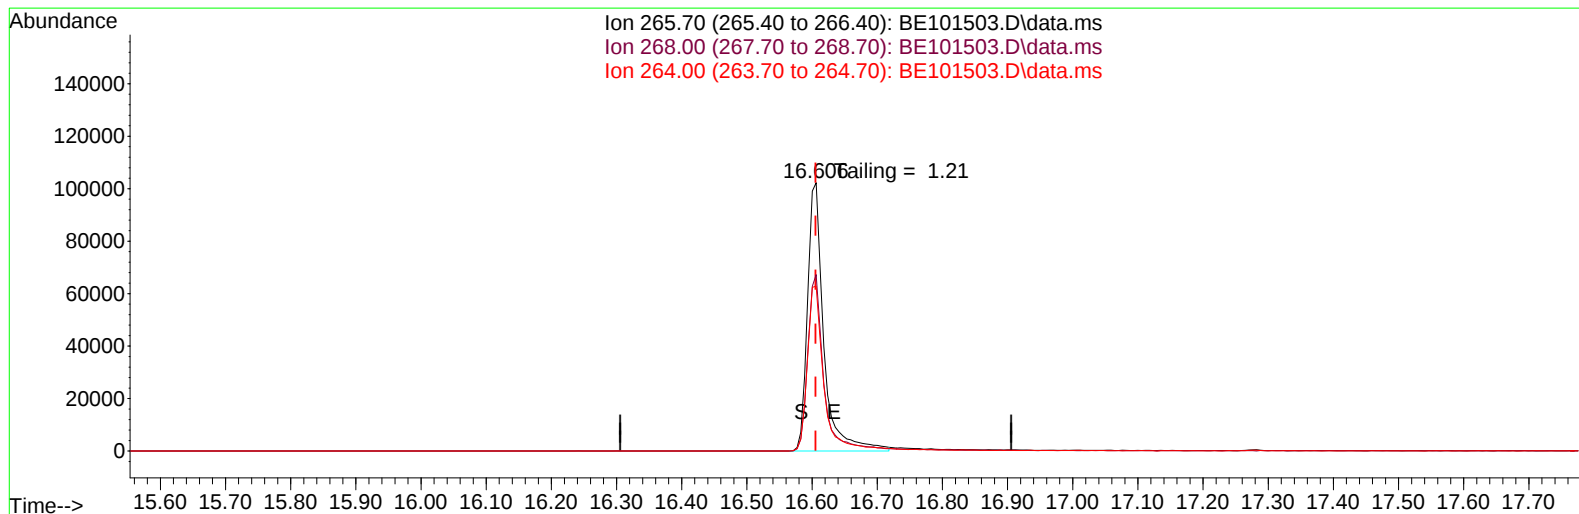

TIC: BE101503.D\data.ms

(70) Pentachlorophenol (C)




16.606min (+ 0.001) 489518.90 ng

response 181203

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	65.72
264.00	62.00	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101503.D
Acq On : 6 Nov 2024 19:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 00:16:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

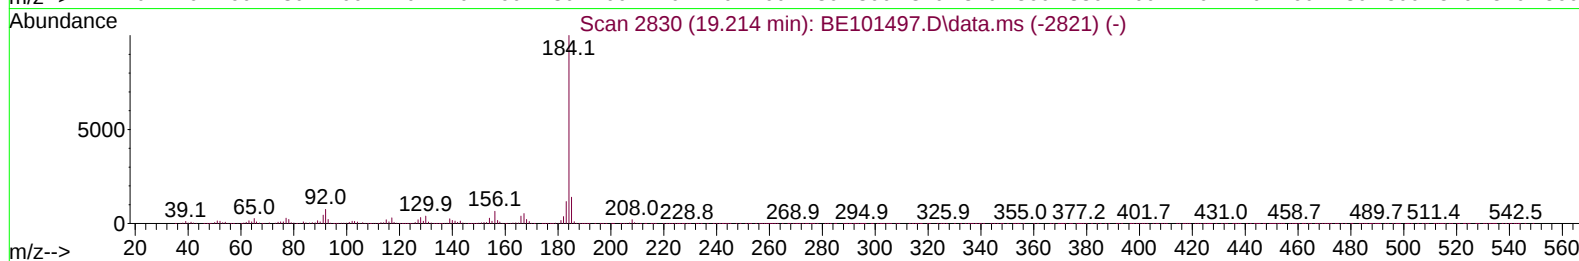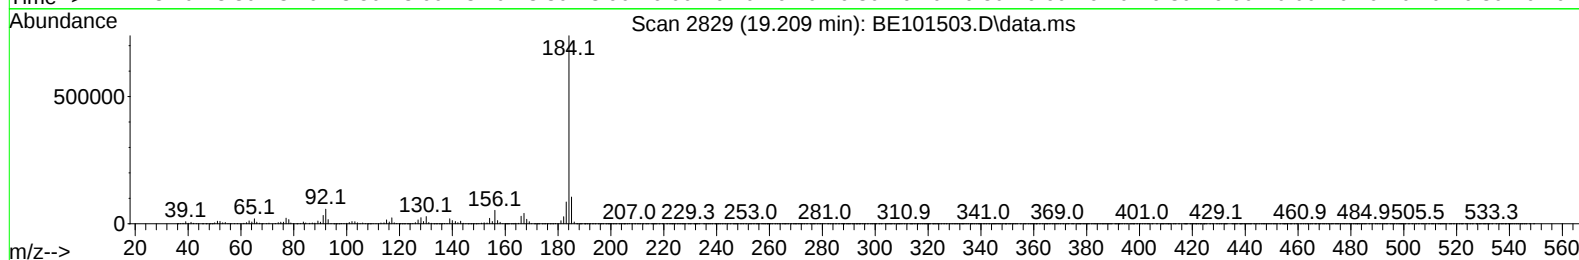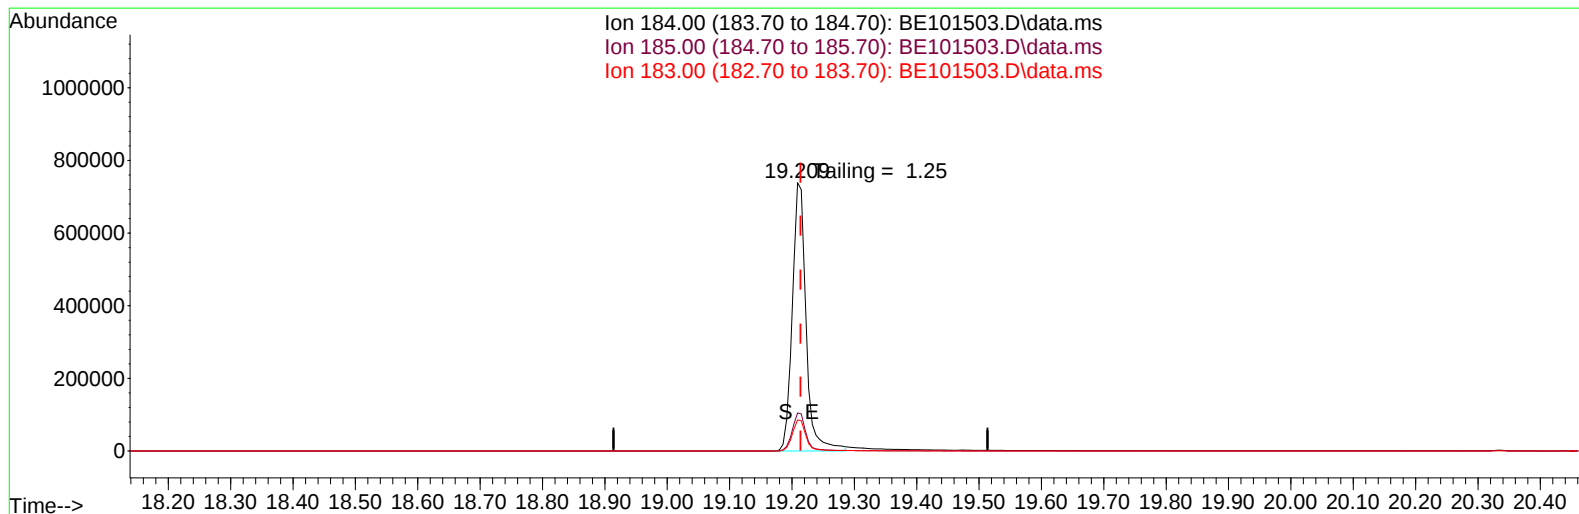

TIC: BE101503.D\data.ms

(77) Benzidine

19.209min (-0.005) 546347.88 ng

response **1185344**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	14.21
--------	-------	-------

183.00	11.70	11.60
--------	-------	-------

0.00 0.00 0.00