

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101528.D
 Acq On : 7 Nov 2024 13:20
 Operator : RC/JU
 Sample : P4667-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F-5RE

Quant Time: Nov 07 13:05:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.565	152	61537	20.000	ng	0.00
21) Naphthalene-d8	10.326	136	259466	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	94006	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	326983	20.000	ng	0.00
76) Chrysene-d12	21.067	240	253445	20.000	ng	-0.01
86) Perylene-d12	23.352	264	44227	20.000	ng	# 0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.320	112	606659	174.315	ng	0.00
7) Phenol-d6	6.948	99	538066	112.762	ng	0.00
23) Nitrobenzene-d5	8.775	82	490377	119.378	ng	0.00
42) 2,4,6-Tribromophenol	15.685	330	527078	297.968	ng	0.00
45) 2-Fluorobiphenyl	12.794	172	1116086	193.854	ng	0.00
79) Terphenyl-d14	19.504	244	2111687	184.433	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101528.D
Acq On : 7 Nov 2024 13:20
Operator : RC/JU
Sample : P4667-08RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-5RE

Quant Time: Nov 07 13:05:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

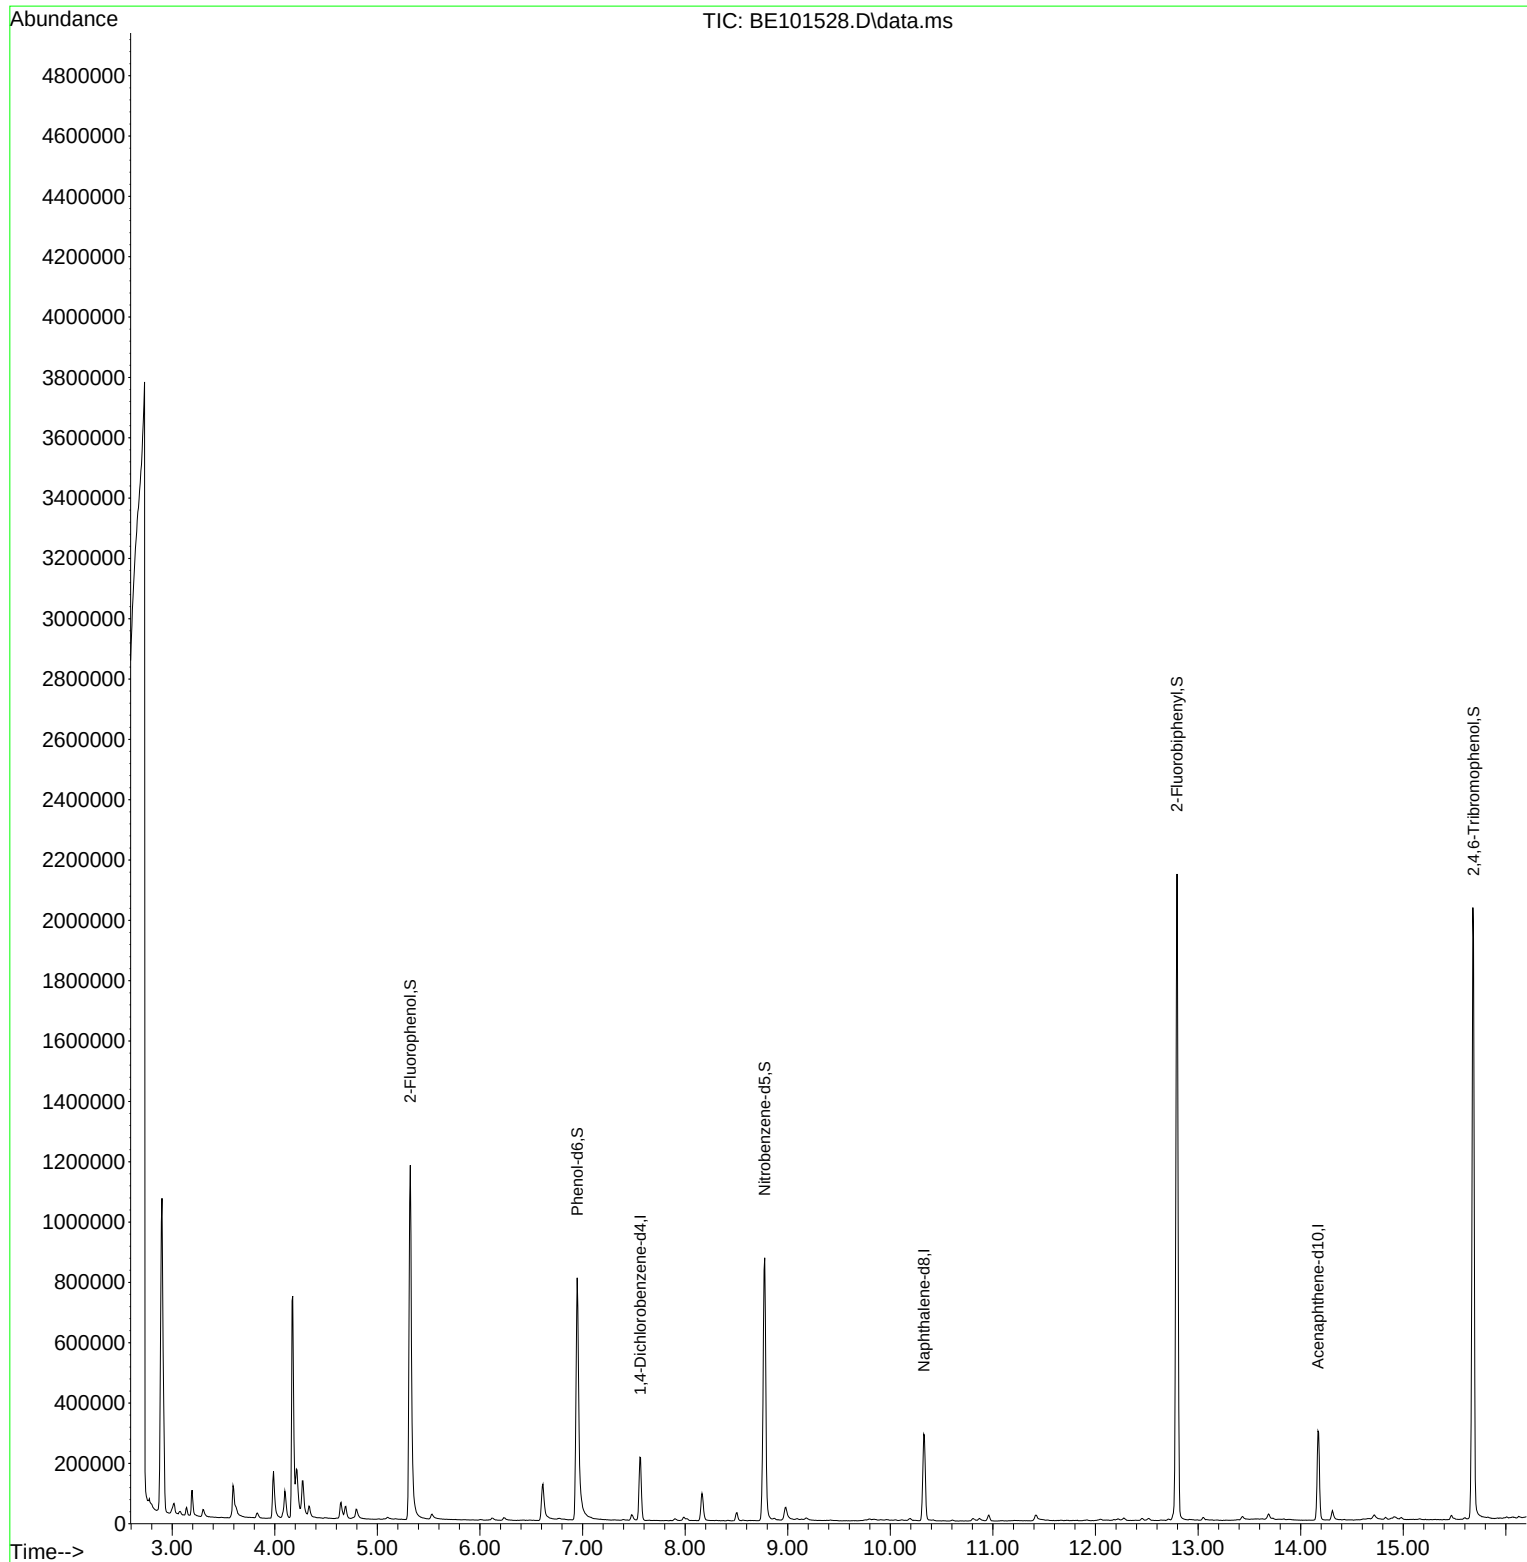

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101528.D
Acq On : 7 Nov 2024 13:20
Operator : RC/JU
Sample : P4667-08RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-5RE

Quant Time: Nov 07 13:05:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

