

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101529.D
Acq On : 7 Nov 2024 13:55
Operator : RC/JU
Sample : P4667-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10

Quant Time: Nov 07 13:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	51607	20.000	ng	0.00
21) Naphthalene-d8	10.332	136	226530	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	141806	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	328797	20.000	ng	0.00
76) Chrysene-d12	21.067	240	376478	20.000	ng	-0.01
86) Perylene-d12	23.358	264	358570	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.320	112	558163	191.240	ng	0.00
7) Phenol-d6	6.948	99	673828	168.385	ng	0.00
23) Nitrobenzene-d5	8.775	82	423797	118.170	ng	0.00
42) 2,4,6-Tribromophenol	15.685	330	476080	178.417	ng	0.00
45) 2-Fluorobiphenyl	12.794	172	986190	113.553	ng	0.00
79) Terphenyl-d14	19.504	244	2159748	126.986	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101529.D
Acq On : 7 Nov 2024 13:55
Operator : RC/JU
Sample : P4667-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10

Quant Time: Nov 07 13:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

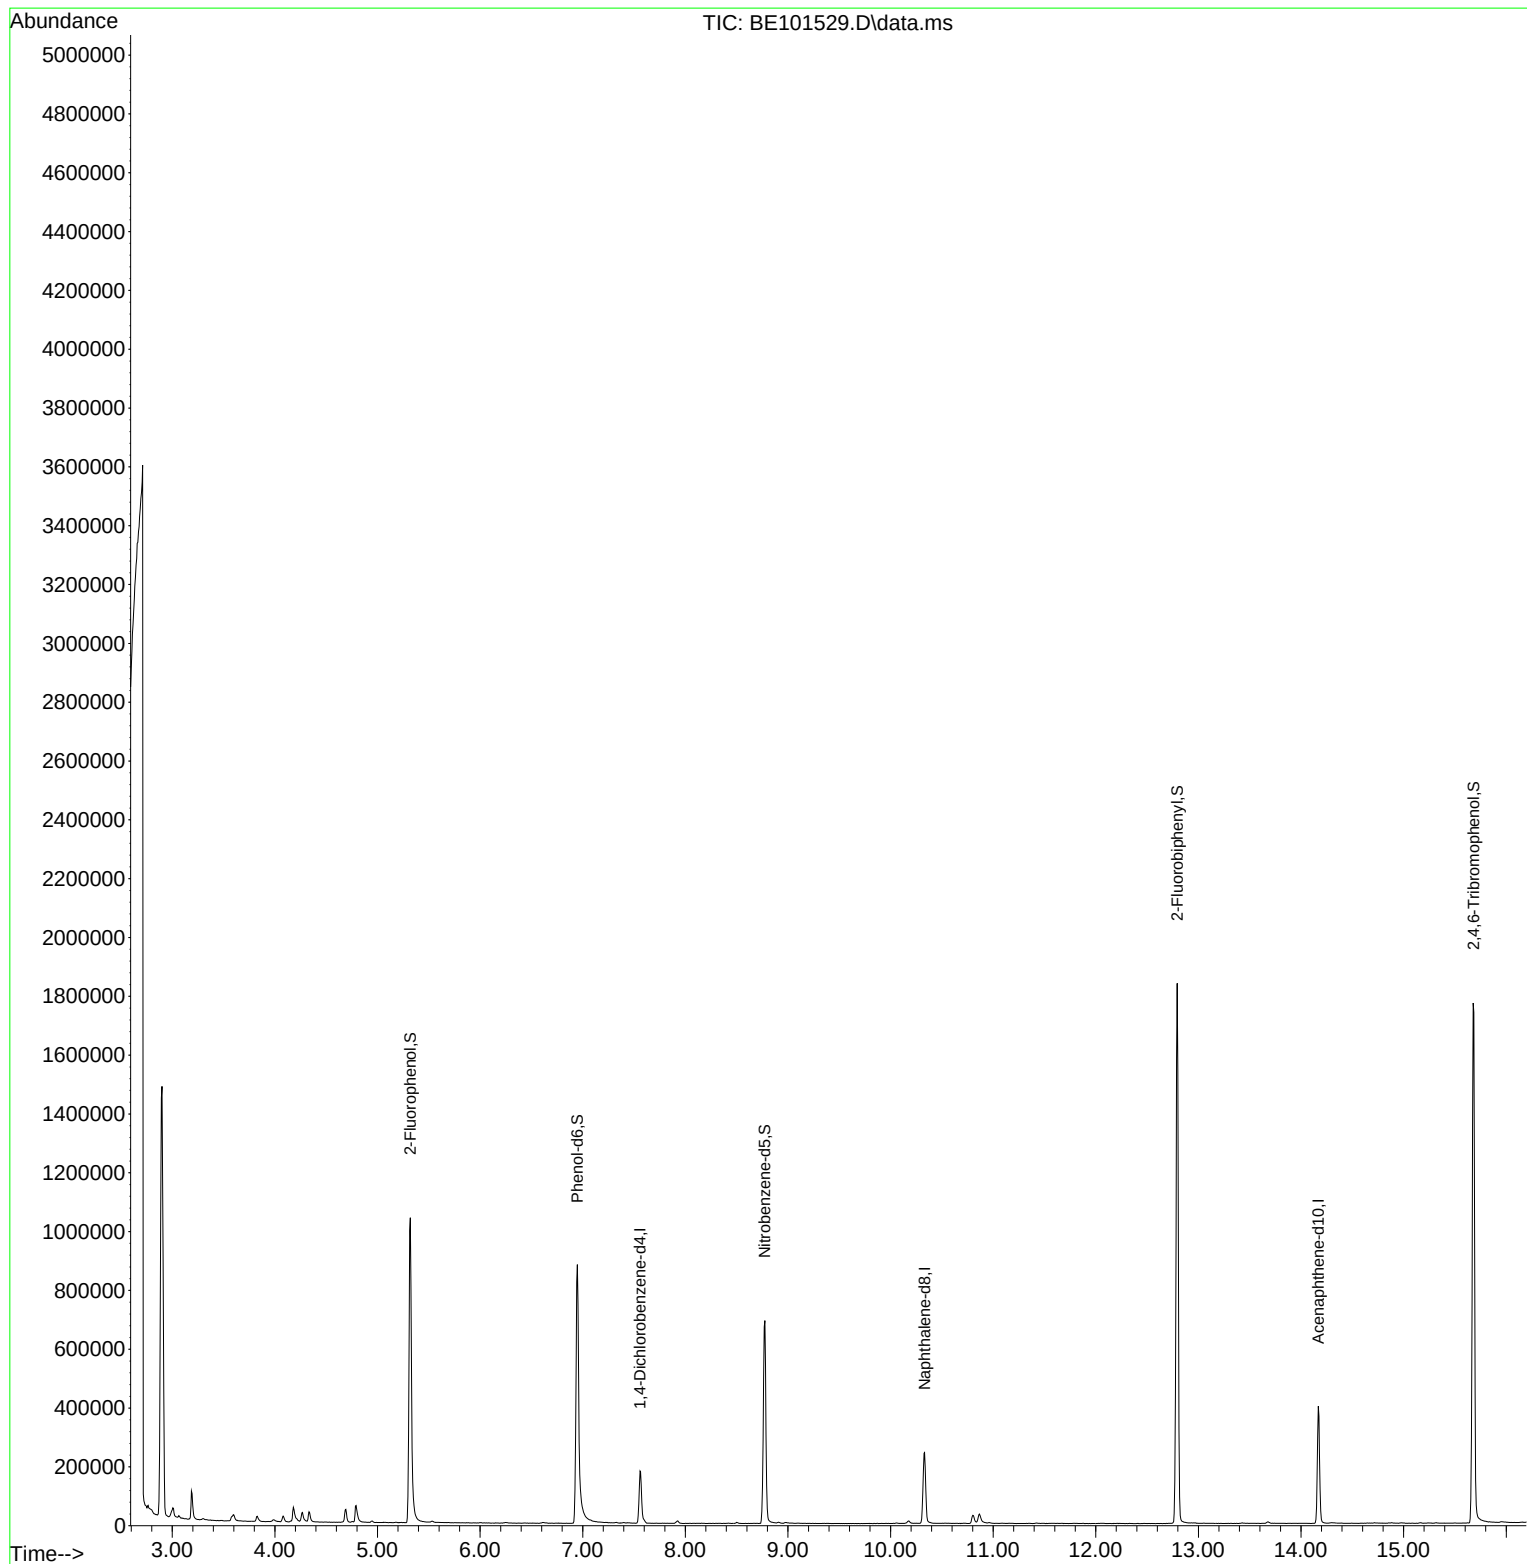

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101529.D
Acq On : 7 Nov 2024 13:55
Operator : RC/JU
Sample : P4667-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10

Quant Time: Nov 07 13:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

