

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101531.D
 Acq On : 7 Nov 2024 15:07
 Operator : RC/JU
 Sample : P4711-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CF-613-COMP-16

Quant Time: Nov 07 14:56:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.561	152	52408	20.000	ng	0.00
21) Naphthalene-d8	10.329	136	218608	20.000	ng	0.00
39) Acenaphthene-d10	14.171	164	139169	20.000	ng	0.00
64) Phenanthrene-d10	16.909	188	325704	20.000	ng	0.00
76) Chrysene-d12	21.069	240	415690	20.000	ng	0.00
86) Perylene-d12	23.355	264	542611	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.317	112	477618	161.142	ng	0.00
7) Phenol-d6	6.945	99	556609	136.967	ng	0.00
23) Nitrobenzene-d5	8.772	82	395260	114.207	ng	0.00
42) 2,4,6-Tribromophenol	15.681	330	457024	174.521	ng	0.00
45) 2-Fluorobiphenyl	12.796	172	988136	115.933	ng	0.00
79) Terphenyl-d14	19.500	244	2228197	118.652	ng	0.00
Target Compounds						
77) Benzdine	19.212	184	27913	3.126	ng	Qvalue # 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101531.D
Acq On : 7 Nov 2024 15:07
Operator : RC/JU
Sample : P4711-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CF-613-COMP-16

Quant Time: Nov 07 14:56:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

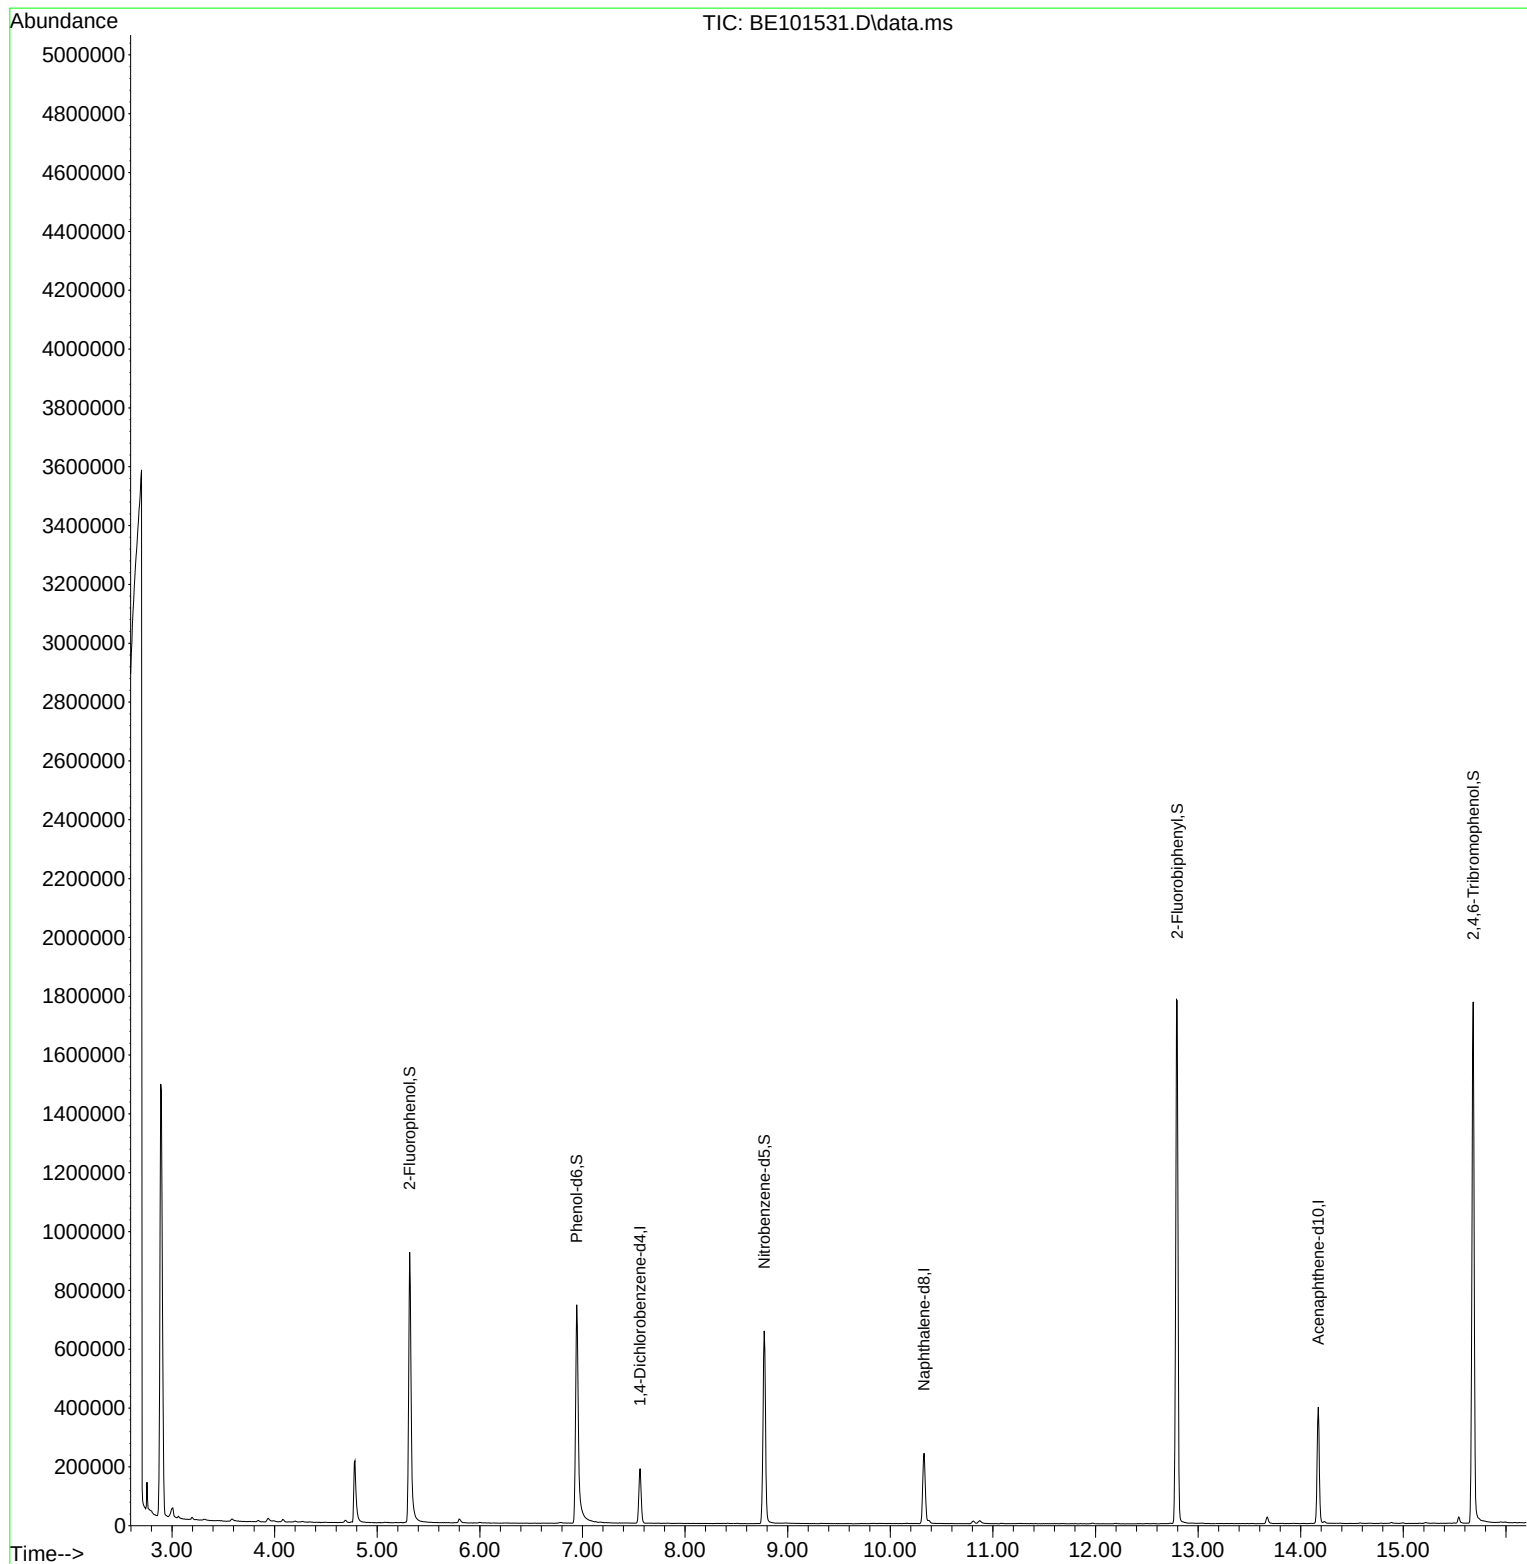

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101531.D
Acq On : 7 Nov 2024 15:07
Operator : RC/JU
Sample : P4711-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CF-613-COMP-16

Quant Time: Nov 07 14:56:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

