

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101533.D
 Acq On : 7 Nov 2024 16:19
 Operator : RC/JU
 Sample : P4680-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F26

Quant Time: Nov 07 16:55:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	49424	20.000	ng	0.00
21) Naphthalene-d8	10.325	136	209567	20.000	ng	0.00
39) Acenaphthene-d10	14.168	164	136302	20.000	ng	0.00
64) Phenanthrene-d10	16.906	188	319261	20.000	ng	0.00
76) Chrysene-d12	21.066	240	395210	20.000	ng	-0.01
86) Perylene-d12	23.351	264	526168	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.314	112	475423	170.086	ng	0.00
7) Phenol-d6	6.941	99	581368	151.697	ng	0.00
23) Nitrobenzene-d5	8.774	82	364388	109.829	ng	0.00
42) 2,4,6-Tribromophenol	15.678	330	426167	166.161	ng	0.00
45) 2-Fluorobiphenyl	12.793	172	880146	105.435	ng	0.00
79) Terphenyl-d14	19.503	244	2036010	114.036	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101533.D
Acq On : 7 Nov 2024 16:19
Operator : RC/JU
Sample : P4680-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F26

Quant Time: Nov 07 16:55:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

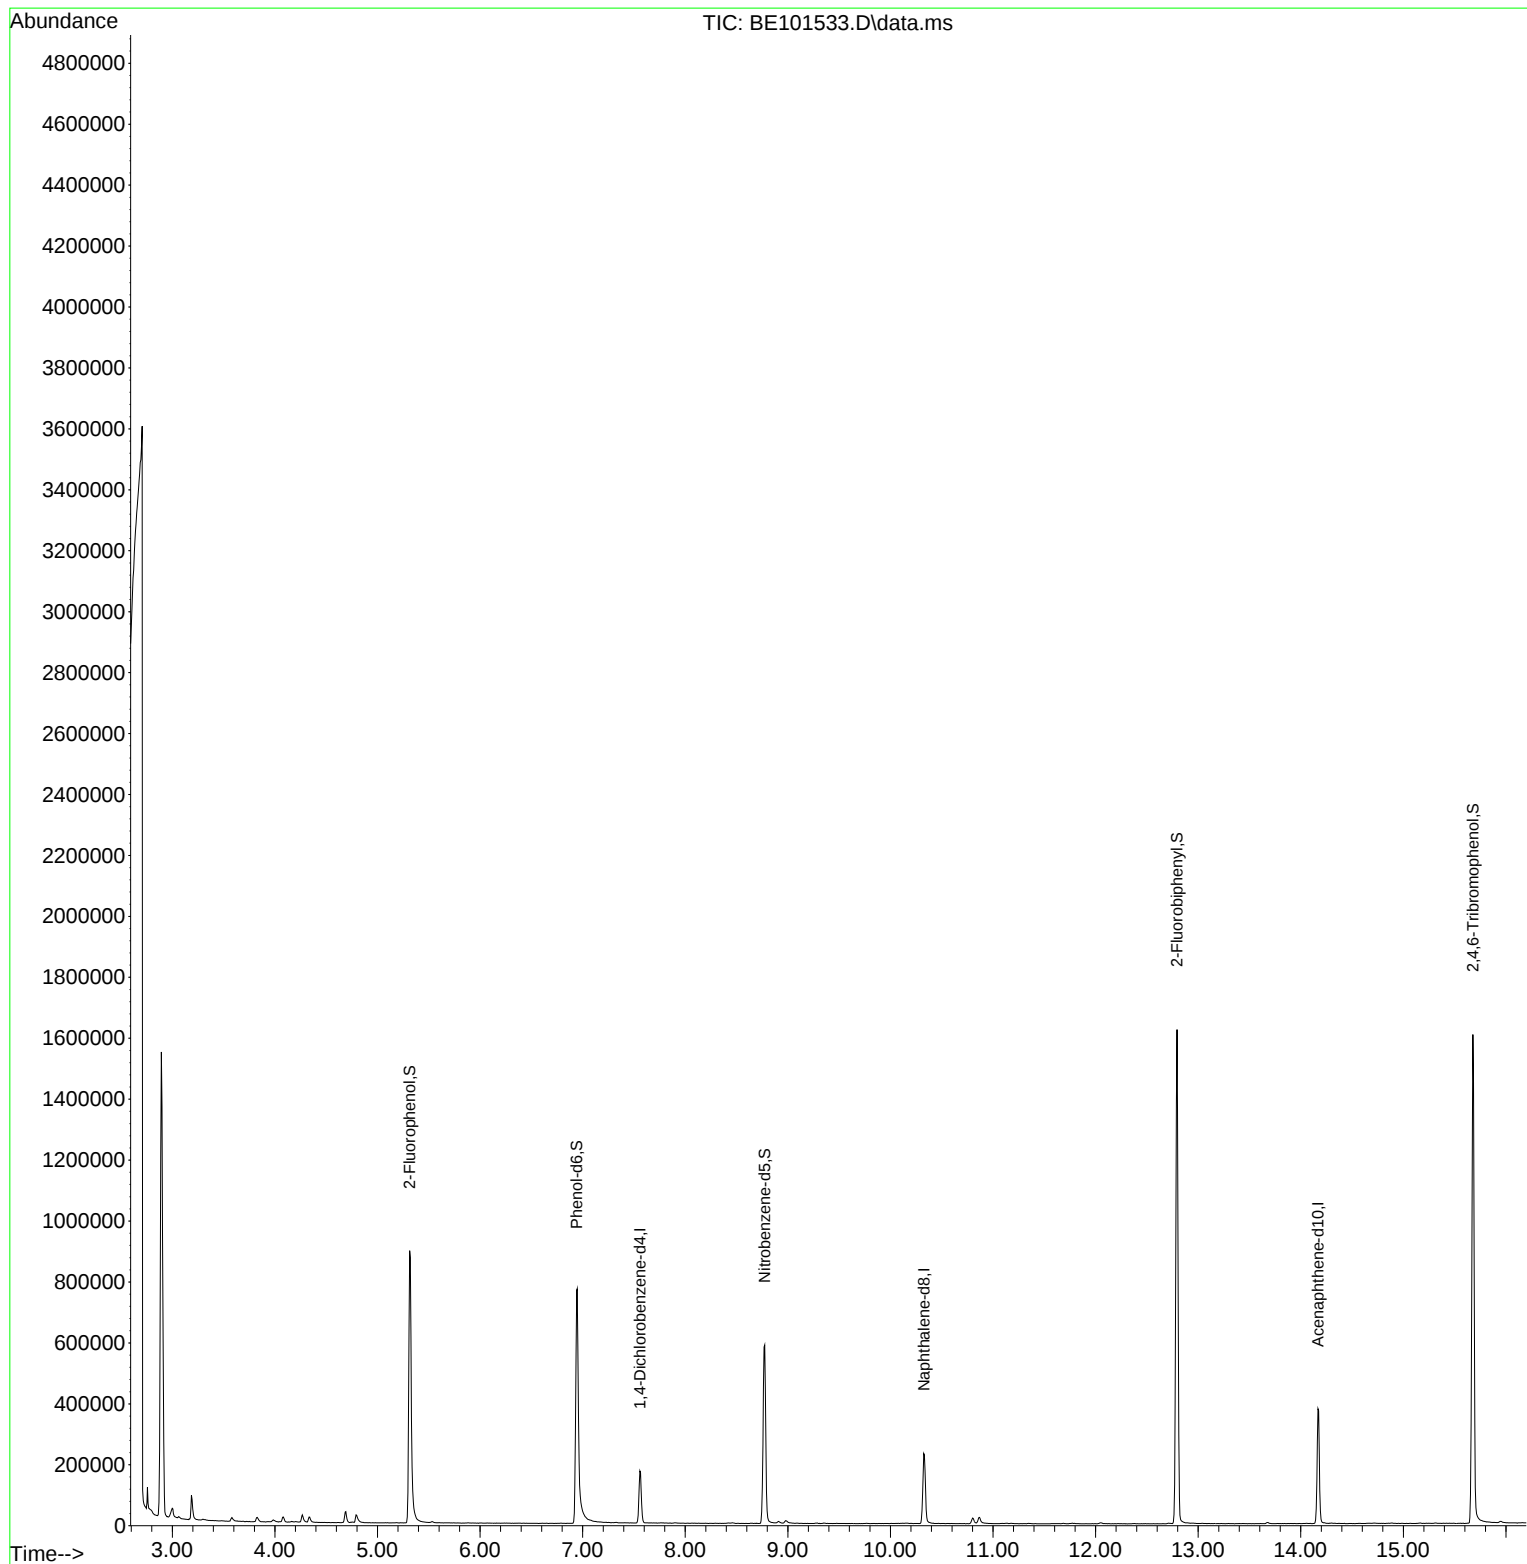

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101533.D
Acq On : 7 Nov 2024 16:19
Operator : RC/JU
Sample : P4680-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F26

Quant Time: Nov 07 16:55:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

