

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101535.D
 Acq On : 7 Nov 2024 17:30
 Operator : RC/JU
 Sample : P4693-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-G4-WC

Quant Time: Nov 07 23:57:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	61445	20.000	ng	0.00
21) Naphthalene-d8	10.328	136	273059	20.000	ng	0.00
39) Acenaphthene-d10	14.170	164	180445	20.000	ng	0.00
64) Phenanthrene-d10	16.908	188	407677	20.000	ng	0.00
76) Chrysene-d12	21.068	240	453182	20.000	ng	0.00
86) Perylene-d12	23.354	264	596162	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.316	112	529101	152.257	ng	0.00
7) Phenol-d6	6.944	99	666580	139.904	ng	0.00
23) Nitrobenzene-d5	8.771	82	418137	96.725	ng	0.00
42) 2,4,6-Tribromophenol	15.680	330	509798	150.142	ng	0.00
45) 2-Fluorobiphenyl	12.796	172	1065226	96.390	ng	0.00
79) Terphenyl-d14	19.505	244	2210173	107.956	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101535.D
Acq On : 7 Nov 2024 17:30
Operator : RC/JU
Sample : P4693-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G4-WC

Quant Time: Nov 07 23:57:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

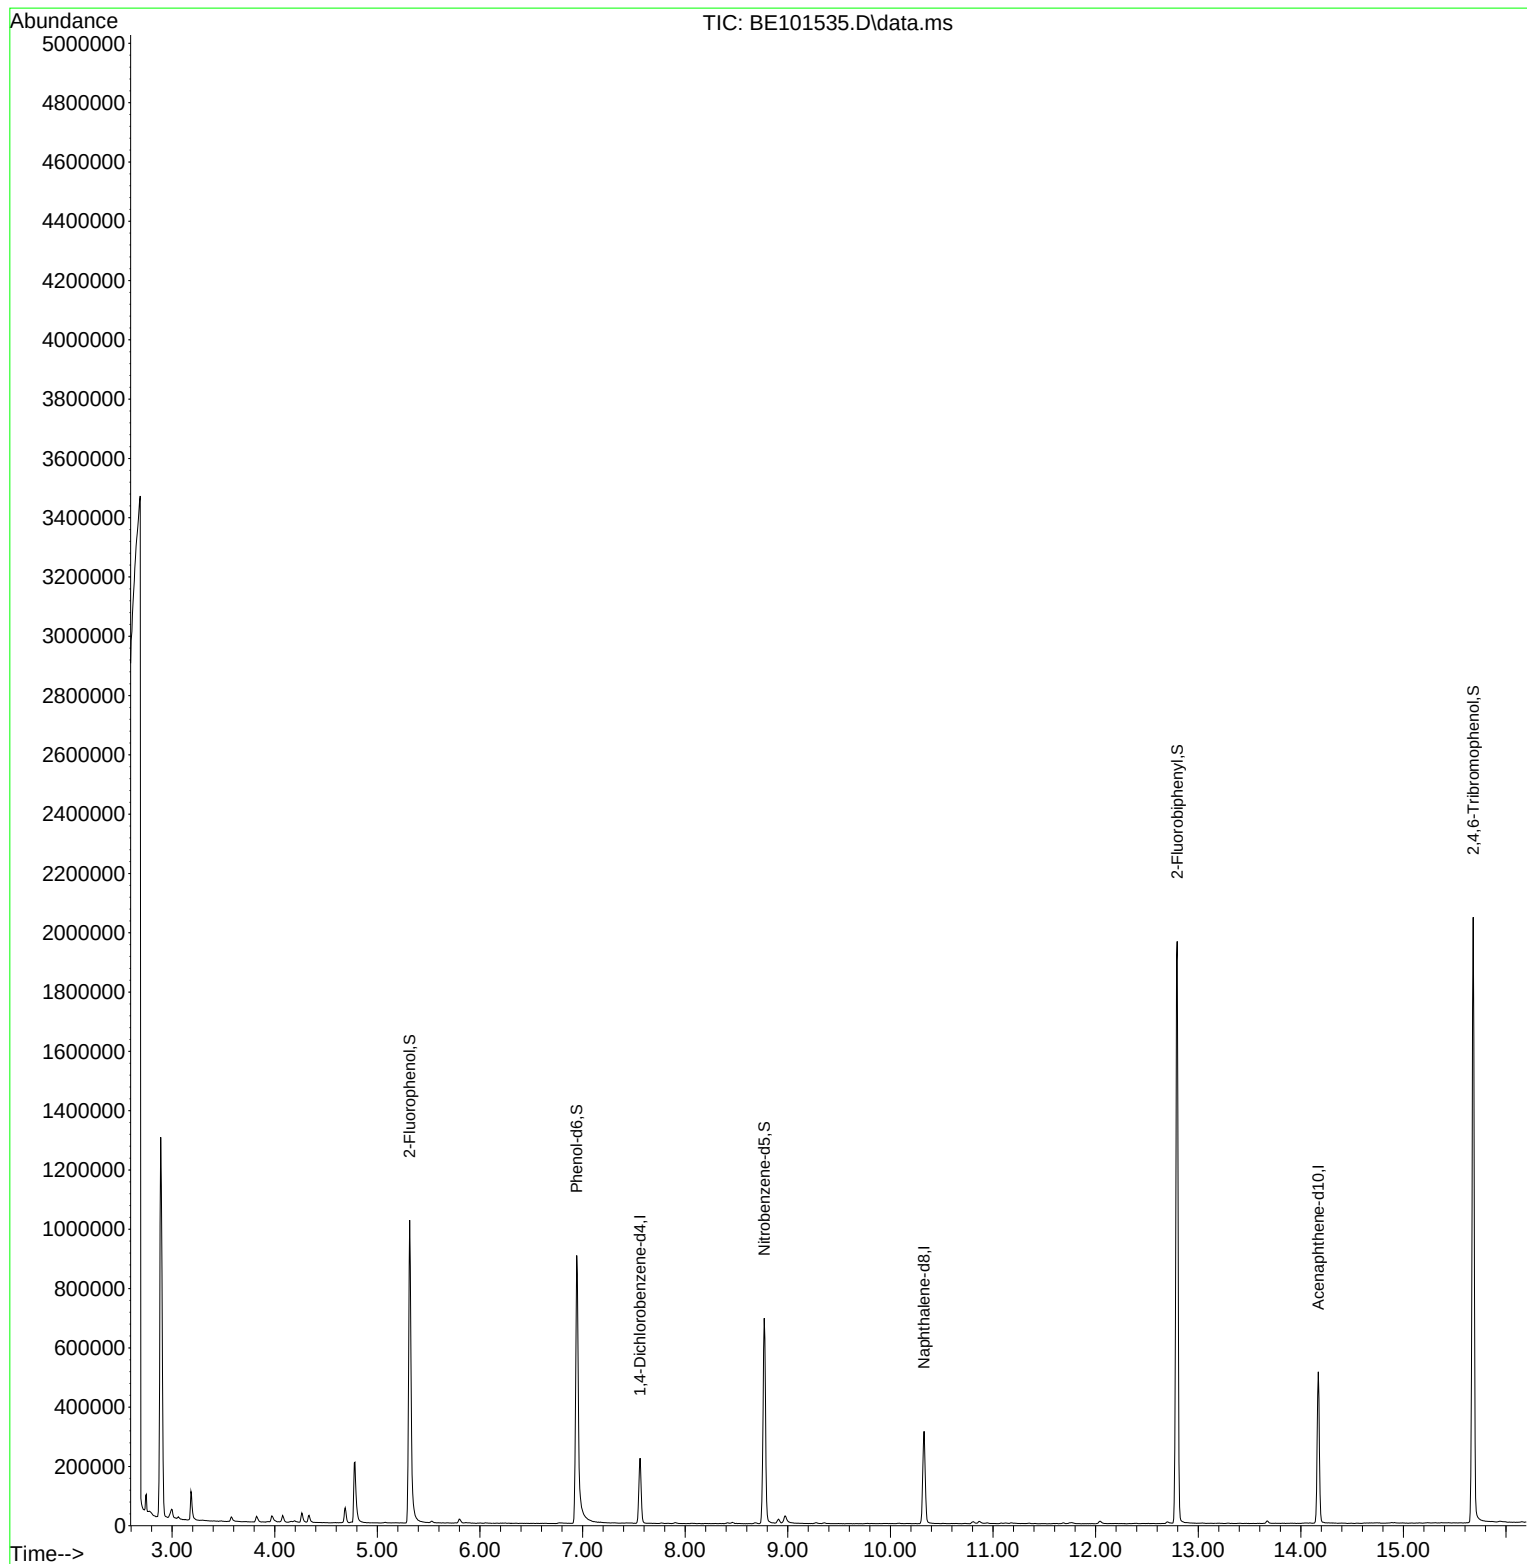

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101535.D
Acq On : 7 Nov 2024 17:30
Operator : RC/JU
Sample : P4693-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G4-WC

Quant Time: Nov 07 23:57:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

