

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101536.D
 Acq On : 7 Nov 2024 18:03
 Operator : RC/JU
 Sample : P4693-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-G5-WC

Quant Time: Nov 07 23:57:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	49732	20.000	ng	0.00
21) Naphthalene-d8	10.328	136	218721	20.000	ng	0.00
39) Acenaphthene-d10	14.170	164	146602	20.000	ng	0.00
64) Phenanthrene-d10	16.908	188	332636	20.000	ng	0.00
76) Chrysene-d12	21.068	240	381237	20.000	ng	0.00
86) Perylene-d12	23.353	264	492462	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.316	112	500458	177.933	ng	0.00
7) Phenol-d6	6.943	99	614313	159.301	ng	0.00
23) Nitrobenzene-d5	8.771	82	404613	116.849	ng	0.00
42) 2,4,6-Tribromophenol	15.680	330	479103	173.676	ng	0.00
45) 2-Fluorobiphenyl	12.795	172	1013496	112.880	ng	0.00
79) Terphenyl-d14	19.505	244	2160182	125.426	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101536.D
Acq On : 7 Nov 2024 18:03
Operator : RC/JU
Sample : P4693-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G5-WC

Quant Time: Nov 07 23:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

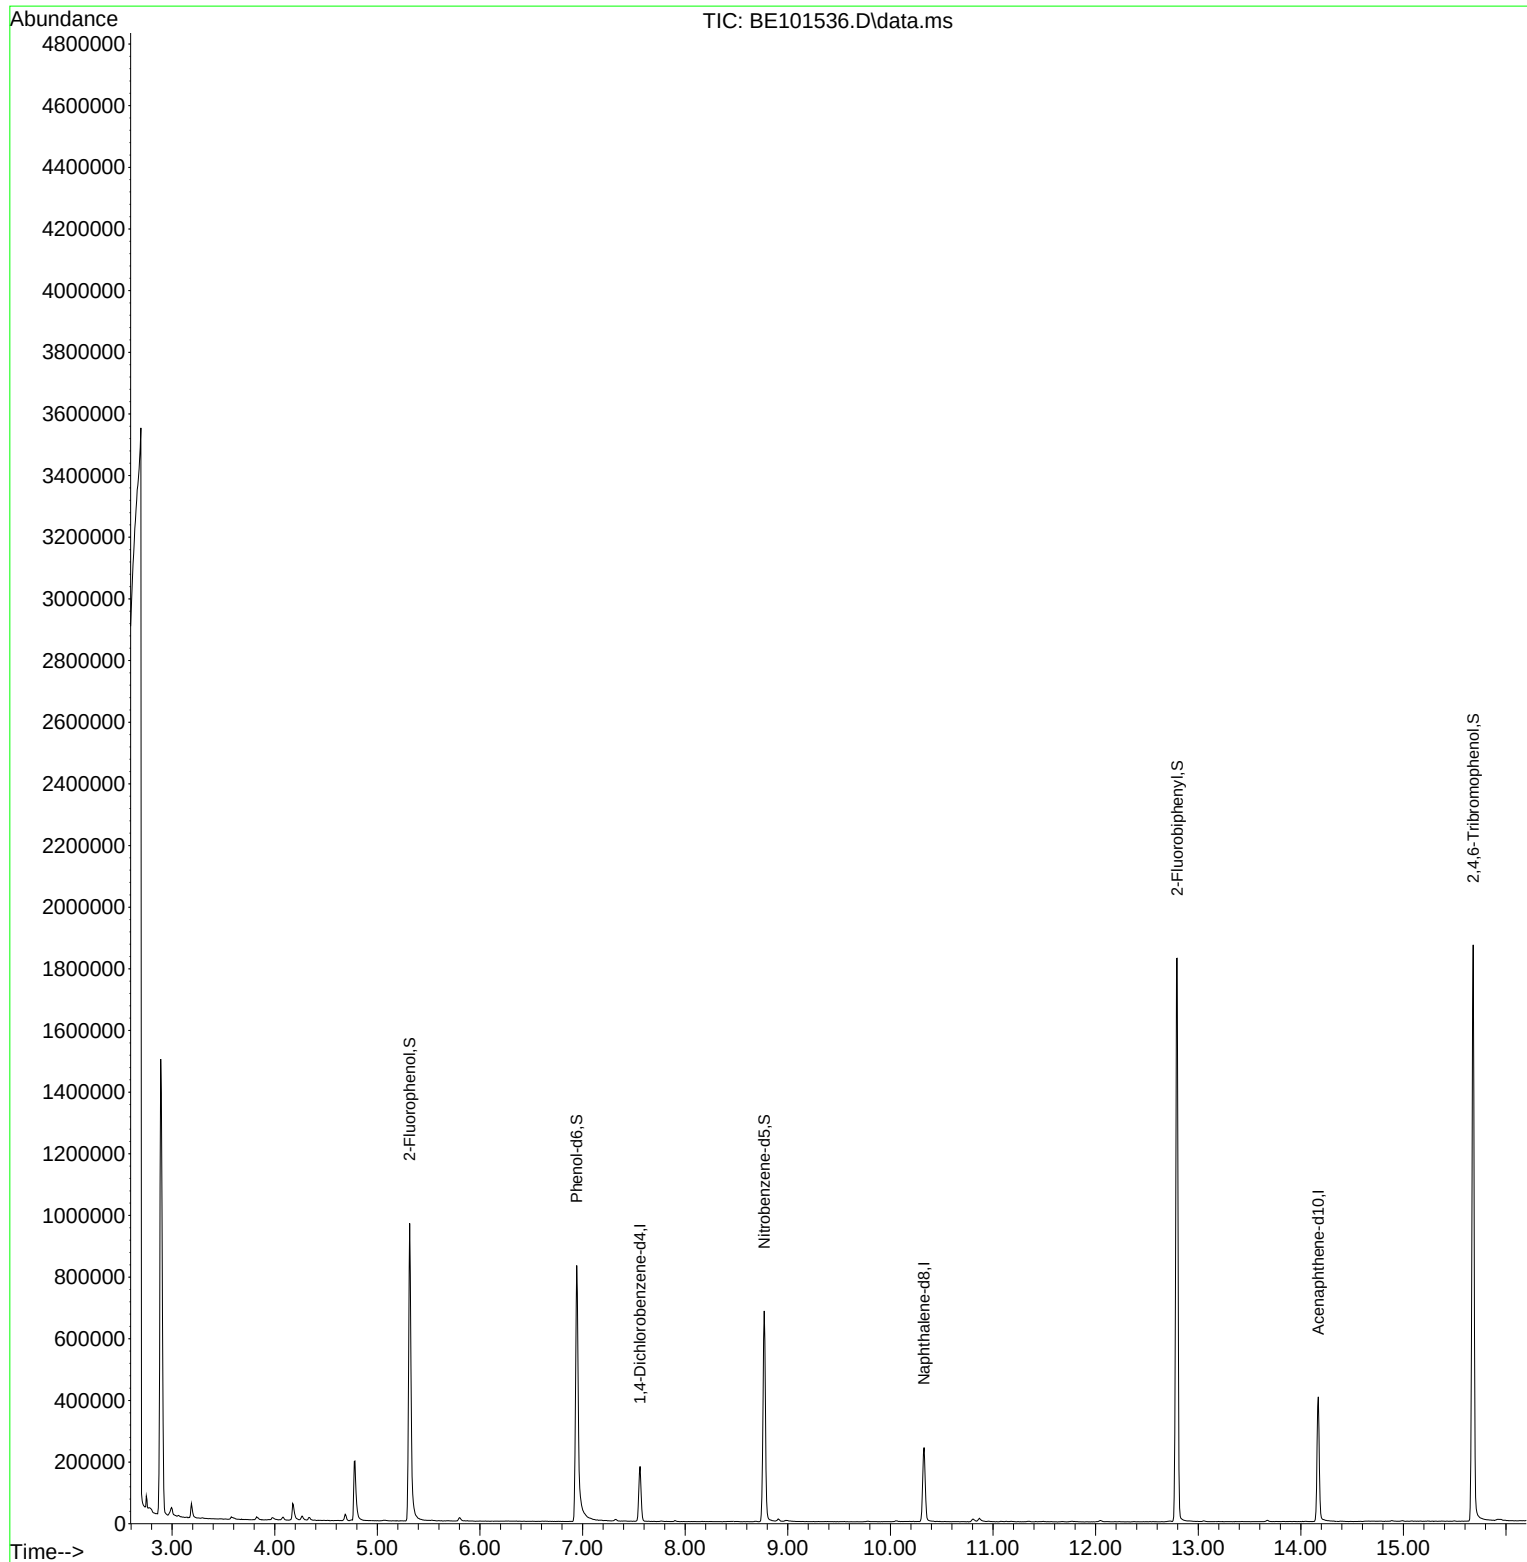

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101536.D
Acq On : 7 Nov 2024 18:03
Operator : RC/JU
Sample : P4693-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G5-WC

Quant Time: Nov 07 23:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

