

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101541.D
 Acq On : 7 Nov 2024 21:02
 Operator : RC/JU
 Sample : P4695-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Z-01

Quant Time: Nov 07 23:59:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	56972	20.000	ng	0.00
21) Naphthalene-d8	10.326	136	247568	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	167071	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	382642	20.000	ng	0.00
76) Chrysene-d12	21.066	240	436296	20.000	ng	-0.01
86) Perylene-d12	23.352	264	568971	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.314	112	456349	141.632	ng	0.00
7) Phenol-d6	6.942	99	549326	124.346	ng	0.00
23) Nitrobenzene-d5	8.769	82	373049	95.180	ng	0.00
42) 2,4,6-Tribromophenol	15.679	330	443691	141.133	ng	0.00
45) 2-Fluorobiphenyl	12.794	172	950510	92.894	ng	0.00
79) Terphenyl-d14	19.504	244	2131761	108.156	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101541.D
Acq On : 7 Nov 2024 21:02
Operator : RC/JU
Sample : P4695-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-01

Quant Time: Nov 07 23:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

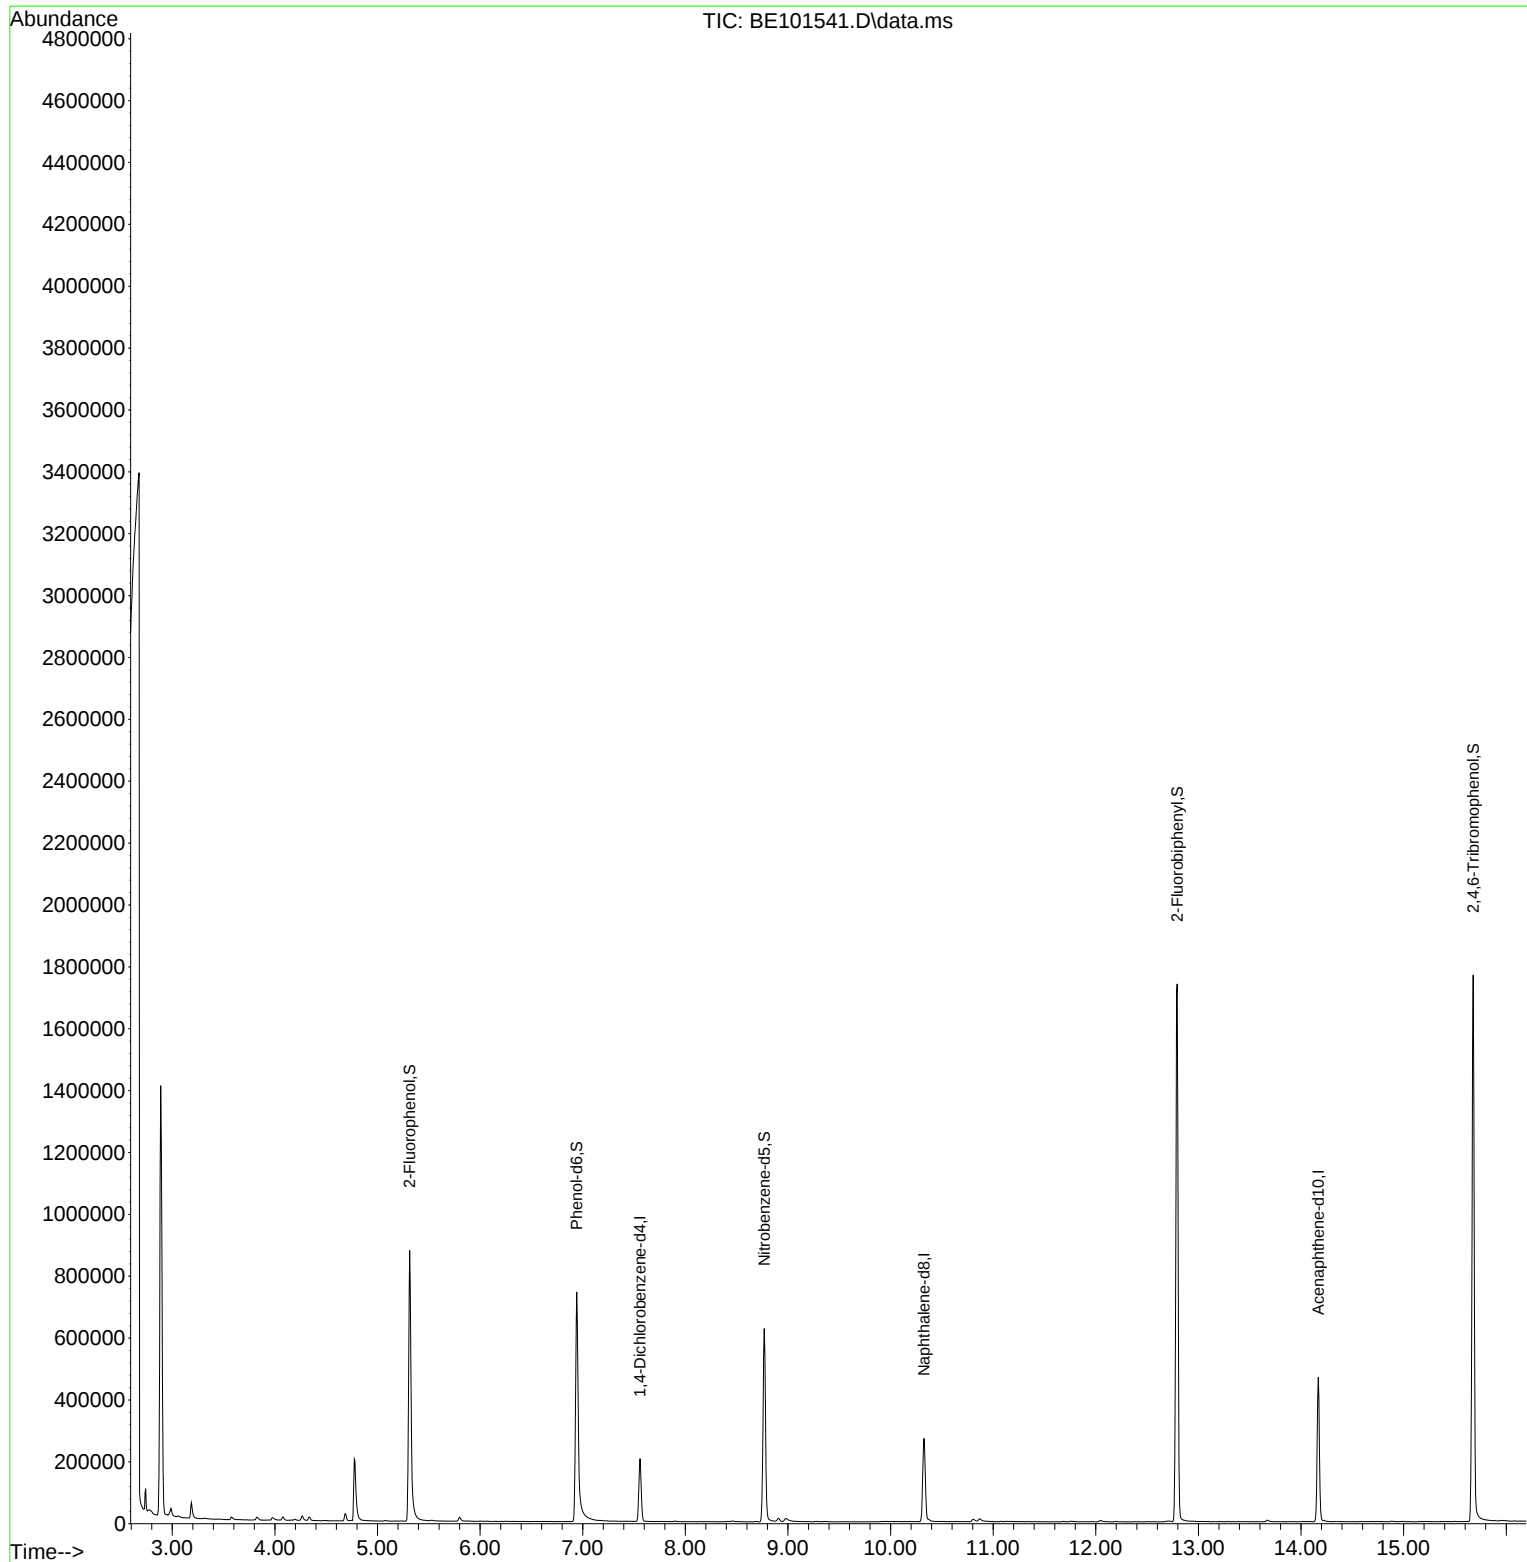

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101541.D
Acq On : 7 Nov 2024 21:02
Operator : RC/JU
Sample : P4695-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-01

Quant Time: Nov 07 23:59:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

