

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
 Data File : BE101542.D
 Acq On : 7 Nov 2024 21:38
 Operator : RC/JU
 Sample : P4701-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F3

Quant Time: Nov 08 00:00:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	51824	20.000	ng	0.00
21) Naphthalene-d8	10.328	136	225065	20.000	ng	0.00
39) Acenaphthene-d10	14.170	164	122500	20.000	ng	0.00
64) Phenanthrene-d10	16.908	188	344504	20.000	ng	0.00
76) Chrysene-d12	21.068	240	355667	20.000	ng	0.00
86) Perylene-d12	23.348	264	161085	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.316	112	474568	161.917	ng	0.00
7) Phenol-d6	6.943	99	515248	128.218	ng	0.00
23) Nitrobenzene-d5	8.771	82	385664	108.237	ng	0.00
42) 2,4,6-Tribromophenol	15.680	330	446239	193.589	ng	0.00
45) 2-Fluorobiphenyl	12.790	172	958354	127.739	ng	0.00
79) Terphenyl-d14	19.505	244	2076378	129.227	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101542.D
Acq On : 7 Nov 2024 21:38
Operator : RC/JU
Sample : P4701-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F3

Quant Time: Nov 08 00:00:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

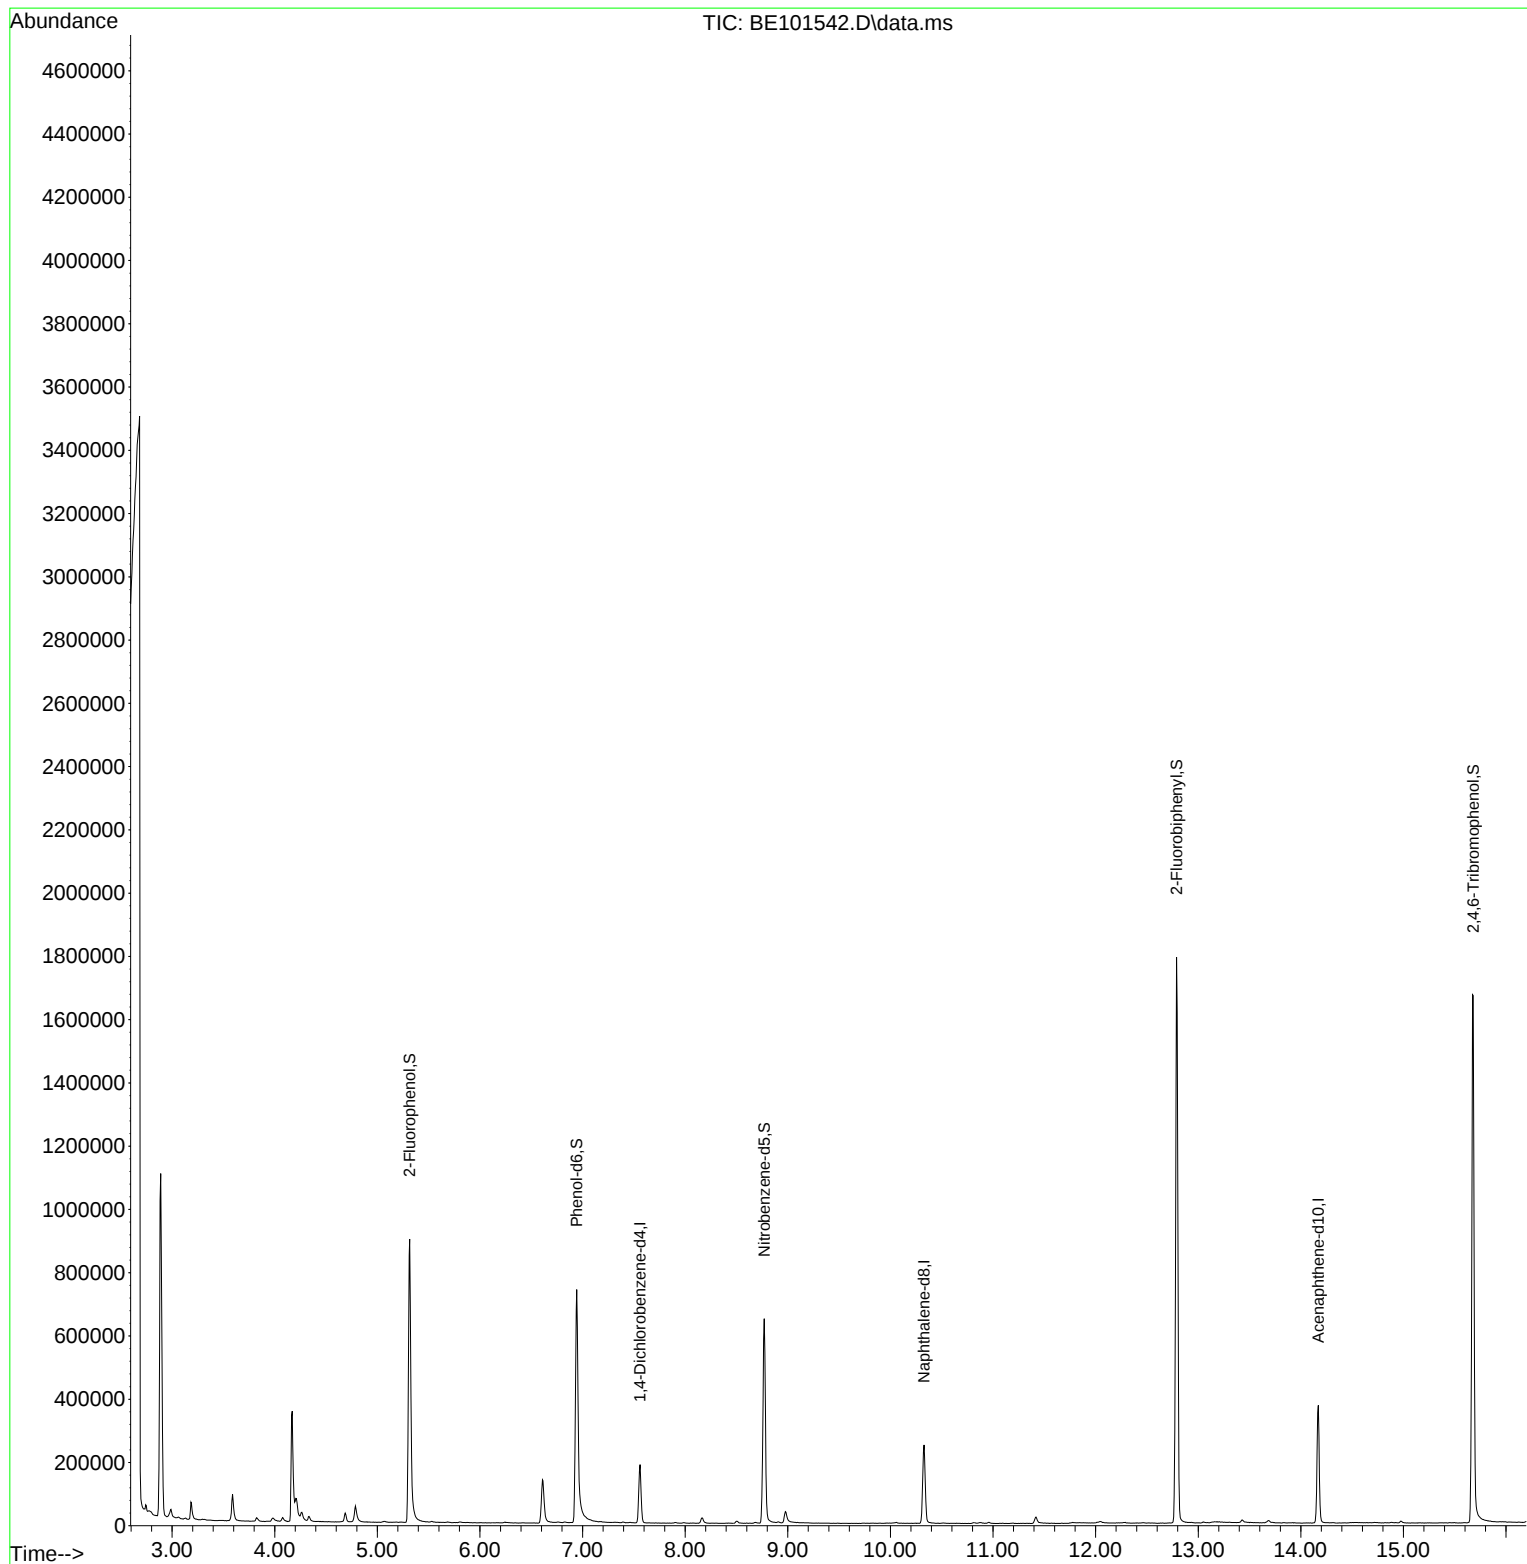

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101542.D
Acq On : 7 Nov 2024 21:38
Operator : RC/JU
Sample : P4701-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F3

Quant Time: Nov 08 00:00:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

