
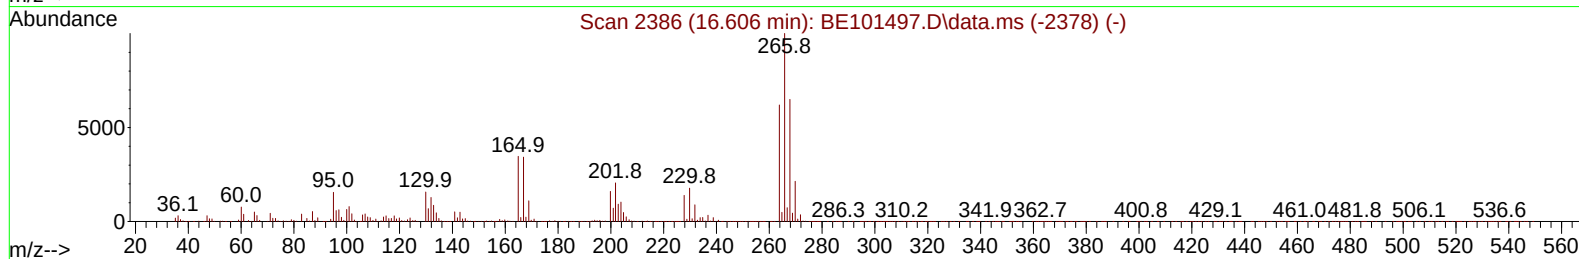
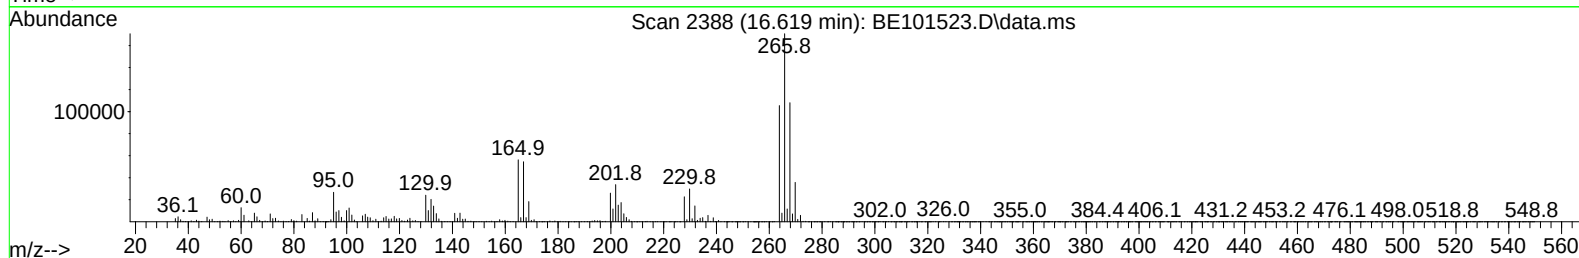


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101523.D
Acq On : 7 Nov 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 11:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

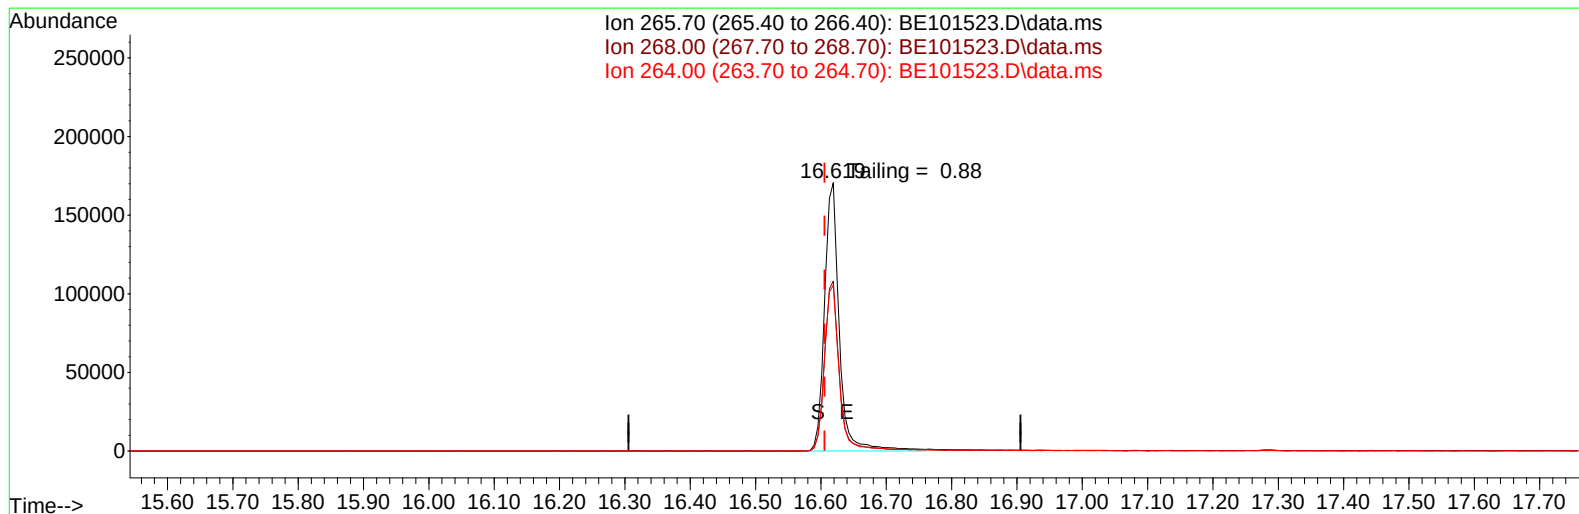

TIC: BE101523.D\data.ms

(70) Pentachlorophenol (C)




16.619min (+ 0.013) 81419.29 ng

response 267400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	63.31
264.00	62.00	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101523.D
Acq On : 7 Nov 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 11:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

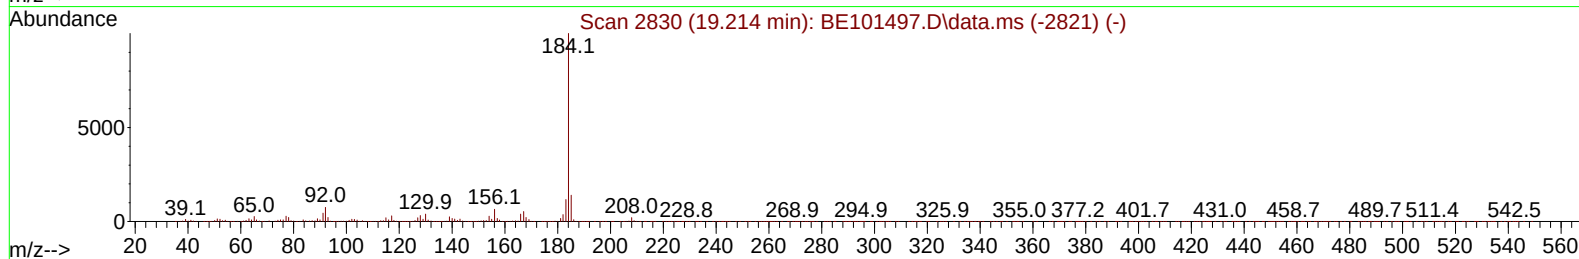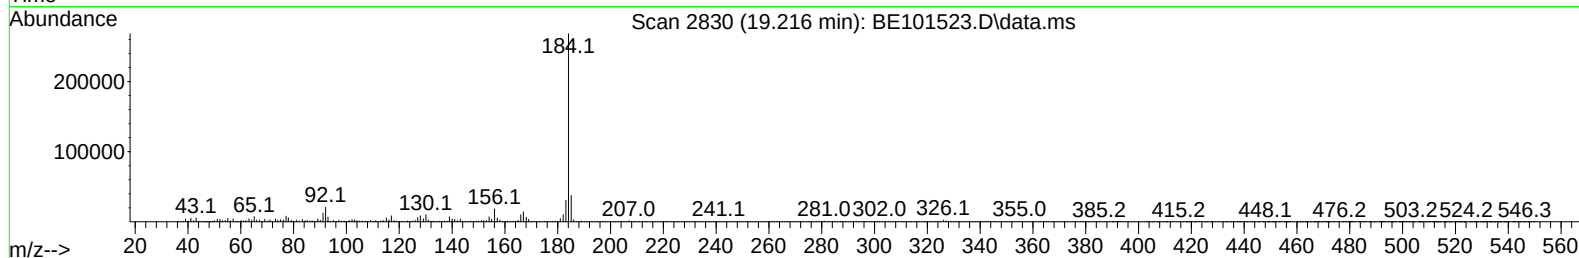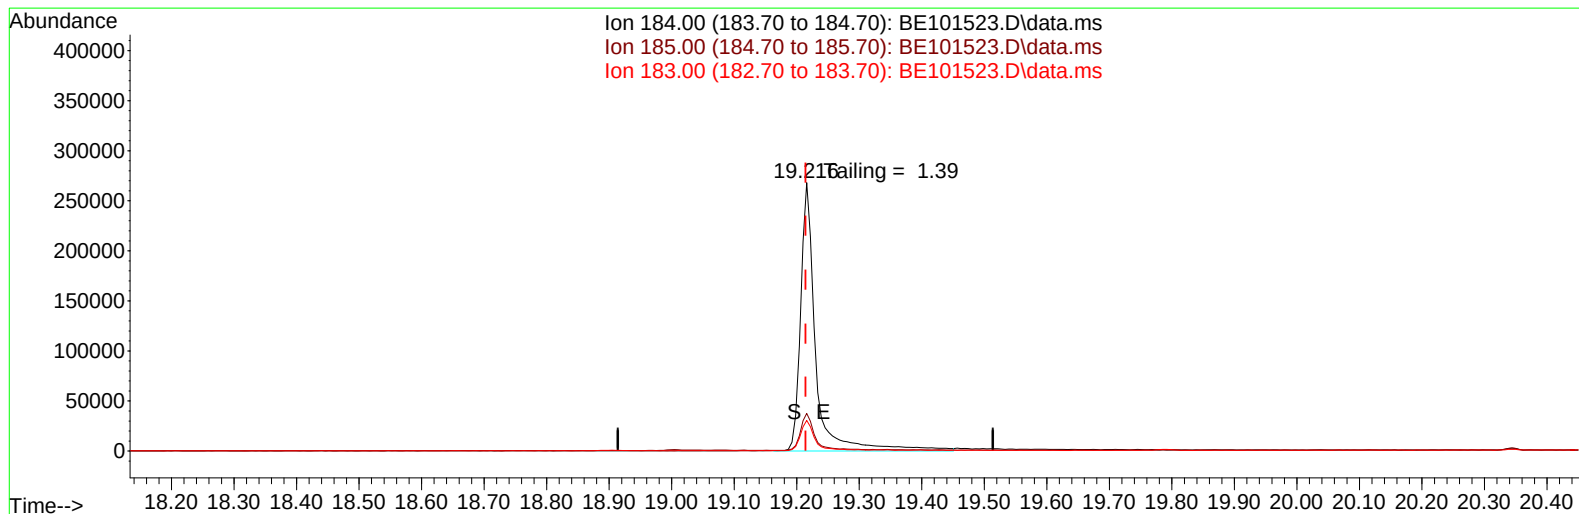

TIC: BE101523.D\data.ms

(77) Benzidine

19.216min (+ 0.002) 13502.07 ng

response 449558

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.70	11.42
0.00	0.00	0.00