
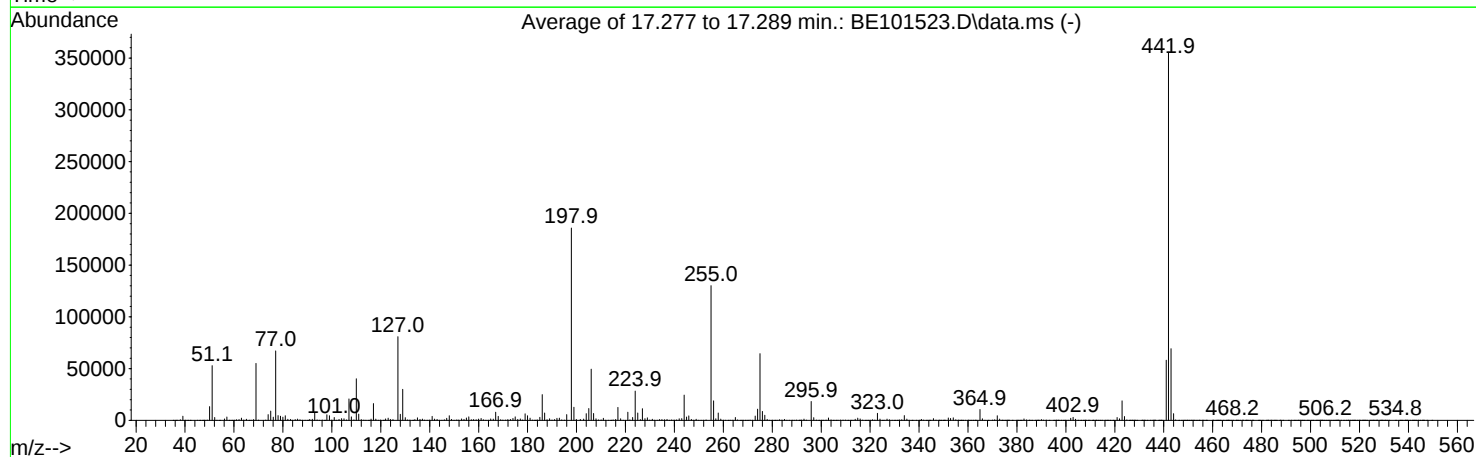


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101523.D
Acq On : 7 Nov 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

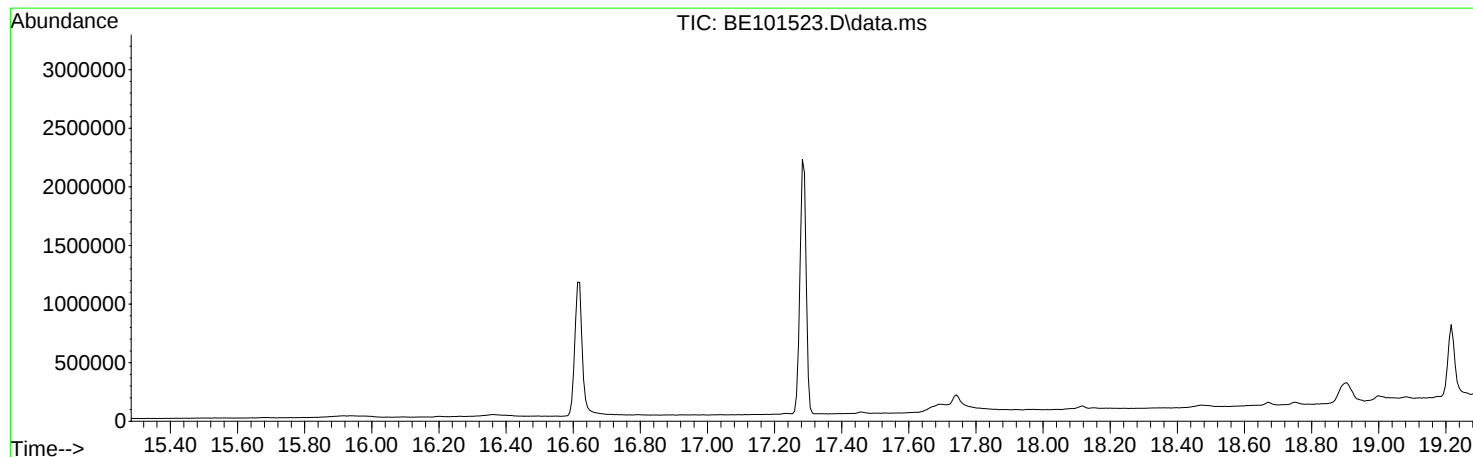

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	52831	PASS
68	69	0.00	2	1.6	858	PASS
69	198	0.00	100	29.6	55031	PASS
70	69	0.00	2	0.5	281	PASS
127	198	10	80	43.5	80780	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	185866	PASS
199	198	5	9	6.9	12746	PASS
275	198	10	60	34.7	64420	PASS
365	198	1	100	5.7	10521	PASS
441	198	0.01	100	31.3	58168	PASS
442	442	50	100	100.0	355362	PASS
443	442	15	24	19.5	69184	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/7/2024	BNA_E	<u>BE101523.D</u>
Compound Name	Response	Retention Time
DDT	747558	20.344
DDD	30153	19.915
DDE	0	19.391
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30153	777711	3.88

Instrument :
BNA_E
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101523.D
Acq On : 7 Nov 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 07 11:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

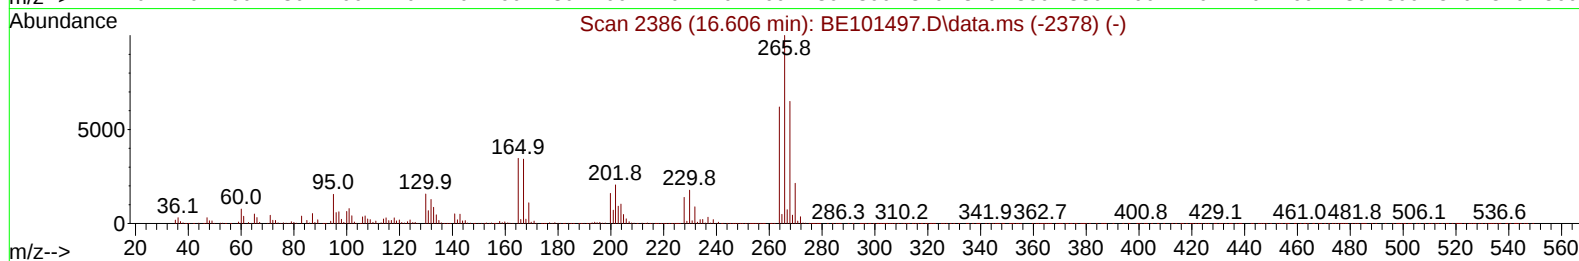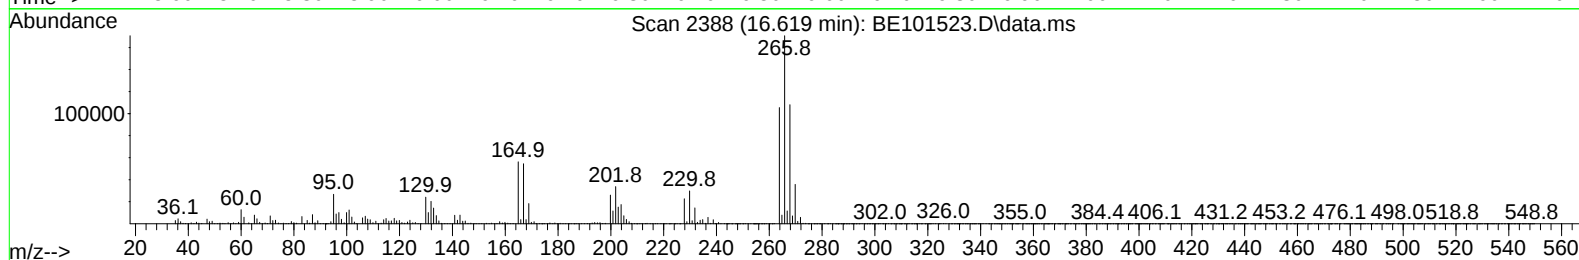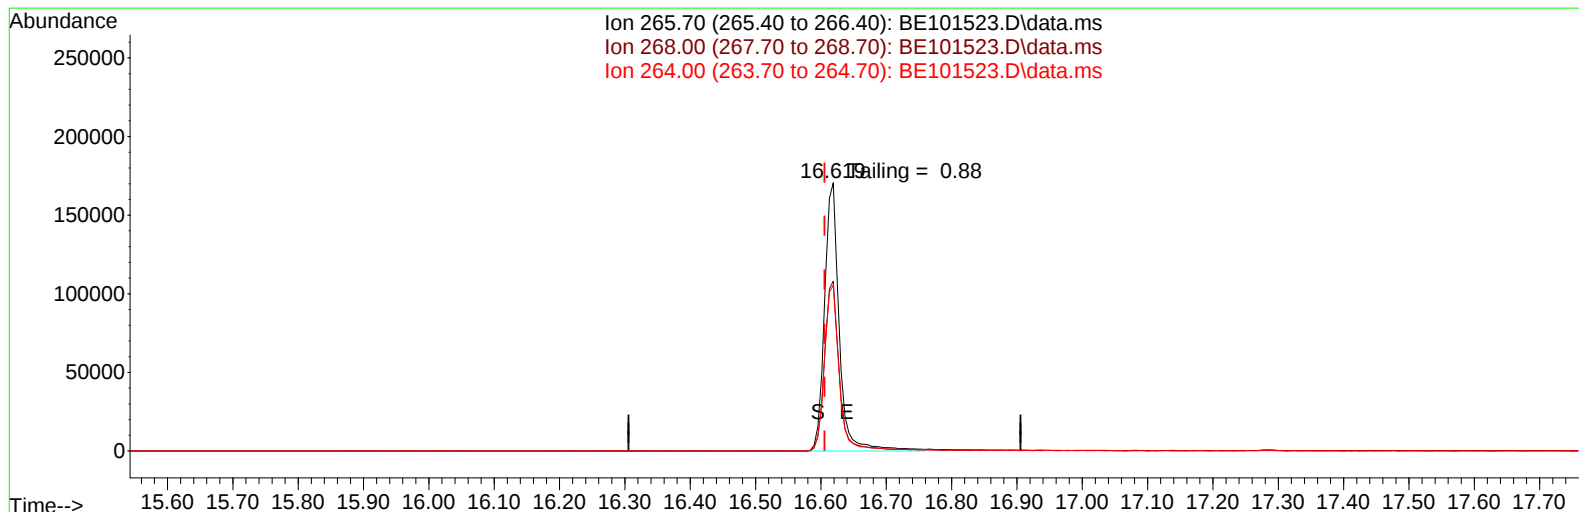

TIC: BE101523.D\data.ms

(70) Pentachlorophenol (C)

16.619min (+ 0.013) 81419.29 ng




response 267400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	63.31
264.00	62.00	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110724\
Data File : BE101523.D
Acq On : 7 Nov 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 07 11:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

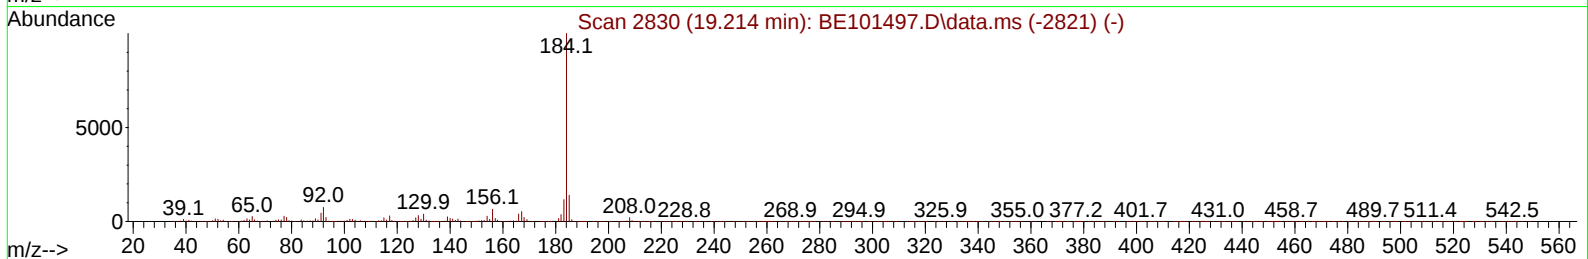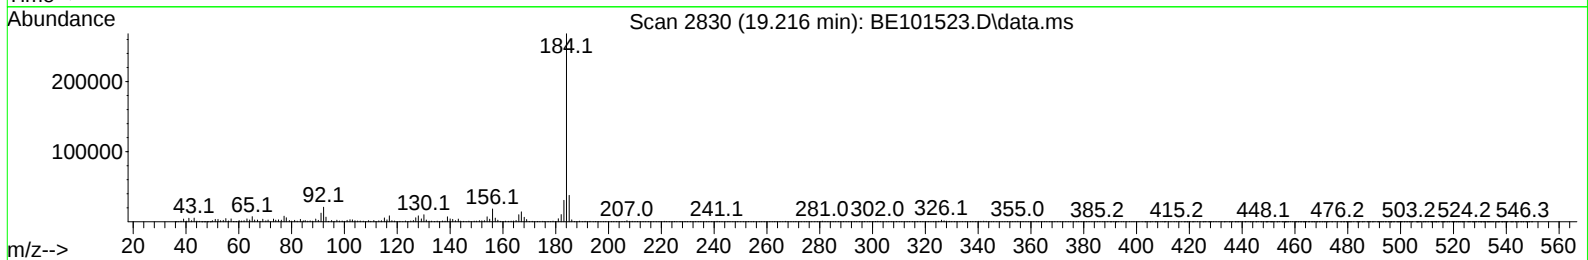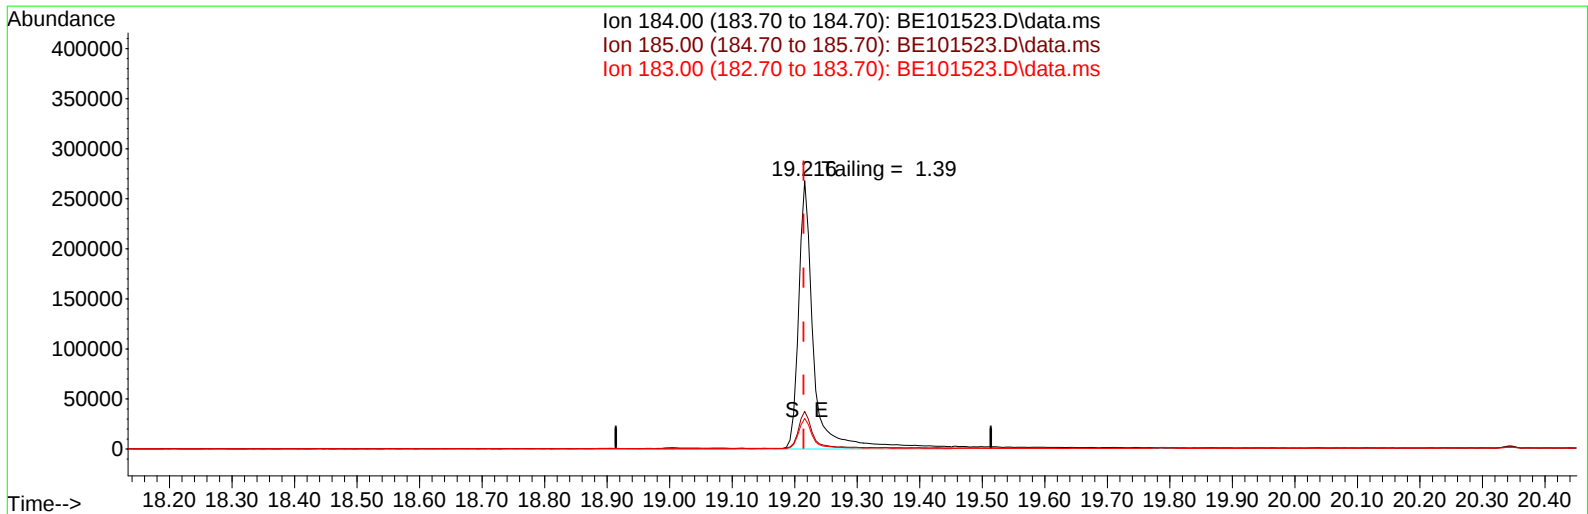

TIC: BE101523.D\data.ms

(77) Benzidine

19.216min (+ 0.002) 13502.07 ng

response 449558

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.70	11.42
0.00	0.00	0.00