


1,4-Dioxane

Response Ratio

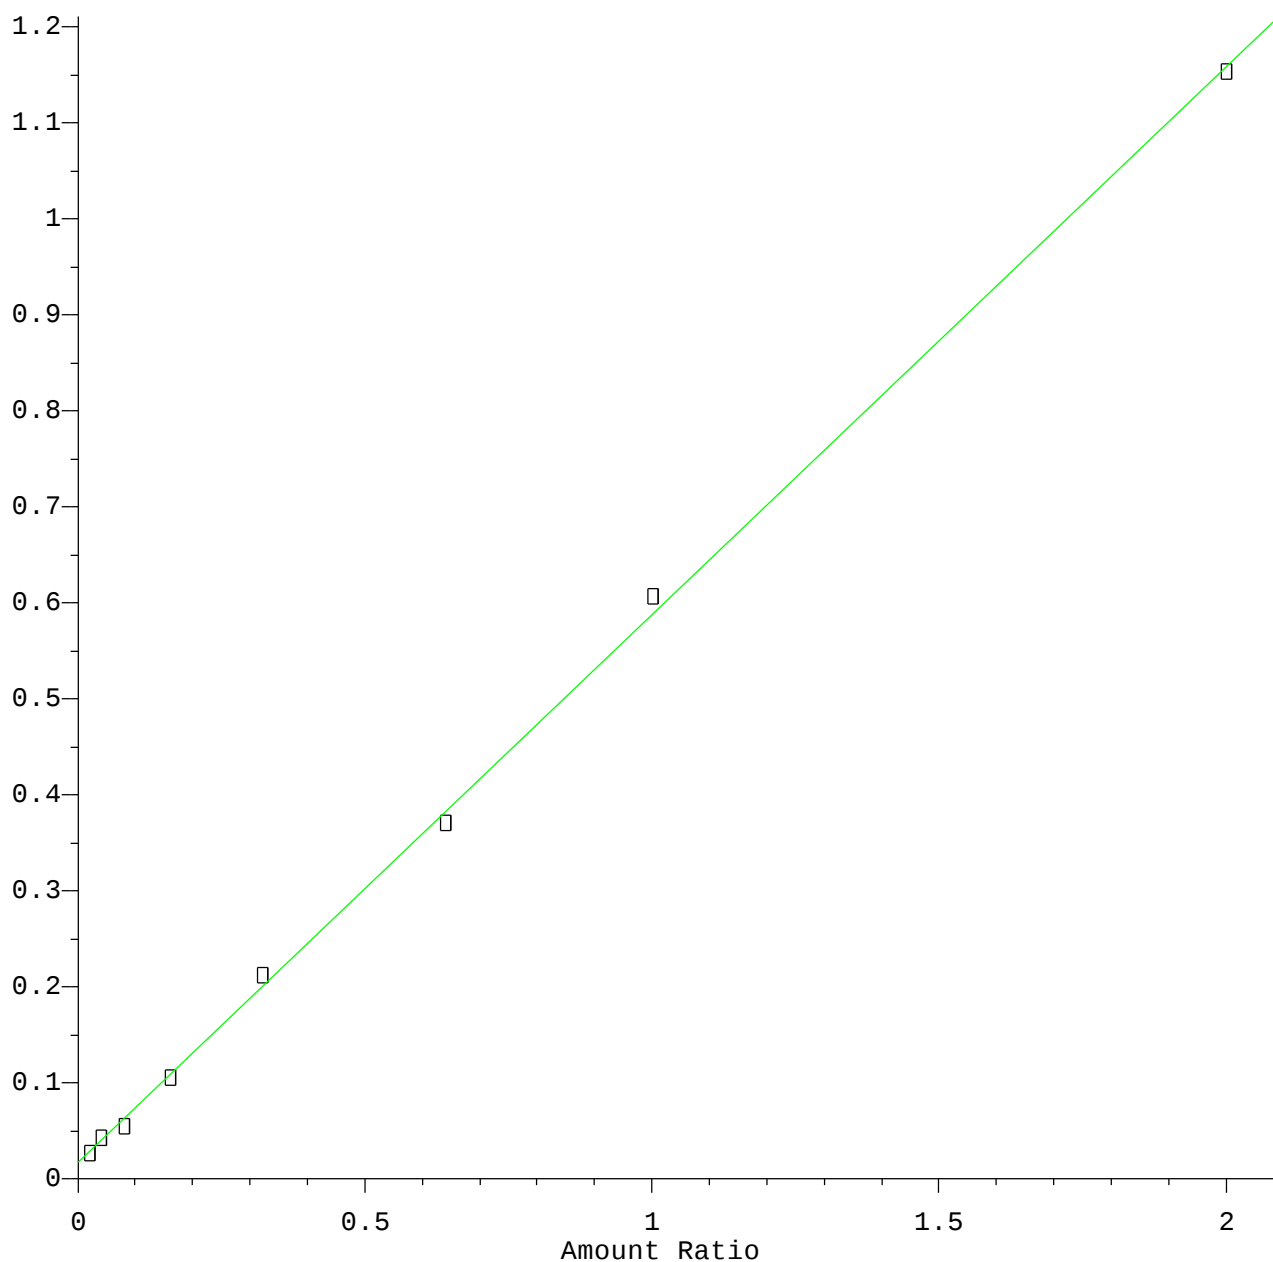


Resp Ratio = $5.71 \times 10^{-1} \times \text{Amt} + 1.74 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016


n-Nitrosodimethylamine

Response Ratio

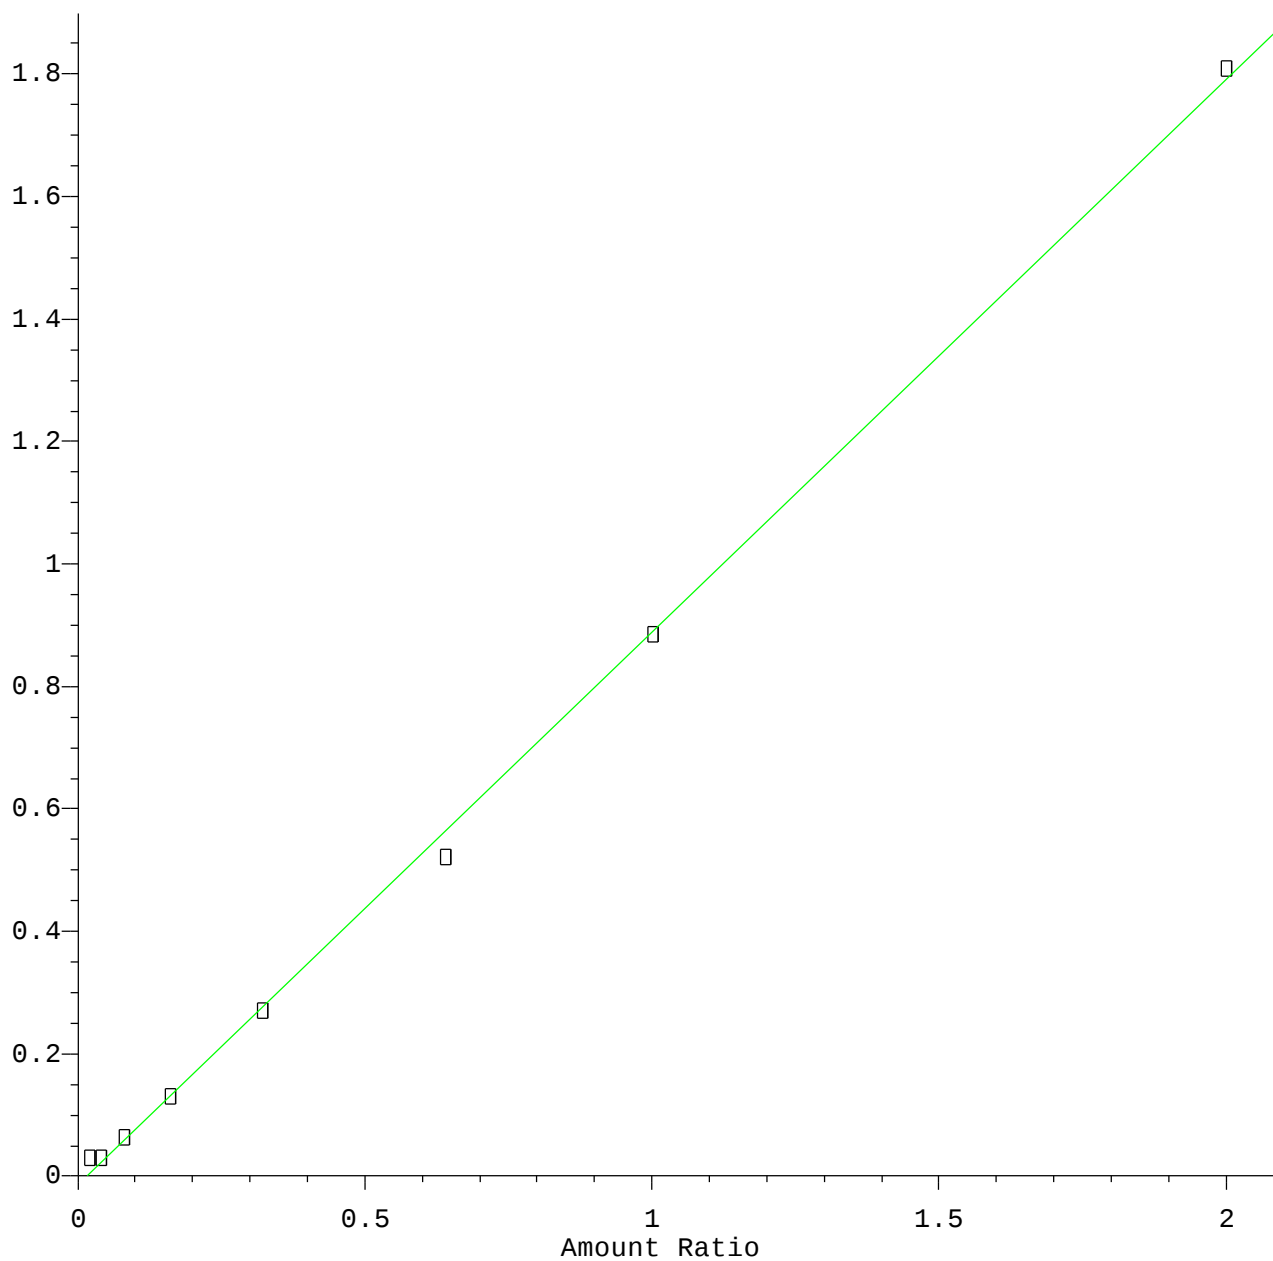

Resp Ratio = $9.03 \times 10^{-1} \times \text{Amt} - 1.42 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016

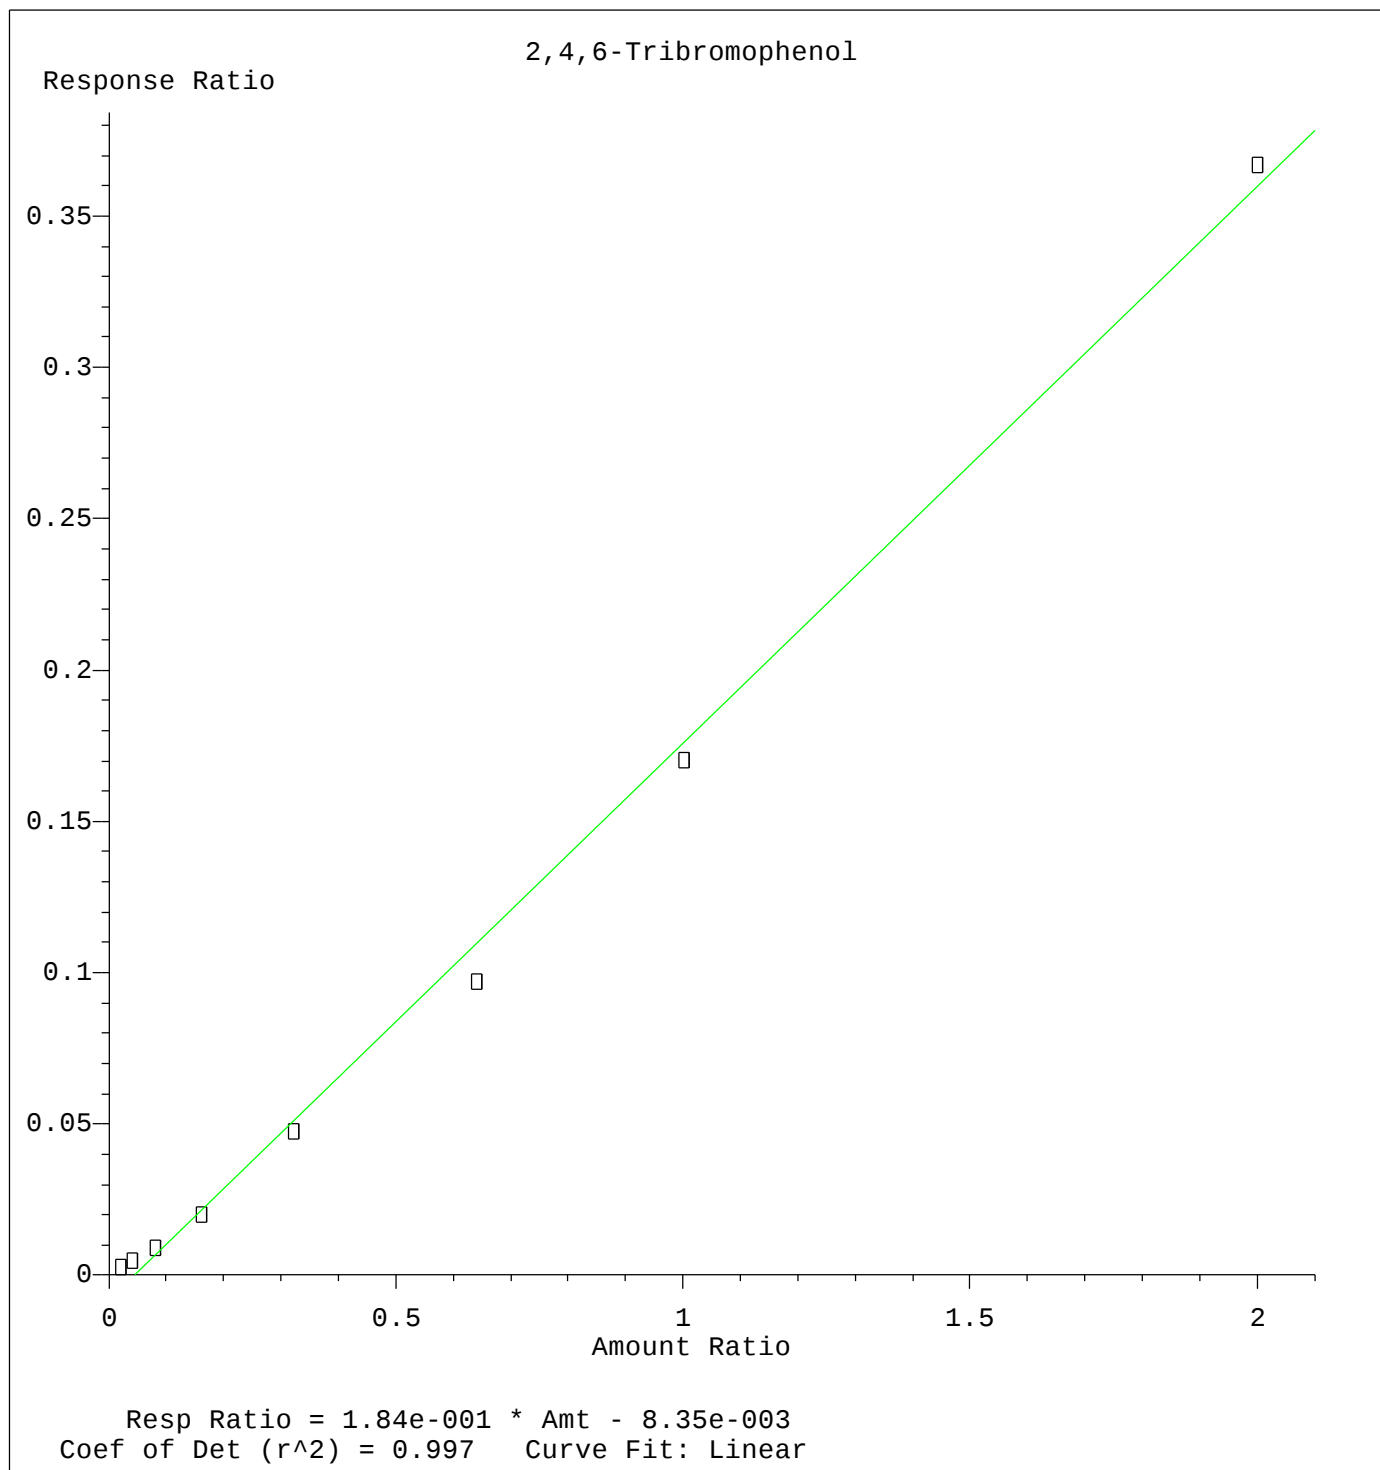

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016

Chrysene

Response Ratio

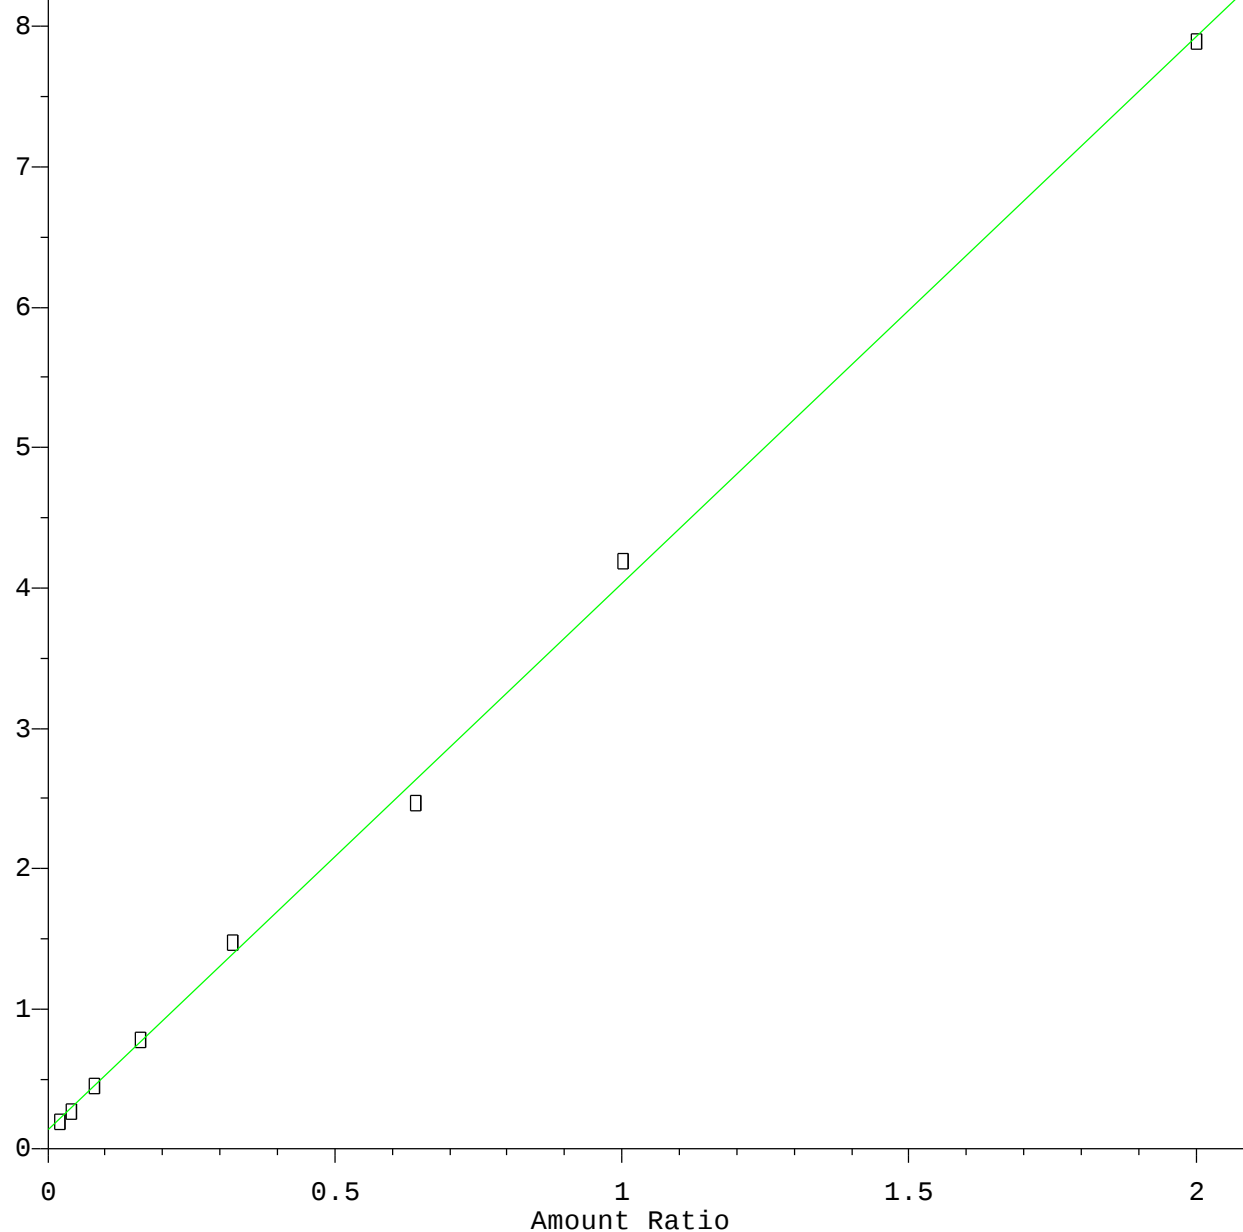


Resp Ratio = $3.89 \times 10^0 \times \text{Amt} + 1.37 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016


Bis(2-ethylhexyl)phthalate

Response Ratio

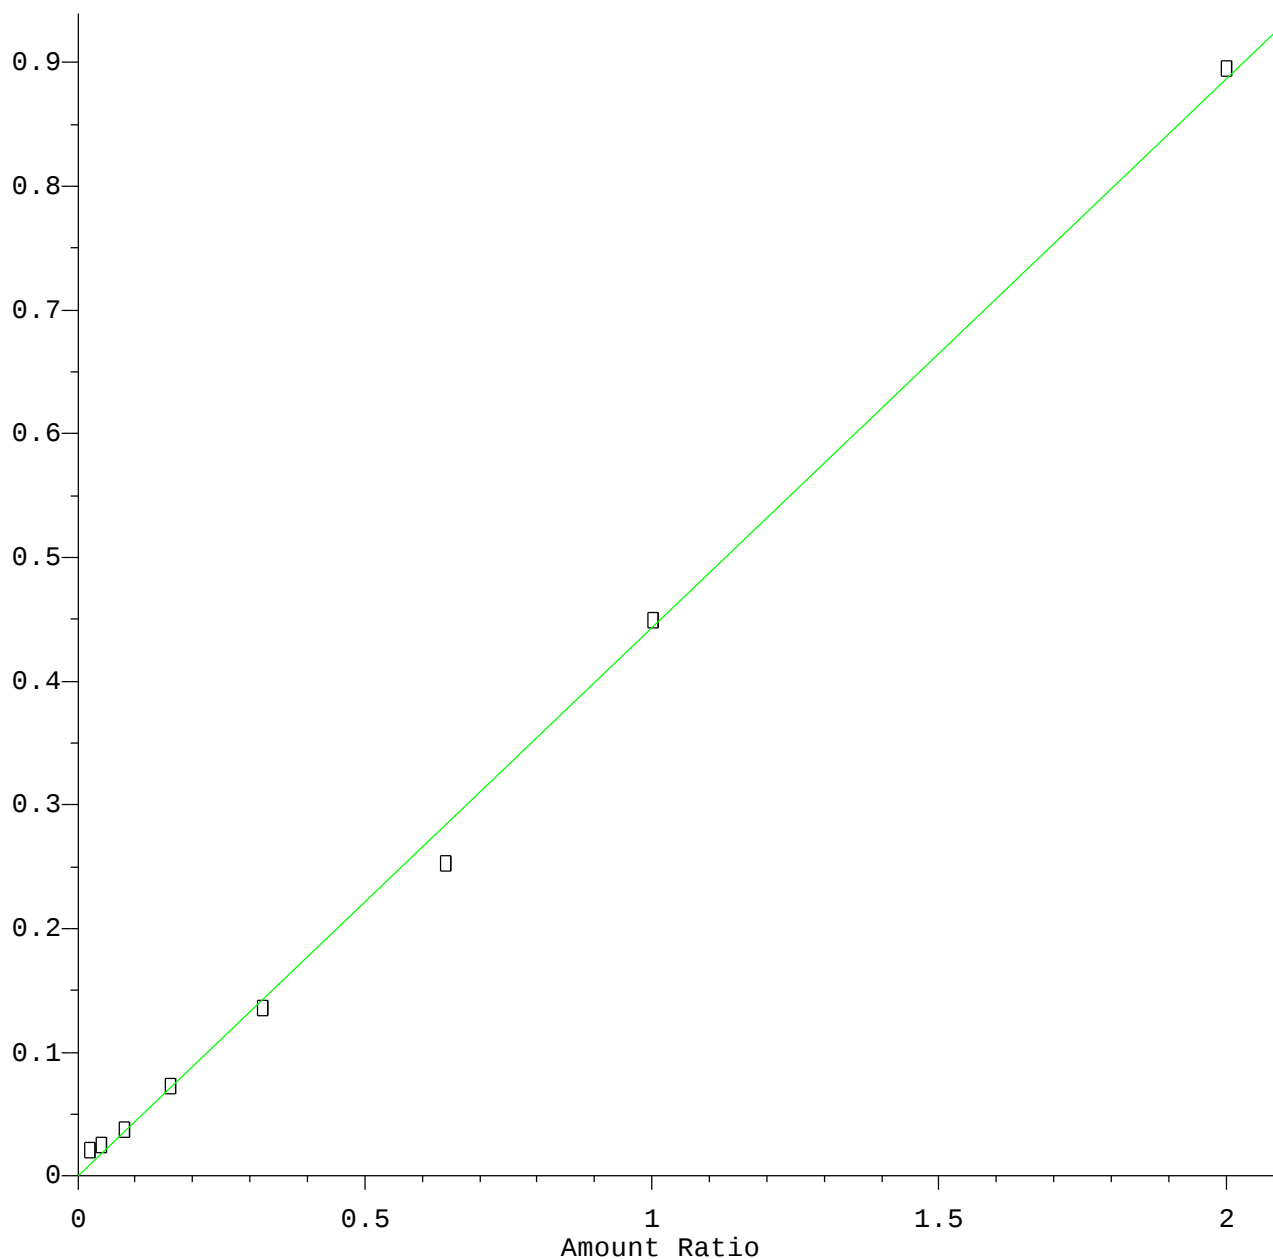


Resp Ratio = $4.44 \times 10^{-1} \times \text{Amt} - 4.53 \times 10^{-4}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016

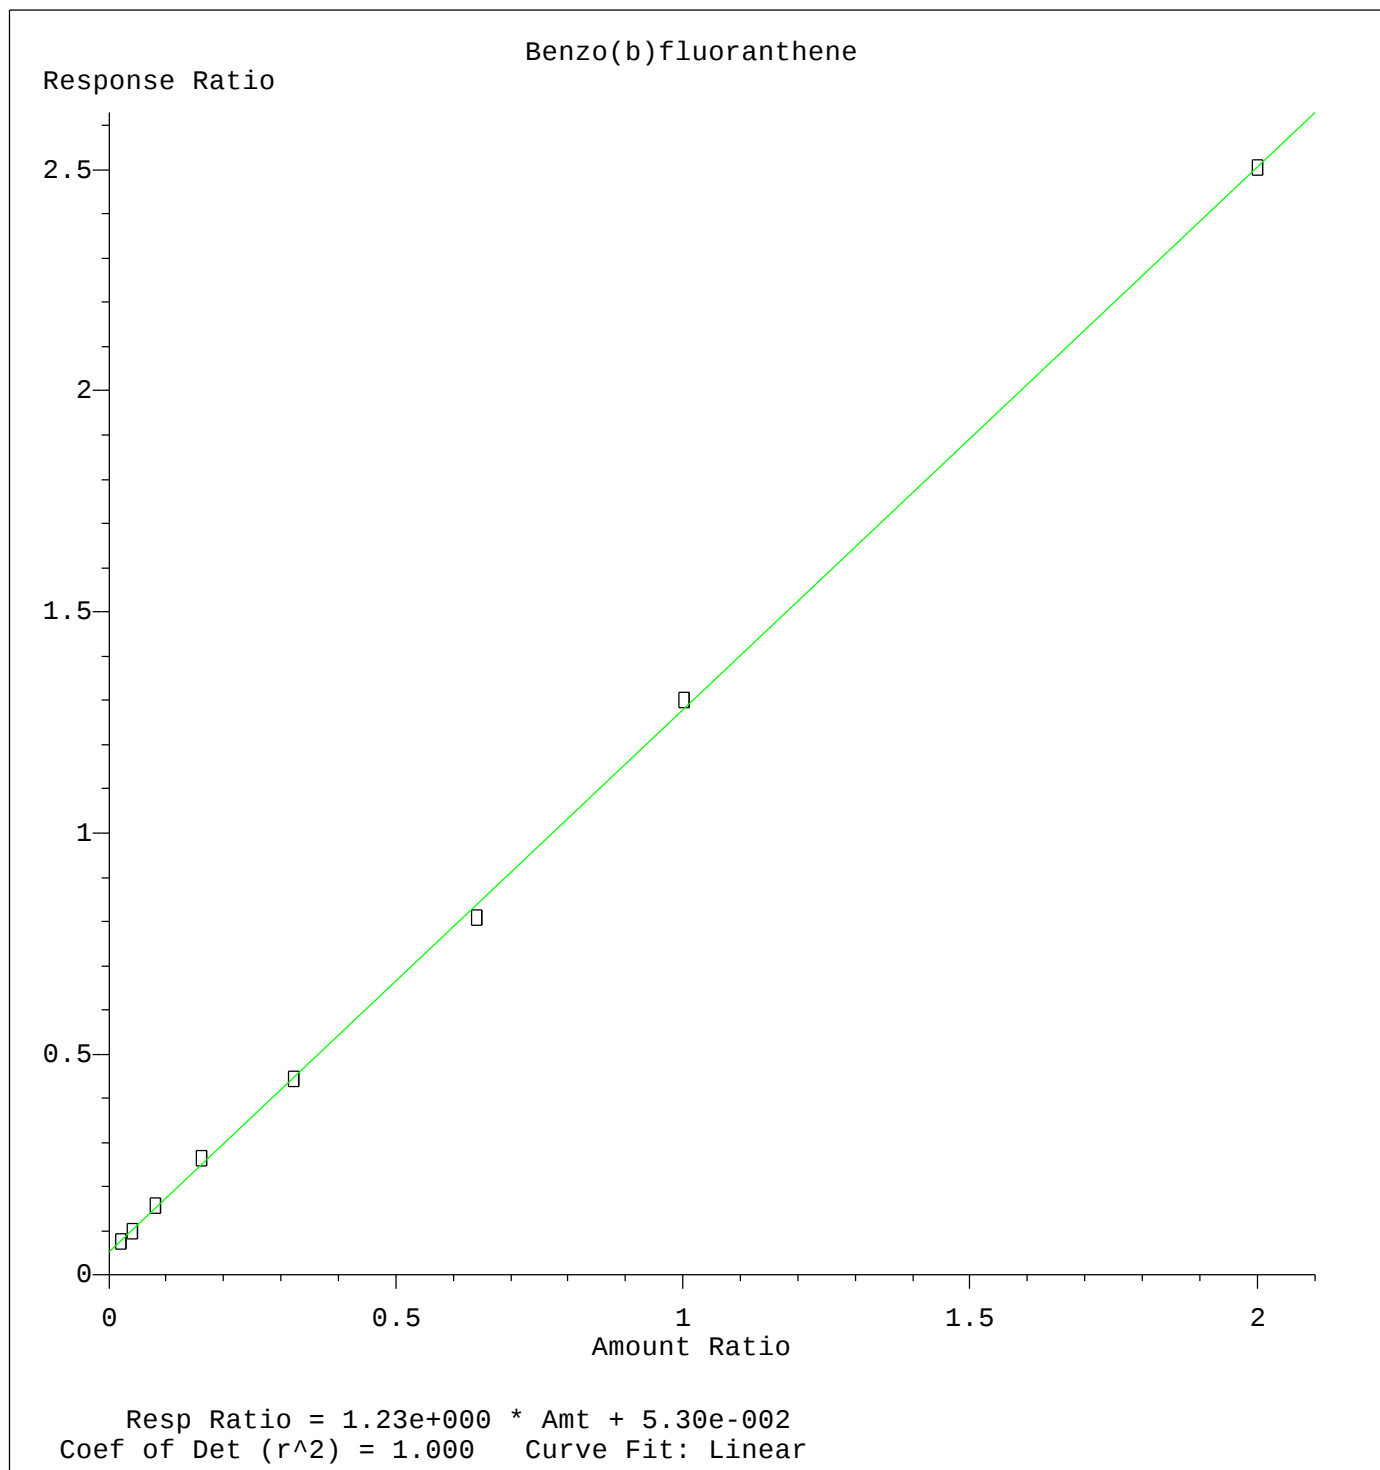

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016

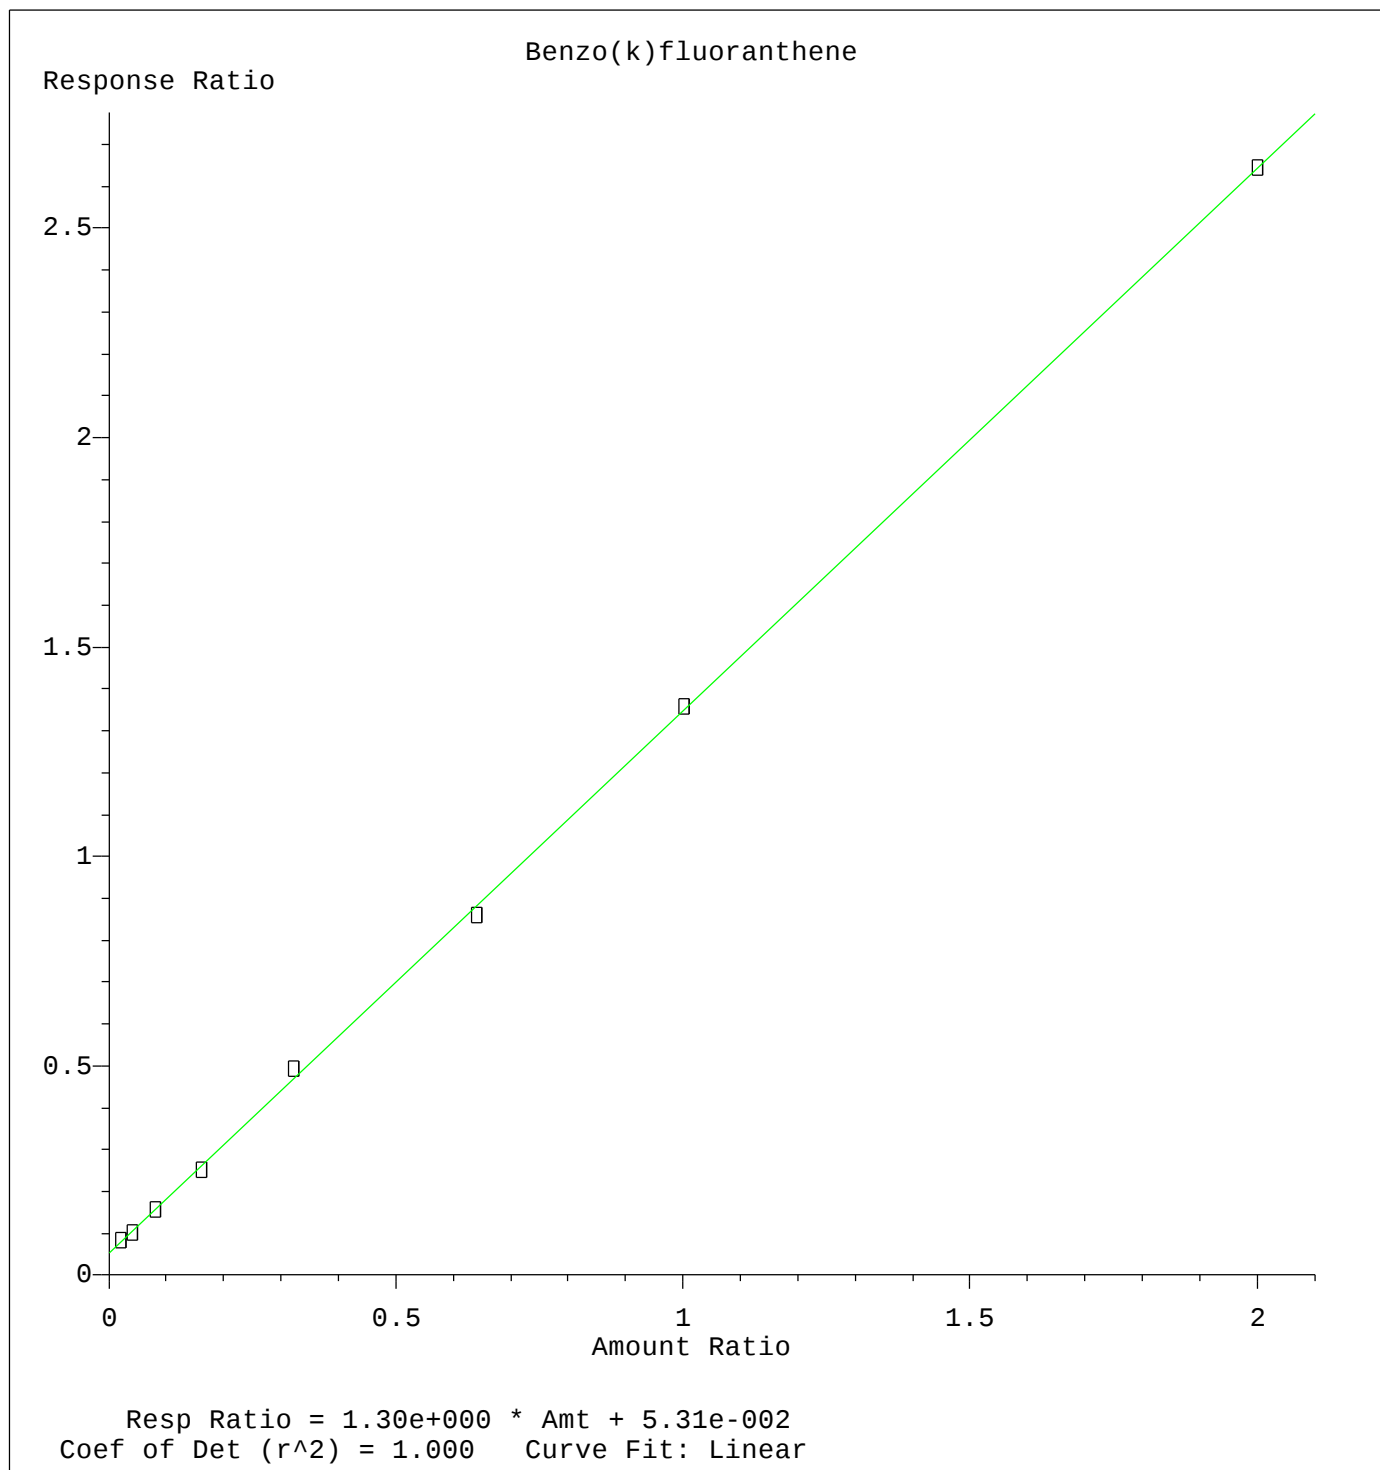

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Calibration Table Last Updated: Tue Nov 08 16:27:22 2016