


Data Path : Z:\HPCHEM1\BNA E\DATA\BE110816\
 Data File : BE092500.D
 Acq On : 8 Nov 2016 9:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 08 16:27:22 2016

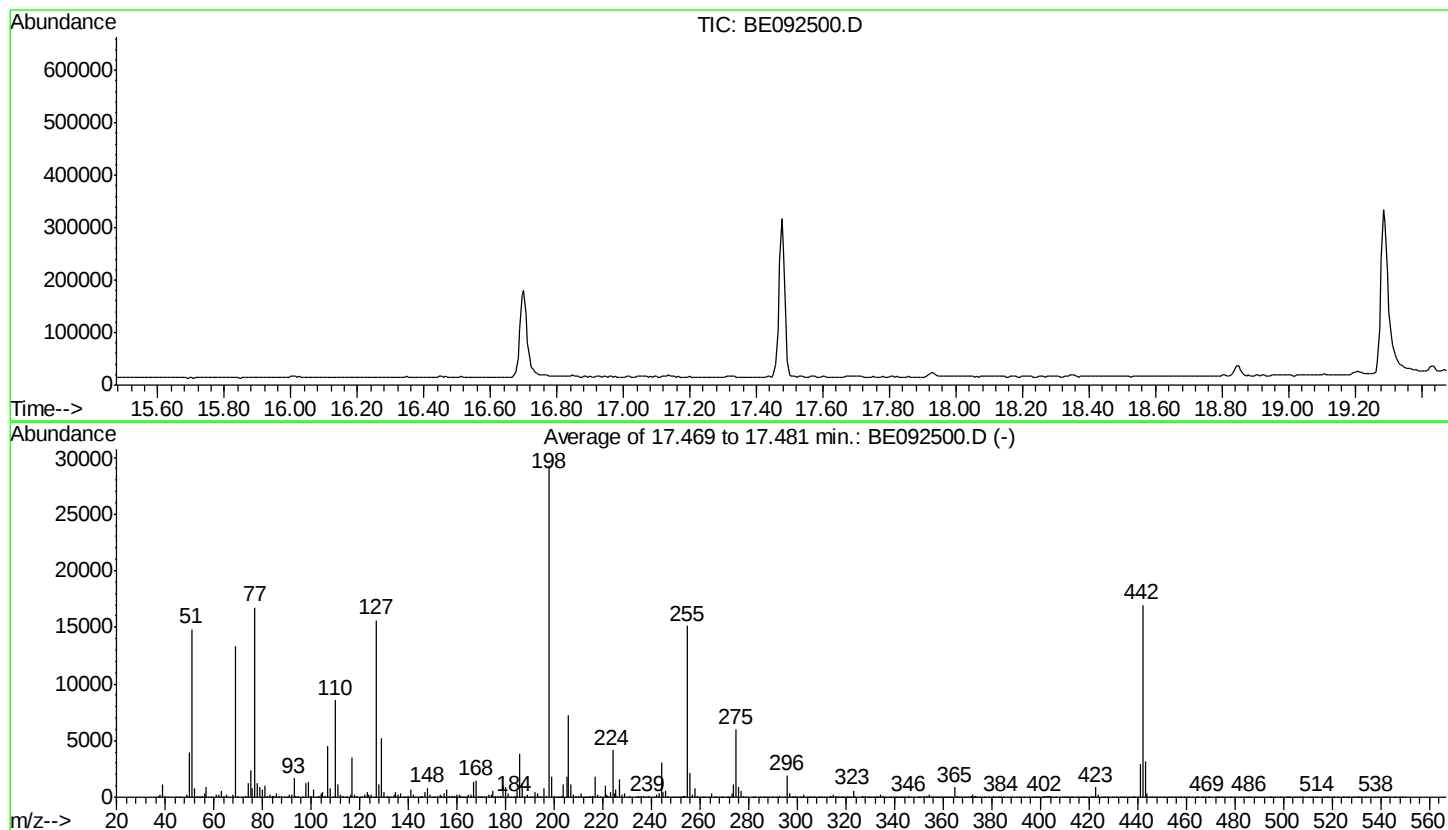

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	14860	PASS
68	69	0.00	2	1.7	221	PASS
69	198	0.00	100	45.5	13328	PASS
70	69	0.00	2	1.0	134	PASS
127	198	10	80	53.4	15633	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29272	PASS
199	198	5	9	6.2	1805	PASS
275	198	10	60	20.3	5951	PASS
365	198	1	100	3.0	891	PASS
441	442	0.01	24	17.1	2905	PASS
442	198	50	100	57.9	16954	PASS
443	442	15	24	18.5	3144	PASS