




Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:00:57 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

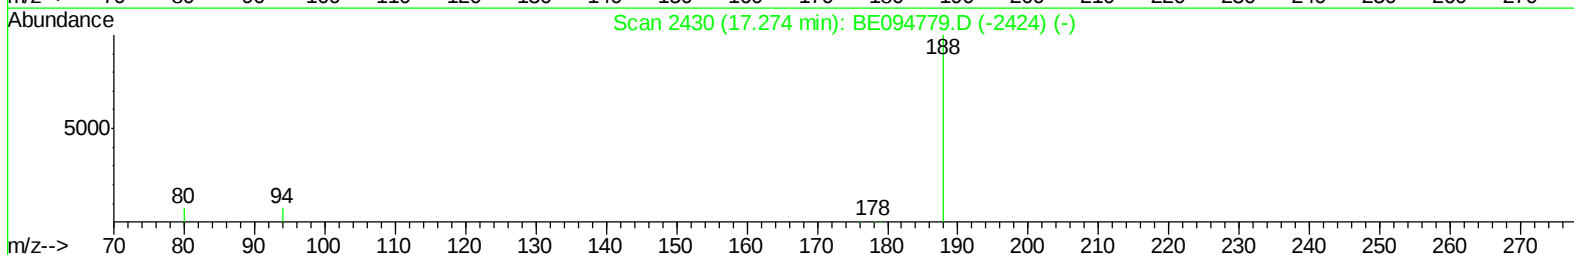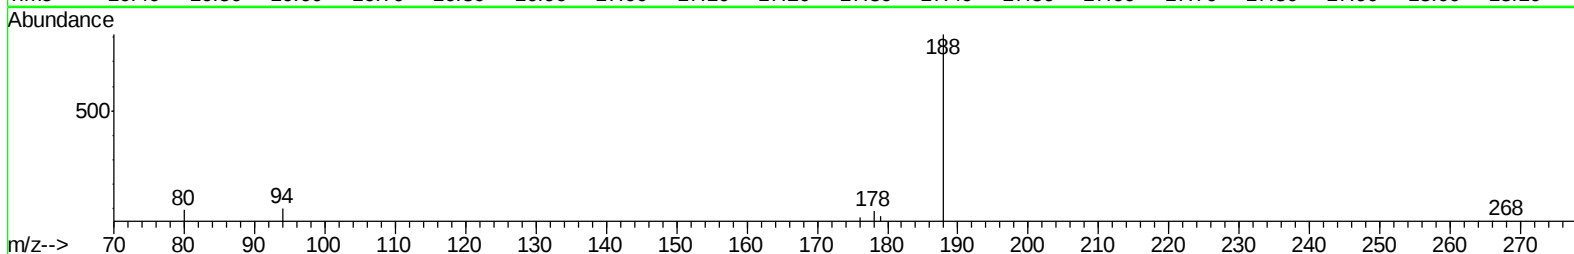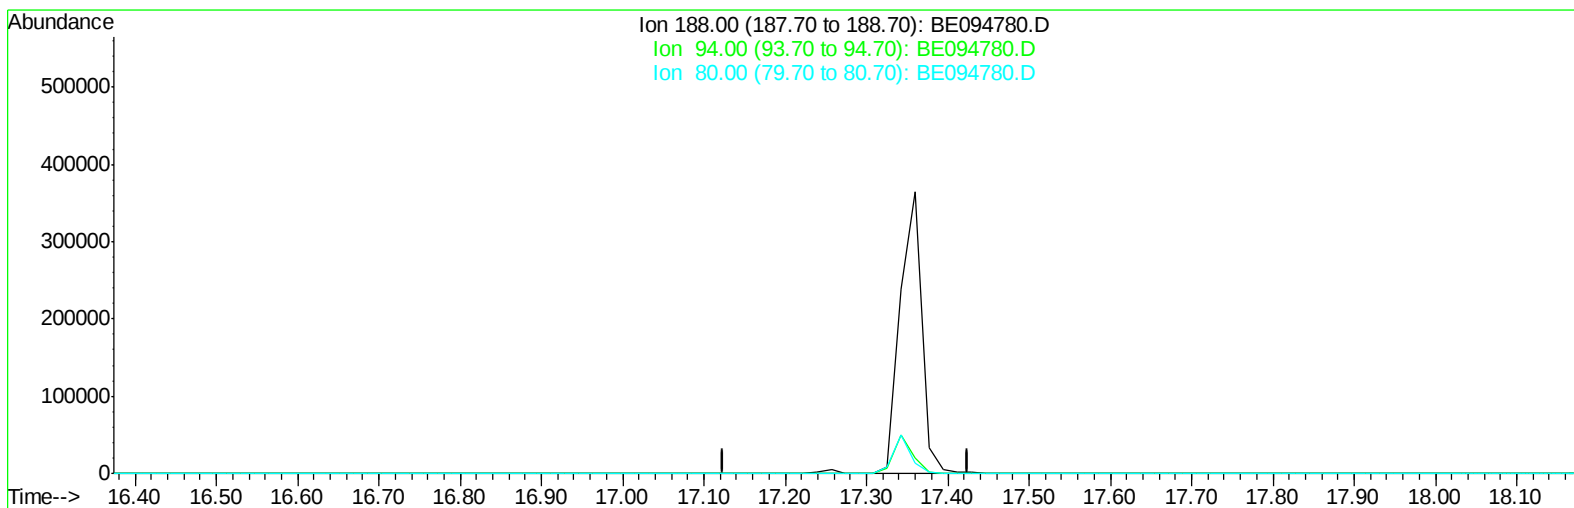

TIC: BE094780.D

(10) Phenanthrene-d10 (I)

17.275min (-17.275) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:00:57 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

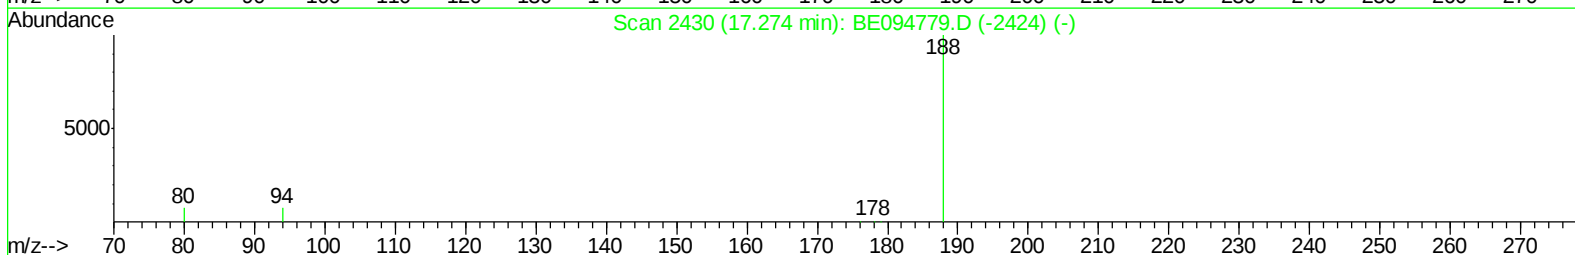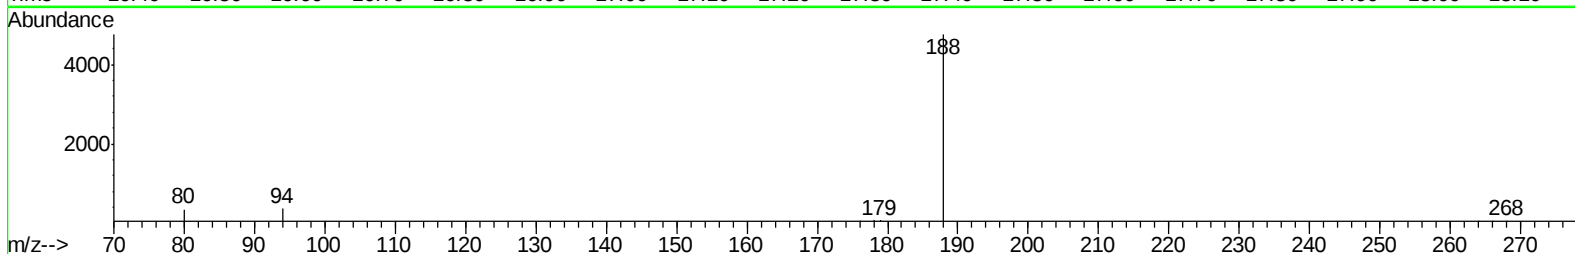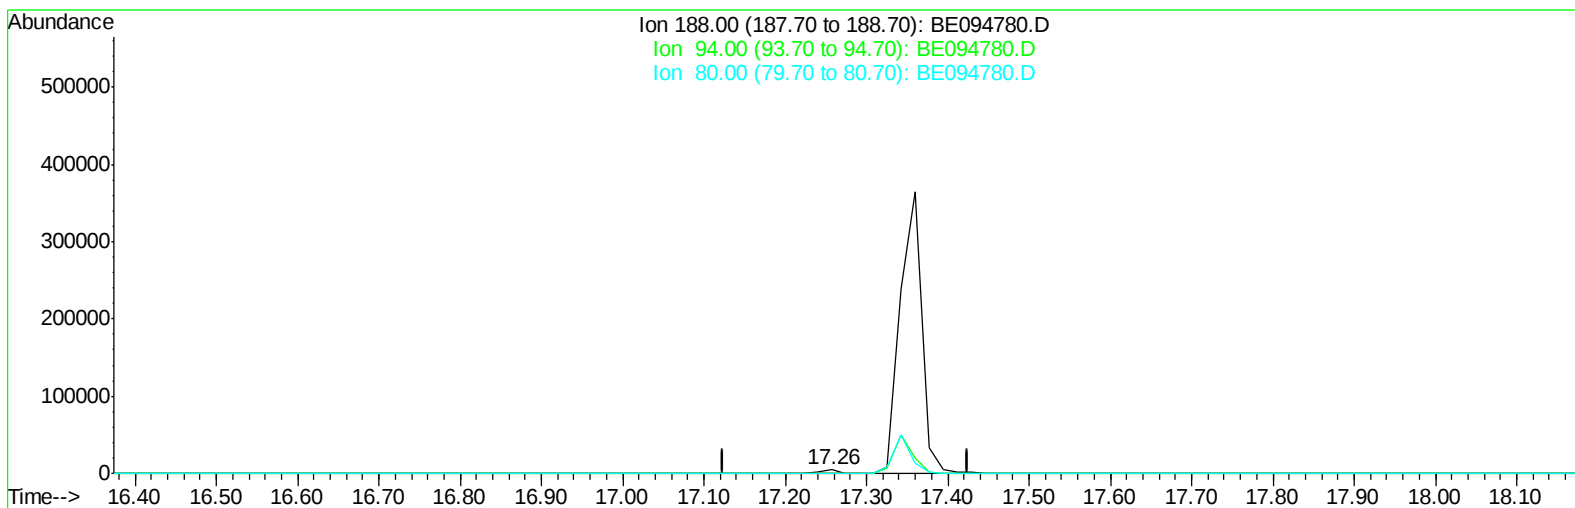

TIC: BE094780.D

(10) Phenanthrene-d10 (I)

17.257min (-0.019) 0.40ng/ul m

response 7368

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.77#
80.00	11.80	7.31#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:18:20 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

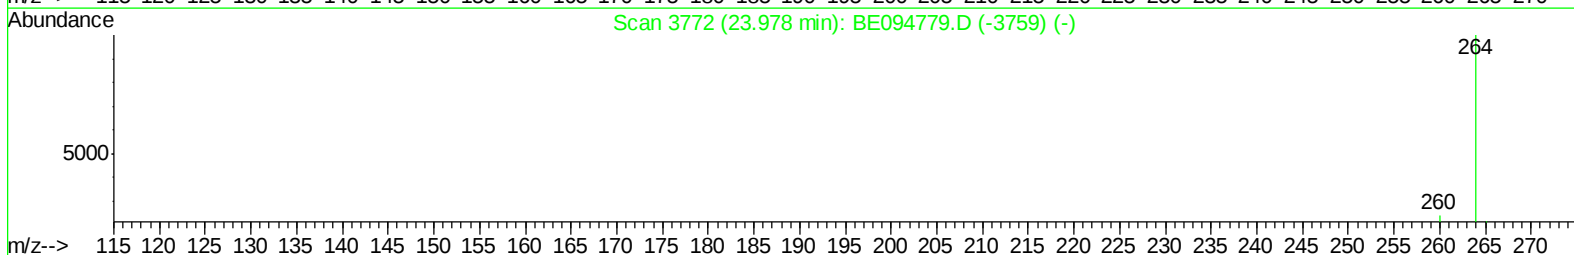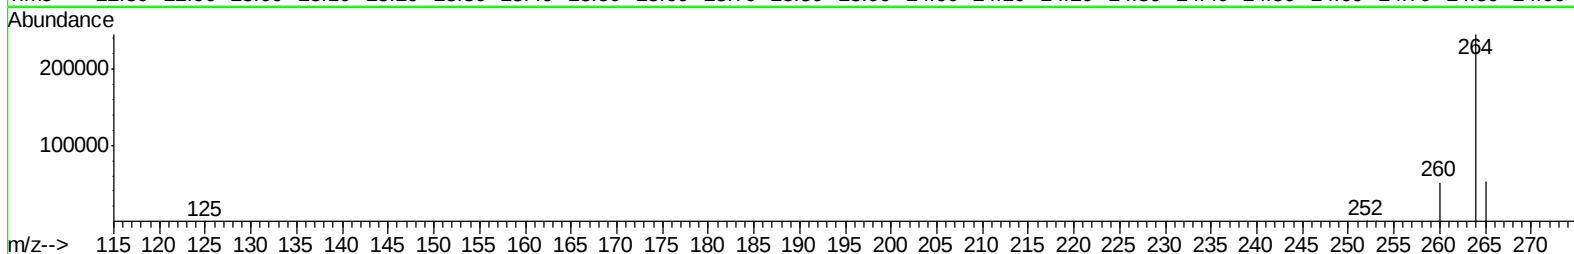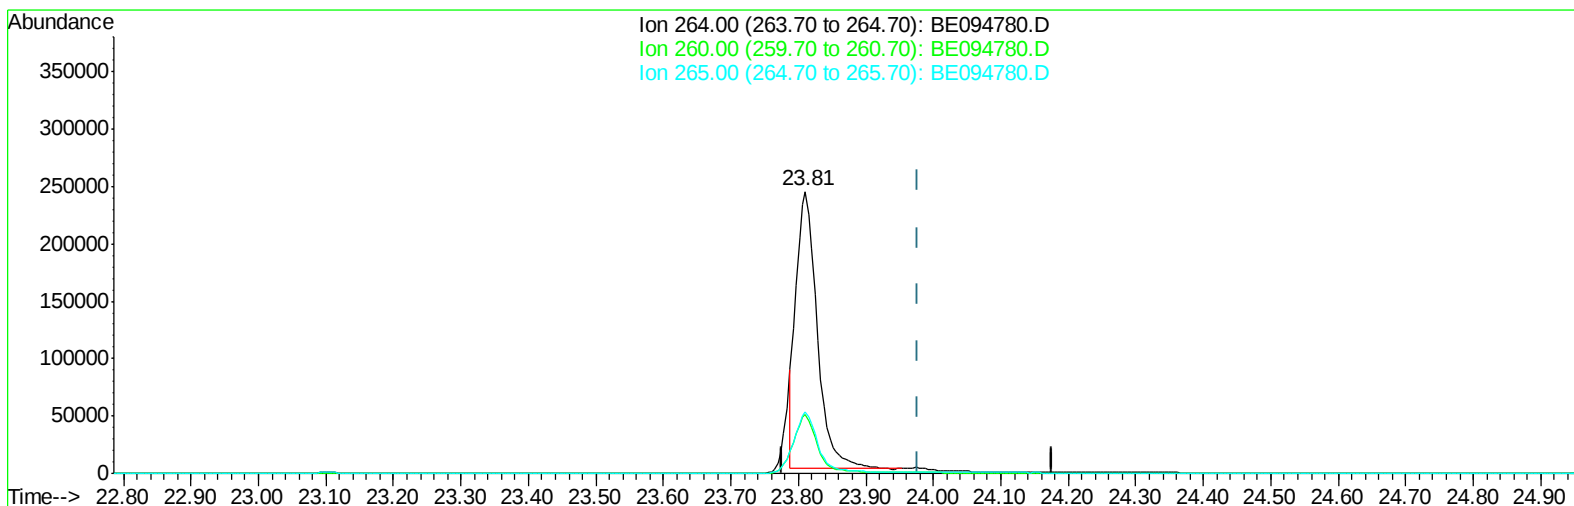

TIC: BE094780.D

(20) Perylene-d12 (I)

23.810min (-0.167) 0.40ng/ul

response 523502

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.76#
265.00	103.50	21.62#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:18:20 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

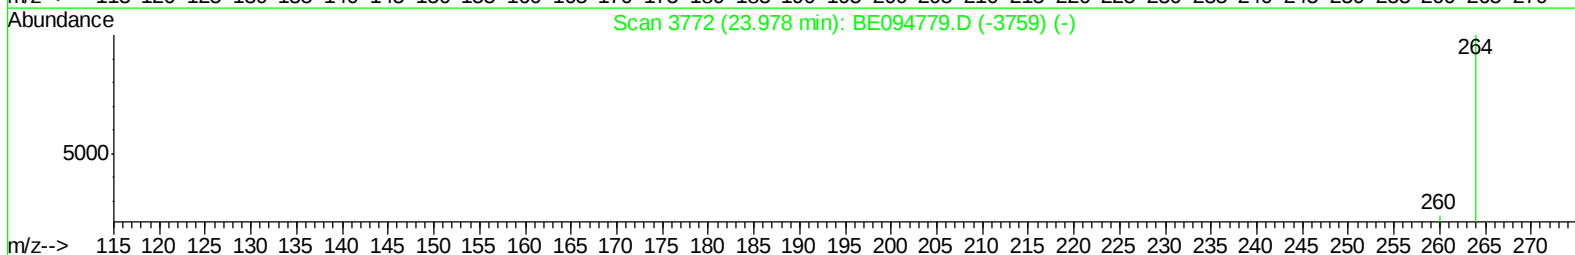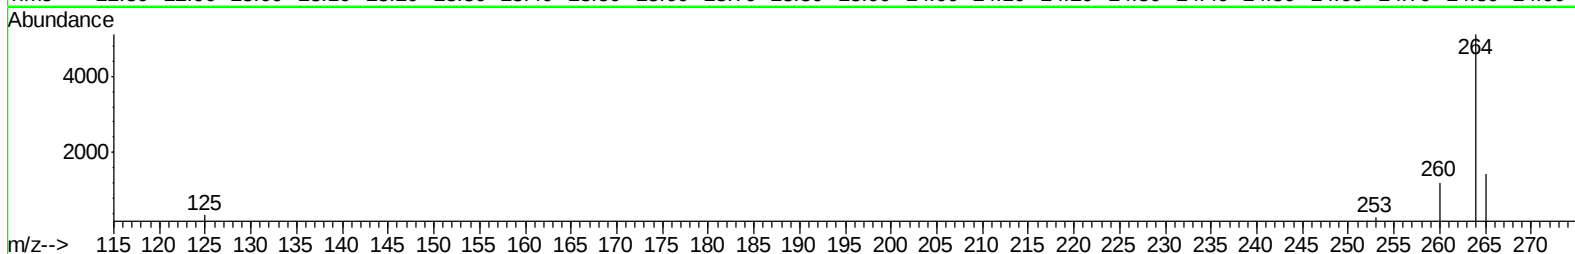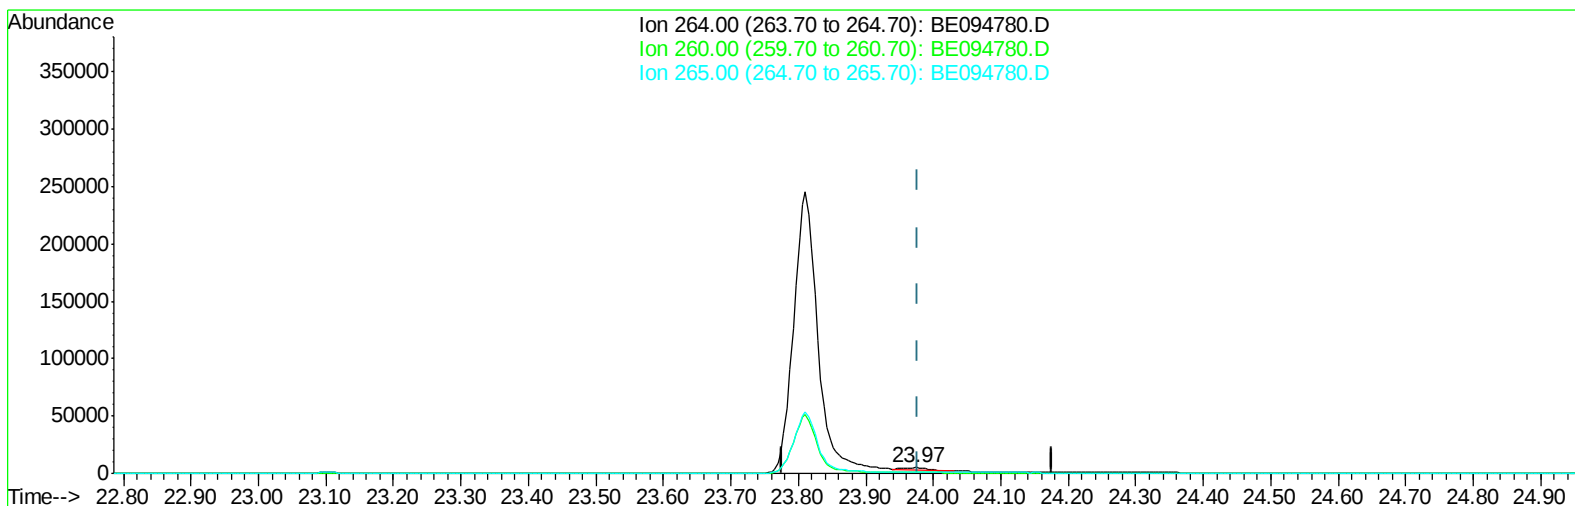

TIC: BE094780.D

(20) Perylene-d12 (I)

23.974min (-0.003) 0.40ng/ul m

response 4234

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.86#
265.00	103.50	28.29#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:19:45 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	950	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	5790	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	3529	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	7368m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	6782	0.40	ng/ul	0.00
20) Perylene-d12	23.97	264	4234m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	3605	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	8893	0.41	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE110817\
Data File : BE094780.D
Acq On : 8 Nov 2017 11:17
Operator : SJ/JU
Sample : I5825-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-3-101117

Manual Integrations
APPROVED

Sohil
11/8/2017 3:43:40 PM

Quant Time: Nov 08 15:19:45 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 15:01:00 2017
Response via : Initial Calibration

