

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101553.D
 Acq On : 8 Nov 2024 15:44
 Operator : RC/JU
 Sample : P4739-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-G2

Quant Time: Nov 08 15:28:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.555	152	37151	20.000	ng	0.00
21) Naphthalene-d8	10.323	136	149942	20.000	ng	0.00
39) Acenaphthene-d10	14.165	164	100255	20.000	ng	0.00
64) Phenanthrene-d10	16.903	188	260781	20.000	ng	0.00
76) Chrysene-d12	21.063	240	352844	20.000	ng	-0.01
86) Perylene-d12	23.348	264	472912	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.311	112	335295	159.581	ng	0.00
7) Phenol-d6	6.938	99	403910	140.210	ng	0.00
23) Nitrobenzene-d5	8.766	82	238937	100.655	ng	0.00
42) 2,4,6-Tribromophenol	15.675	330	322975	171.204	ng	0.00
45) 2-Fluorobiphenyl	12.790	172	603572	98.301	ng	0.00
79) Terphenyl-d14	19.500	244	1854912	116.368	ng	0.00
Target Compounds						
32) Benzoic acid	9.876	122	12	6.841	ng	Qvalue # 21

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101553.D
Acq On : 8 Nov 2024 15:44
Operator : RC/JU
Sample : P4739-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G2


Quant Time: Nov 08 15:28:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

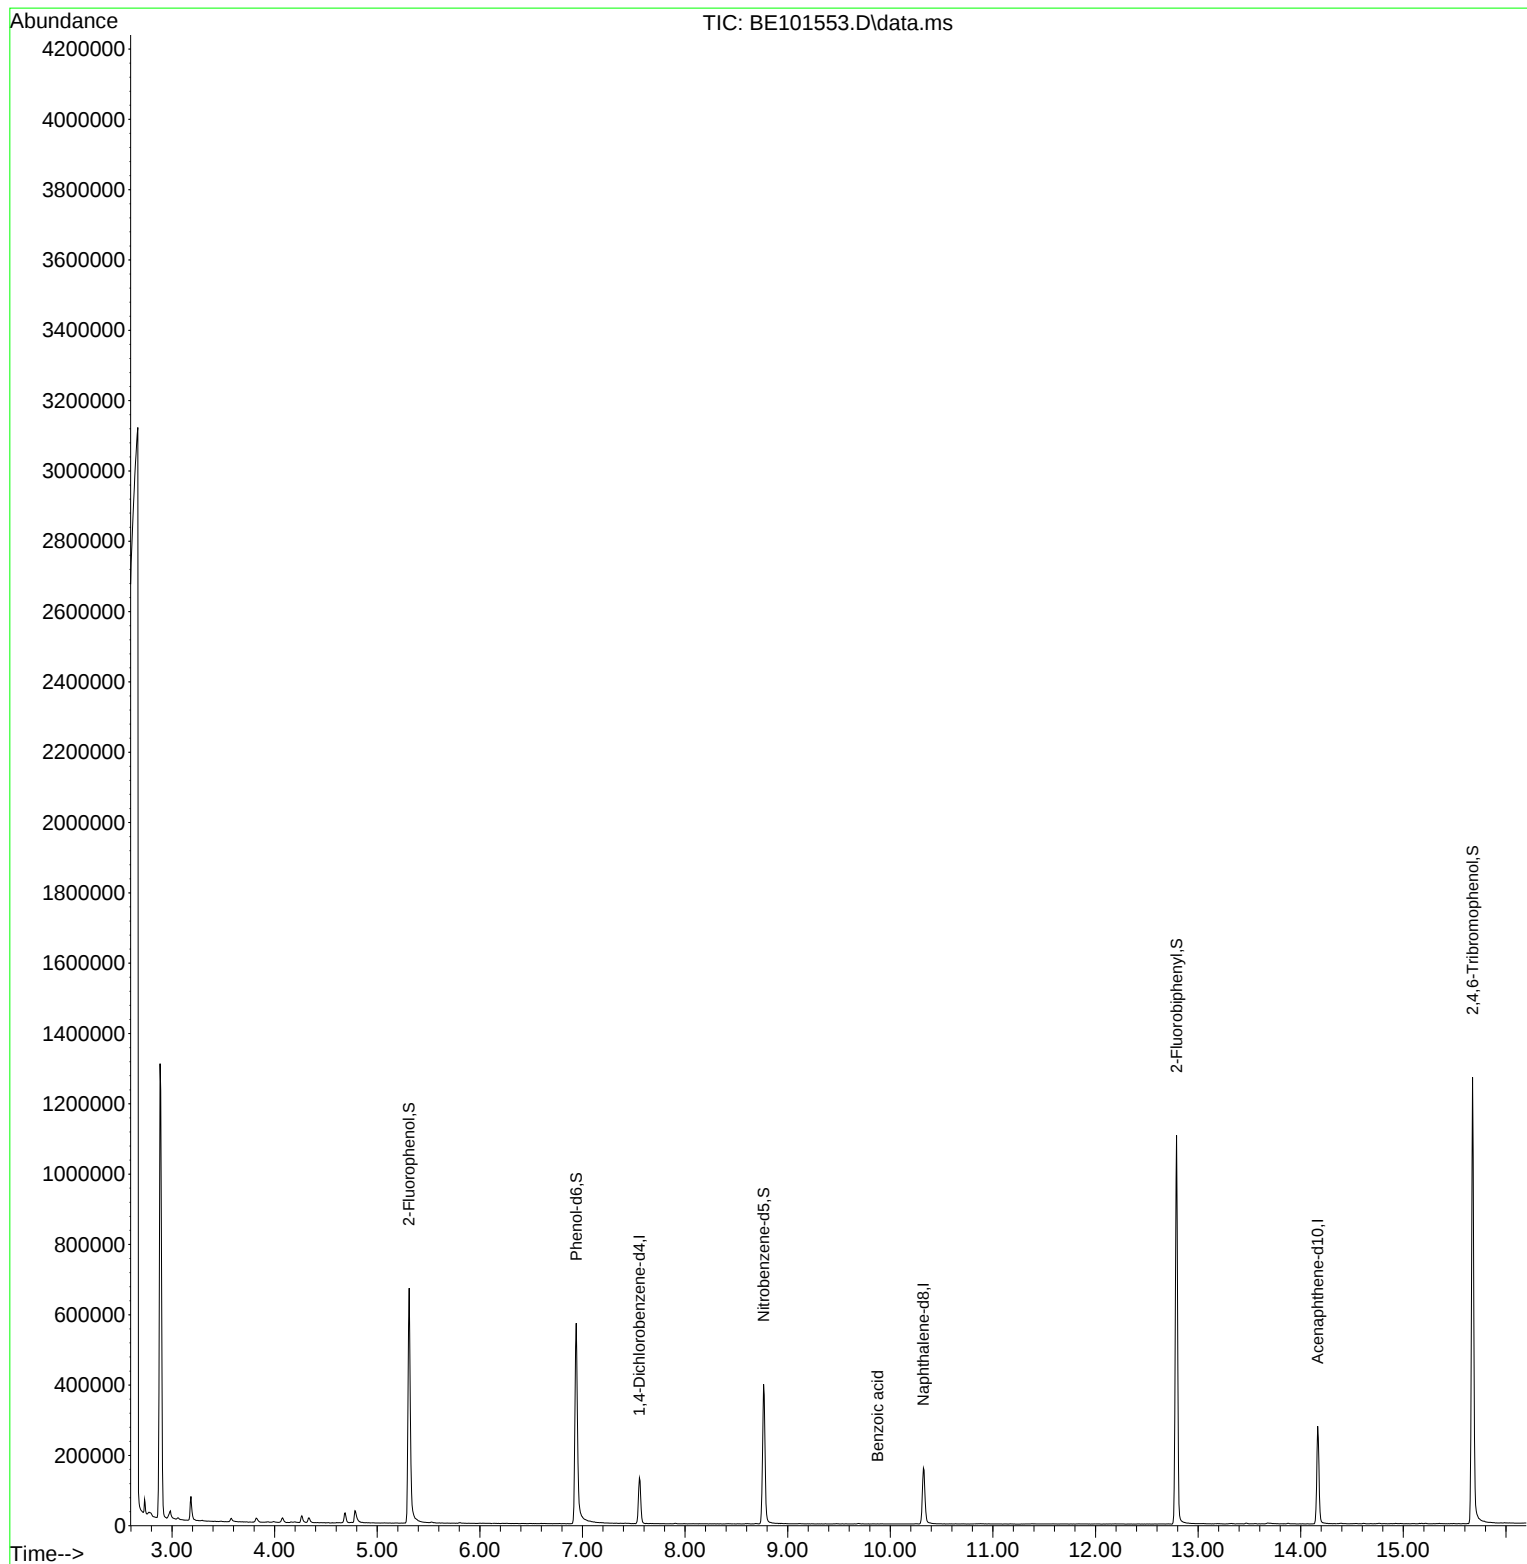

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101553.D
Acq On : 8 Nov 2024 15:44
Operator : RC/JU
Sample : P4739-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G2

Quant Time: Nov 08 15:28:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration



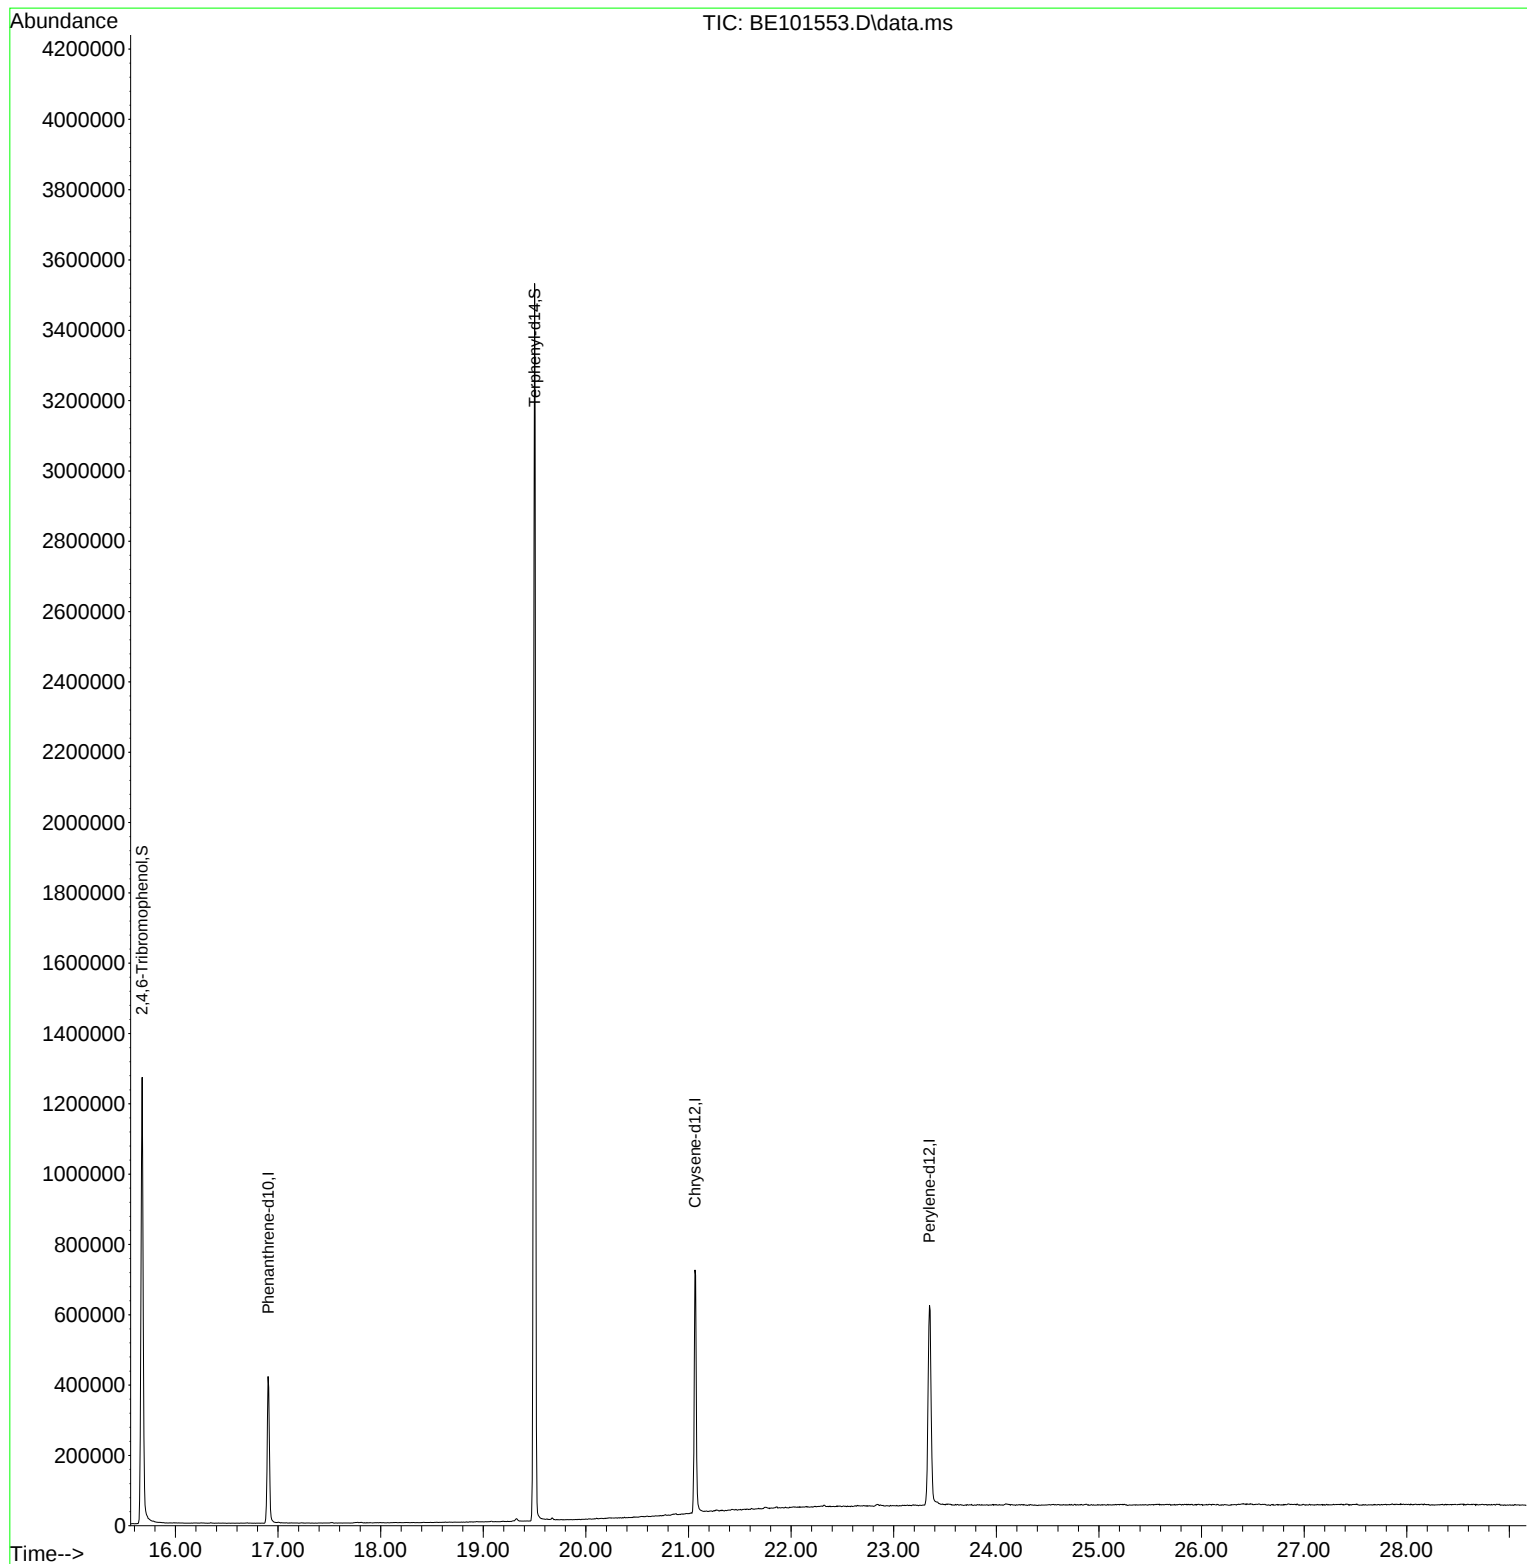




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.555 min Scan# 84
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44




Instrument :
BNA_E
ClientSampleId :
BP-G2

Tgt Ion:152 Resp: 37151
Ion Ratio Lower Upper
152 100
150 158.9 126.3 189.5
115 59.1 45.0 67.4

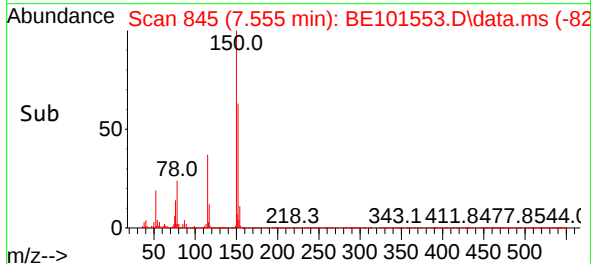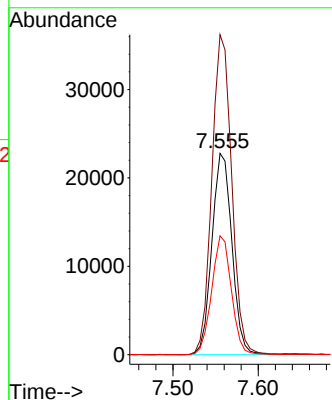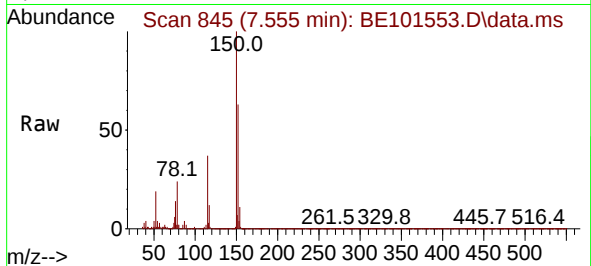

#5
2-Fluorophenol
Concen: 159.581 ng
RT: 5.311 min Scan# 463
Delta R.T. -0.002 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Tgt Ion:112 Resp: 335295
Ion Ratio Lower Upper
112 100
64 54.5 43.2 64.8
63 27.6 21.8 32.6


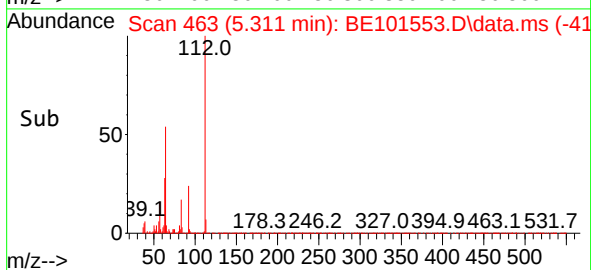
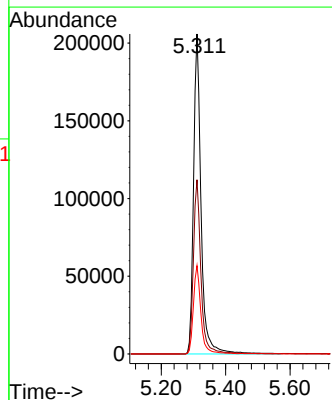
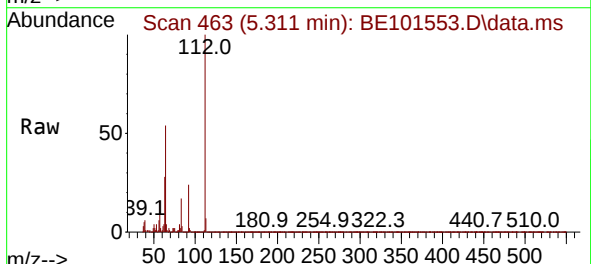




#7
Phenol-d6
Concen: 140.210 ng
RT: 6.938 min Scan# 741
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44




Instrument :
BNA_E
ClientSampleId :
BP-G2


Tgt Ion: 99 Resp: 403910
Ion Ratio Lower Upper
99 100
42 16.5 12.5 18.7
71 30.6 24.2 36.2

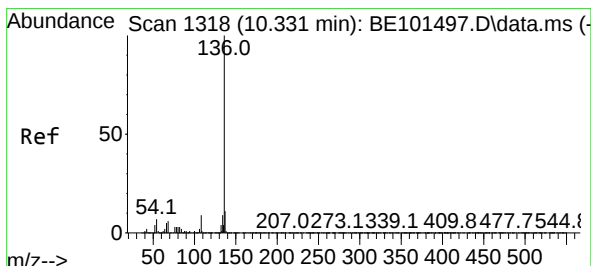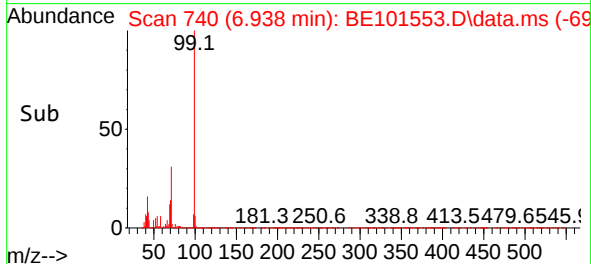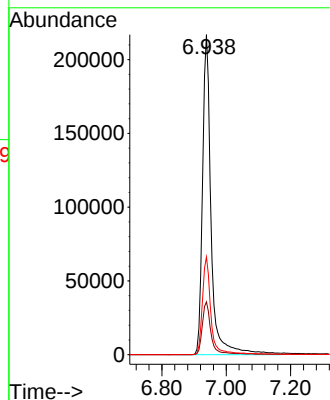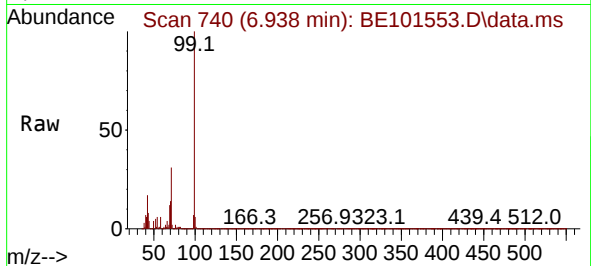

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.323 min Scan# 1316
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Tgt Ion: 136 Resp: 149942
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 7.7 5.6 8.4
68 6.4 4.8 7.2


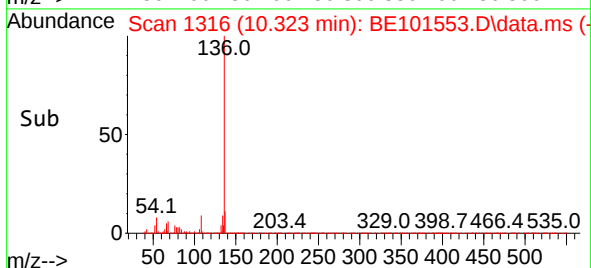
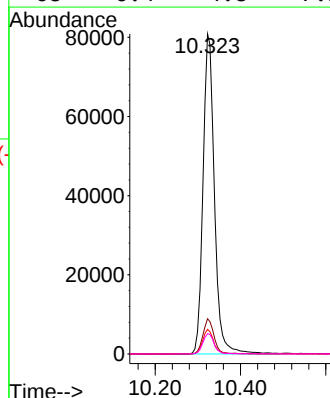
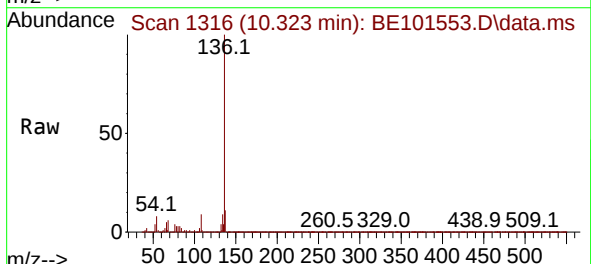


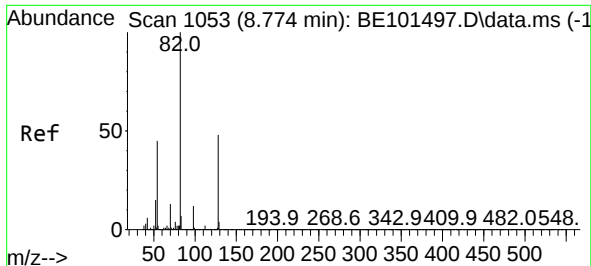

#23
Nitrobenzene-d5
Concen: 100.655 ng
RT: 8.766 min Scan# 1051
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44




Instrument :
BNA_E
ClientSampleId :
BP-G2


Tgt Ion: 82 Resp: 238937
Ion Ratio Lower Upper
82 100
128 47.6 38.6 58.0
54 47.4 36.3 54.5

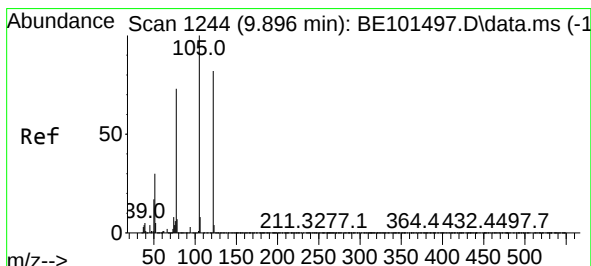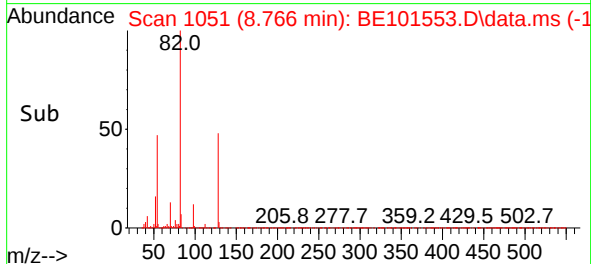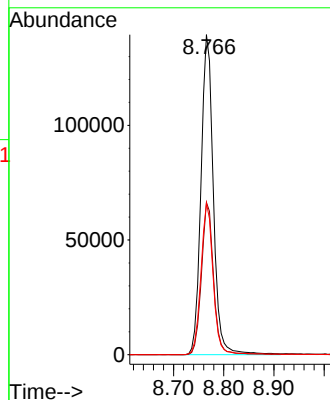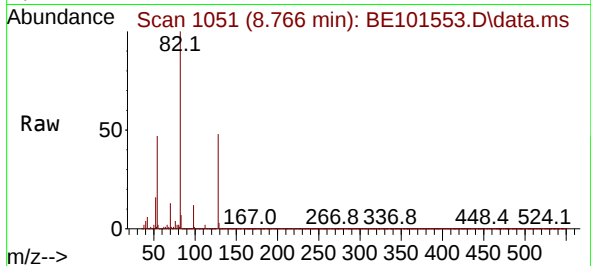

#32
Benzoic acid
Concen: 6.841 ng
RT: 9.876 min Scan# 1240
Delta R.T. -0.020 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Tgt Ion: 122 Resp: 12
Ion Ratio Lower Upper
122 100
105 37.5 100.6 140.6#
77 168.8 68.6 108.6#


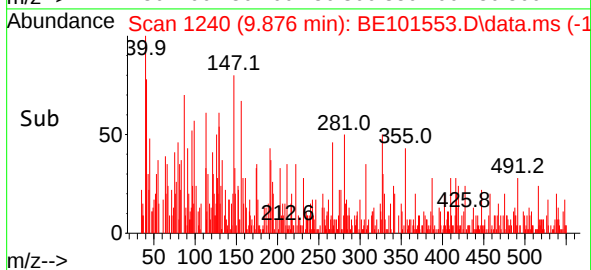
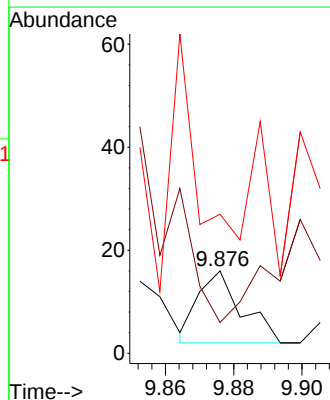
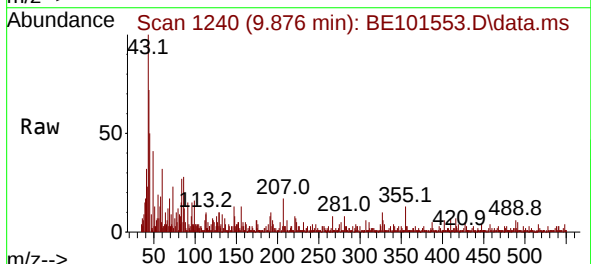


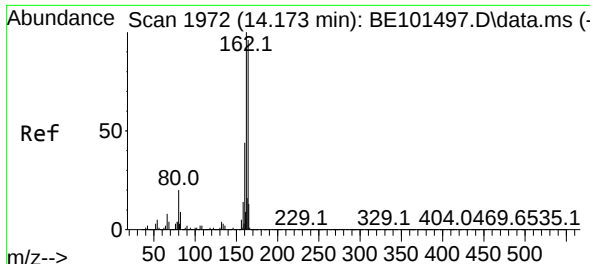

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.165 min Scan# 1972
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44




Instrument :
BNA_E
ClientSampleId :
BP-G2


Tgt Ion:164 Resp: 100255
Ion Ratio Lower Upper
164 100
162 102.9 83.7 125.5
160 45.0 37.1 55.7

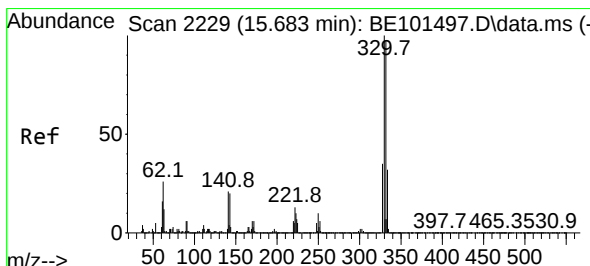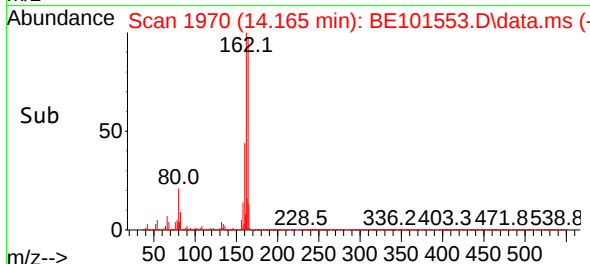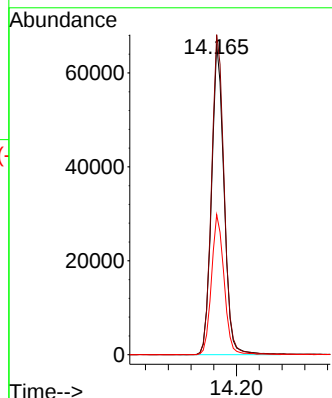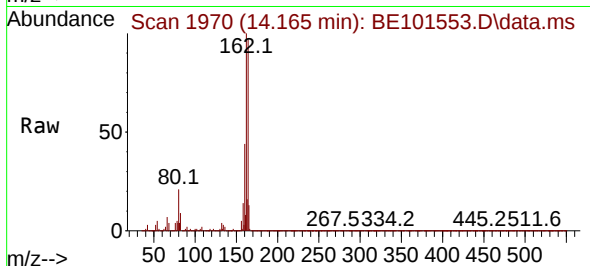

#42
2,4,6-Tribromophenol
Concen: 171.204 ng
RT: 15.675 min Scan# 2227
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Tgt Ion:330 Resp: 322975
Ion Ratio Lower Upper
330 100
332 97.6 77.7 116.5
141 22.0 17.0 25.4


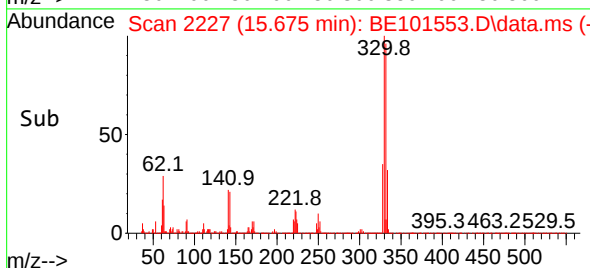
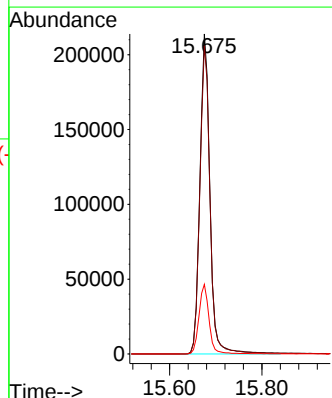
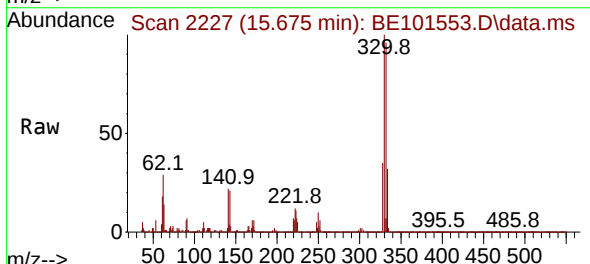


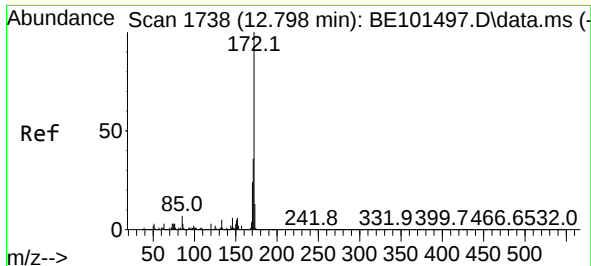

#45
2-Fluorobiphenyl
Concen: 98.301 ng
RT: 12.790 min Scan# 1736
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44




Instrument :
BNA_E
ClientSampleId :
BP-G2


Tgt Ion:172 Resp: 603572
Ion Ratio Lower Upper
172 100
171 35.1 28.6 43.0
170 23.4 18.9 28.3

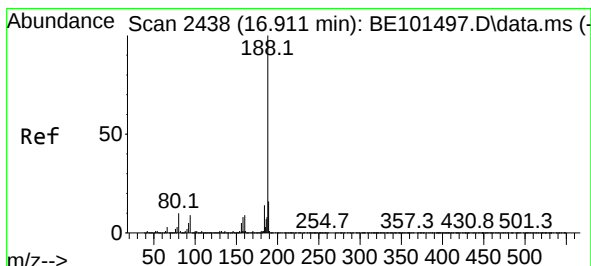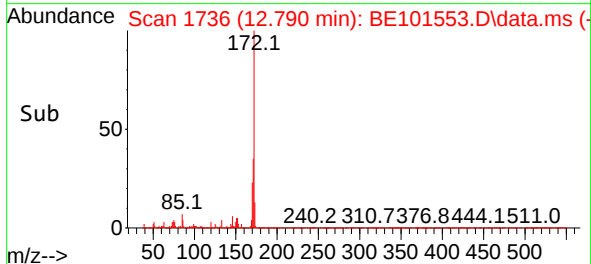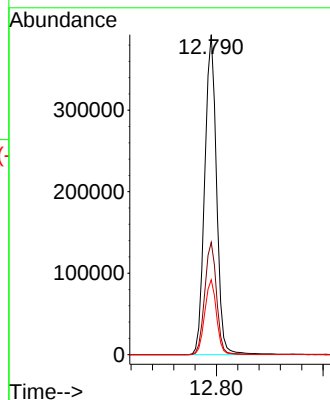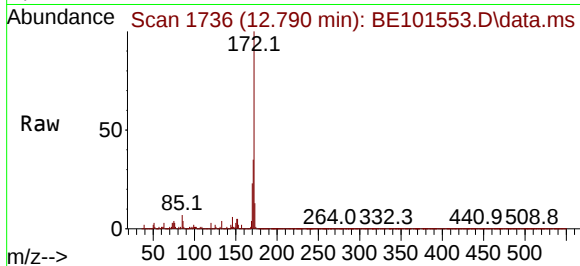

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.903 min Scan# 2436
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Tgt Ion:188 Resp: 260781
Ion Ratio Lower Upper
188 100
94 9.9 7.4 11.2
80 10.7 8.0 12.0

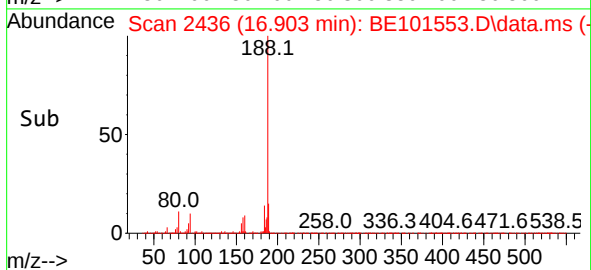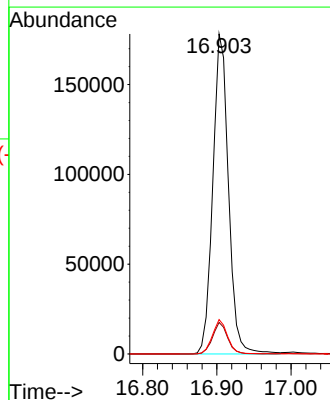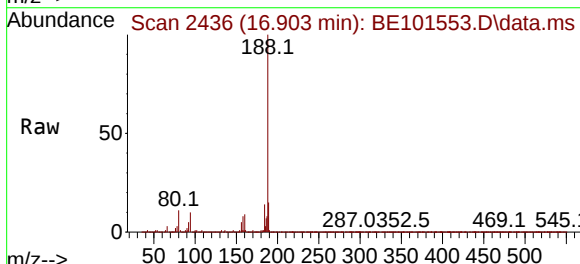

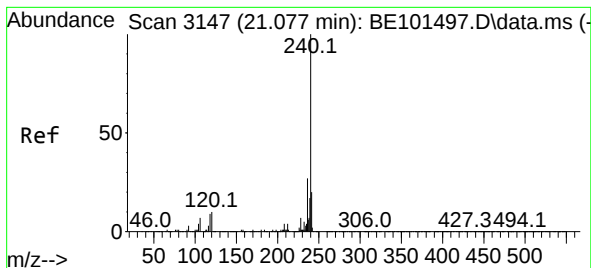

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.063 min Scan# 31

Delta R.T. -0.014 min

Lab File: BE101553.D

Acq: 8 Nov 2024 15:44

Instrument :

BNA_E

ClientSampleId :

BP-G2





Tgt Ion:240 Resp: 352844

Ion Ratio Lower Upper

240 100

120 11.6 8.2 12.4

236 26.6 21.4 32.2

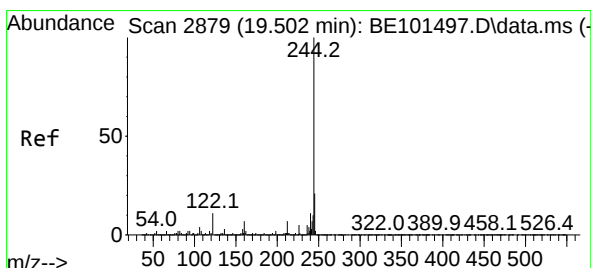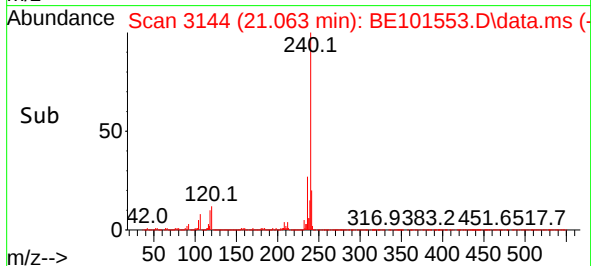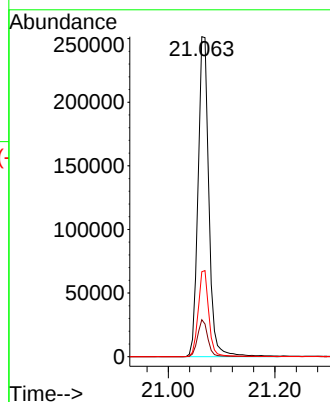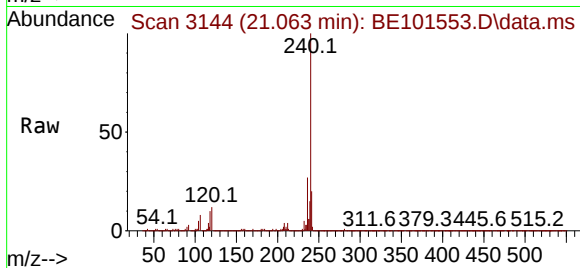

#79

Terphenyl-d14

Concen: 116.368 ng

RT: 19.500 min Scan# 2878

Delta R.T. -0.002 min

Lab File: BE101553.D

Acq: 8 Nov 2024 15:44




Tgt Ion:244 Resp: 1854912


Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.8

122 10.7 8.4 12.6

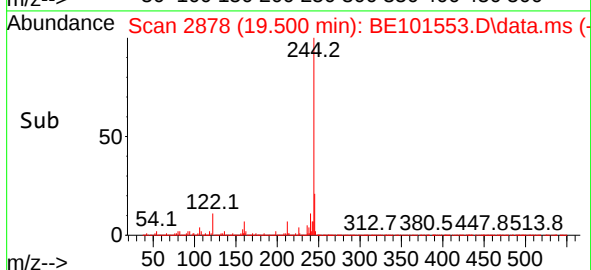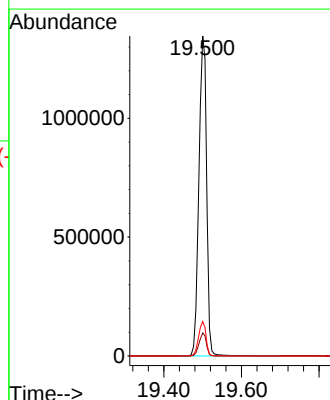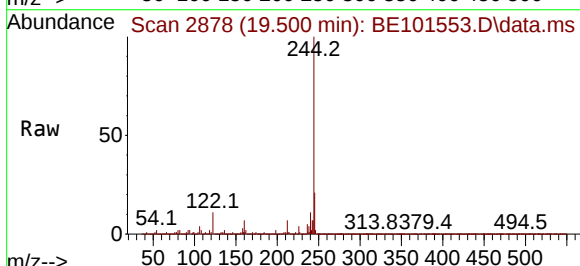

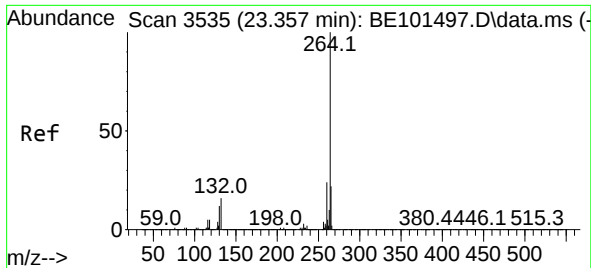

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.348 min Scan# 31
Delta R.T. -0.008 min
Lab File: BE101553.D
Acq: 8 Nov 2024 15:44

Instrument :
BNA_E
ClientSampleId :
BP-G2

Tgt Ion:264 Resp: 472912

Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.4	29.2
265	21.7	17.4	26.2

