

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101548.D
 Acq On : 8 Nov 2024 12:45
 Operator : RC/JU
 Sample : P4701-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F4

Quant Time: Nov 08 12:30:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.555	152	44068	20.000	ng	0.00
21) Naphthalene-d8	10.322	136	181062	20.000	ng	0.00
39) Acenaphthene-d10	14.165	164	105245	20.000	ng	0.00
64) Phenanthrene-d10	16.903	188	292283	20.000	ng	0.00
76) Chrysene-d12	21.069	240	353318	20.000	ng	0.00
86) Perylene-d12	23.348	264	122638	20.000	ng	# 0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.311	112	379381	152.222	ng	0.00
7) Phenol-d6	6.938	99	424051	124.096	ng	0.00
23) Nitrobenzene-d5	8.765	82	296773	103.532	ng	0.00
42) 2,4,6-Tribromophenol	15.675	330	358925	181.239	ng	0.00
45) 2-Fluorobiphenyl	12.790	172	737749	114.456	ng	0.00
79) Terphenyl-d14	19.500	244	1942665	121.709	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101548.D
Acq On : 8 Nov 2024 12:45
Operator : RC/JU
Sample : P4701-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F4

Quant Time: Nov 08 12:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

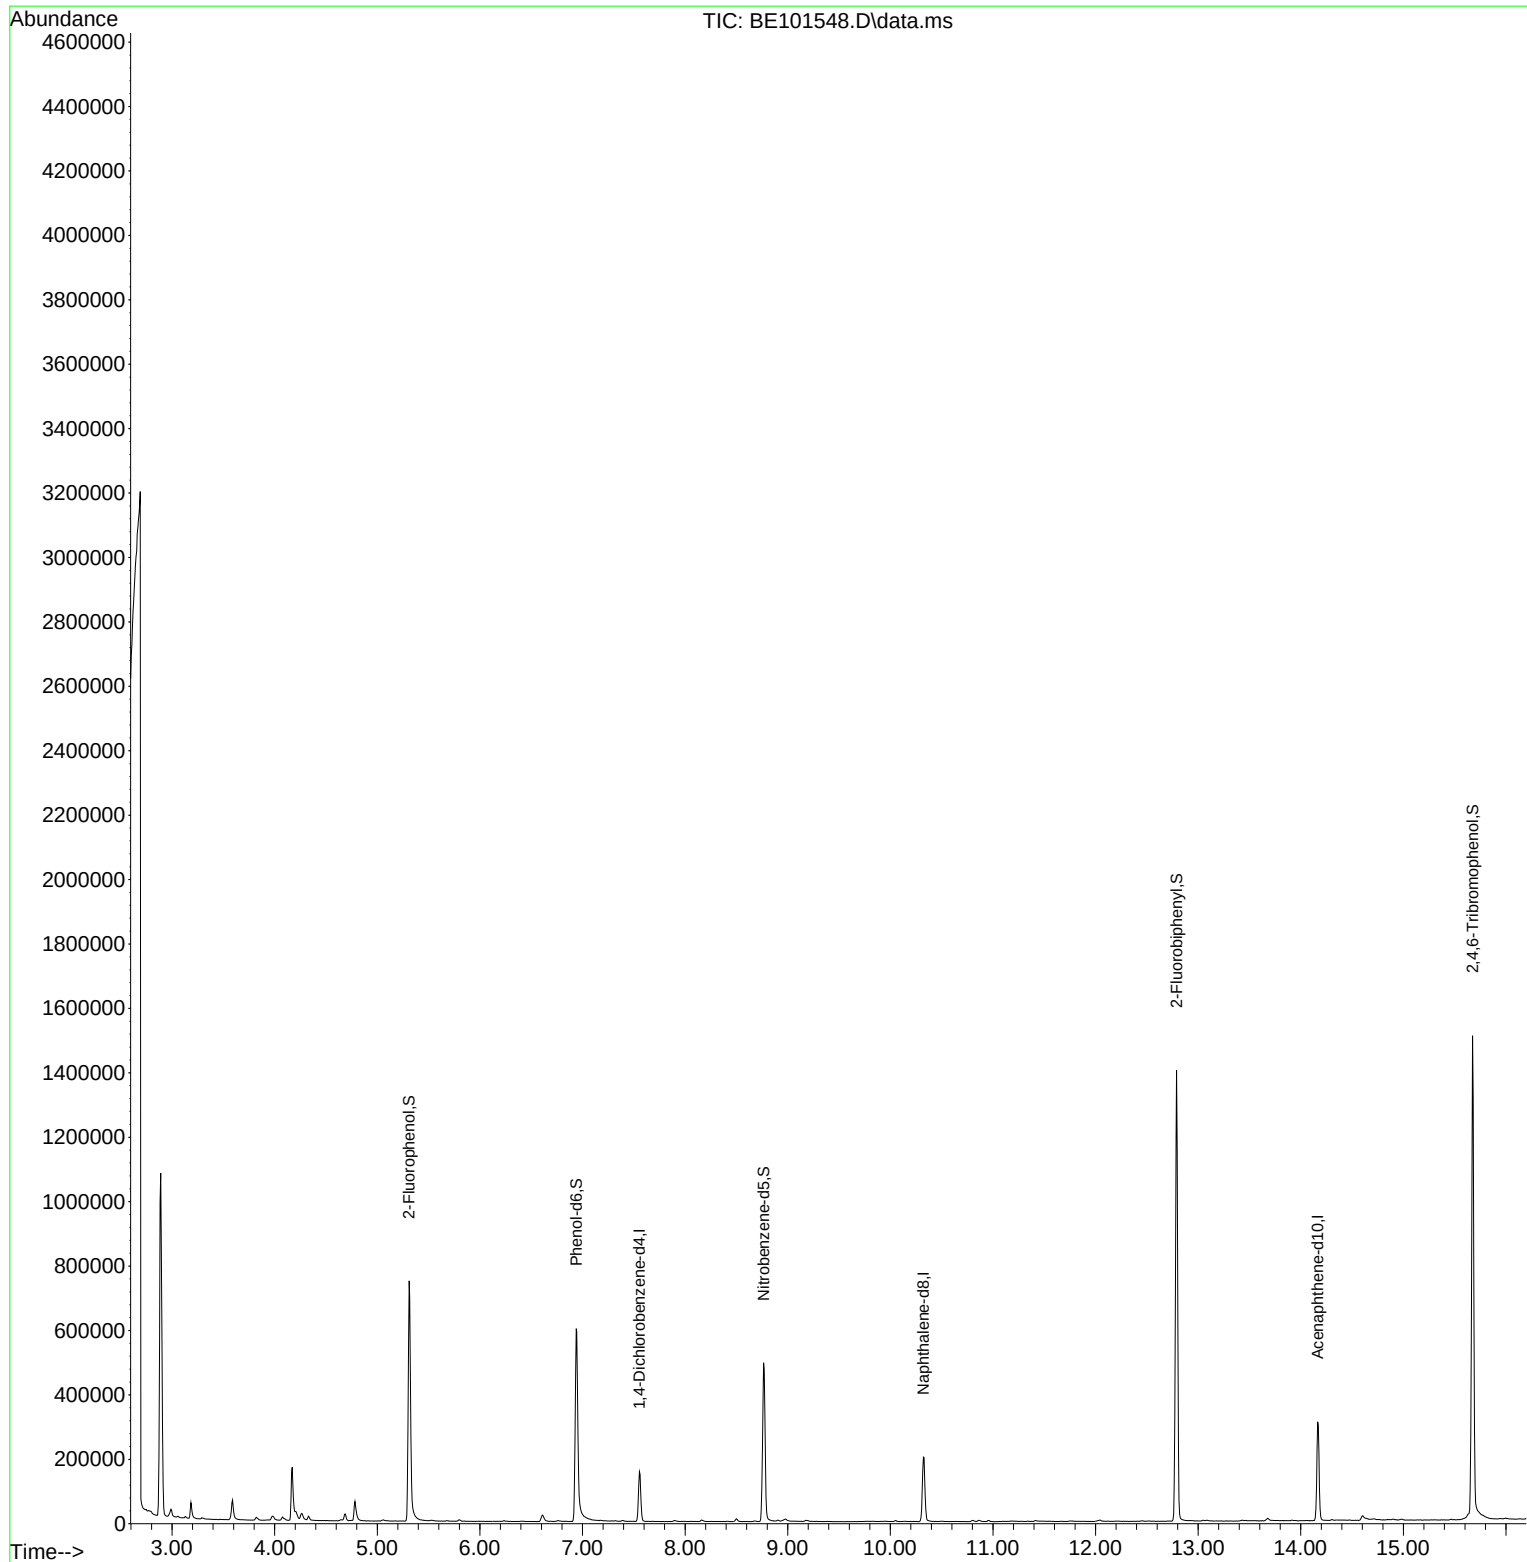

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101548.D
Acq On : 8 Nov 2024 12:45
Operator : RC/JU
Sample : P4701-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F4

Quant Time: Nov 08 12:30:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

