

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101550.D
Acq On : 8 Nov 2024 13:56
Operator : RC/JU
Sample : P4694-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-04

Quant Time: Nov 08 13:48:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	36100	20.000	ng	0.00
21) Naphthalene-d8	10.325	136	148758	20.000	ng	0.00
39) Acenaphthene-d10	14.168	164	102994	20.000	ng	0.00
64) Phenanthrene-d10	16.906	188	264891	20.000	ng	0.00
76) Chrysene-d12	21.066	240	363180	20.000	ng	-0.01
86) Perylene-d12	23.351	264	458354	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.308	112	318281	155.894	ng	0.00
7) Phenol-d6	6.941	99	375774	134.240	ng	0.00
23) Nitrobenzene-d5	8.768	82	258715	109.854	ng	0.00
42) 2,4,6-Tribromophenol	15.678	330	357131	184.275	ng	0.00
45) 2-Fluorobiphenyl	12.787	172	678682	107.594	ng	-0.01
79) Terphenyl-d14	19.503	244	1960302	119.479	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101550.D
Acq On : 8 Nov 2024 13:56
Operator : RC/JU
Sample : P4694-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-04

Quant Time: Nov 08 13:48:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

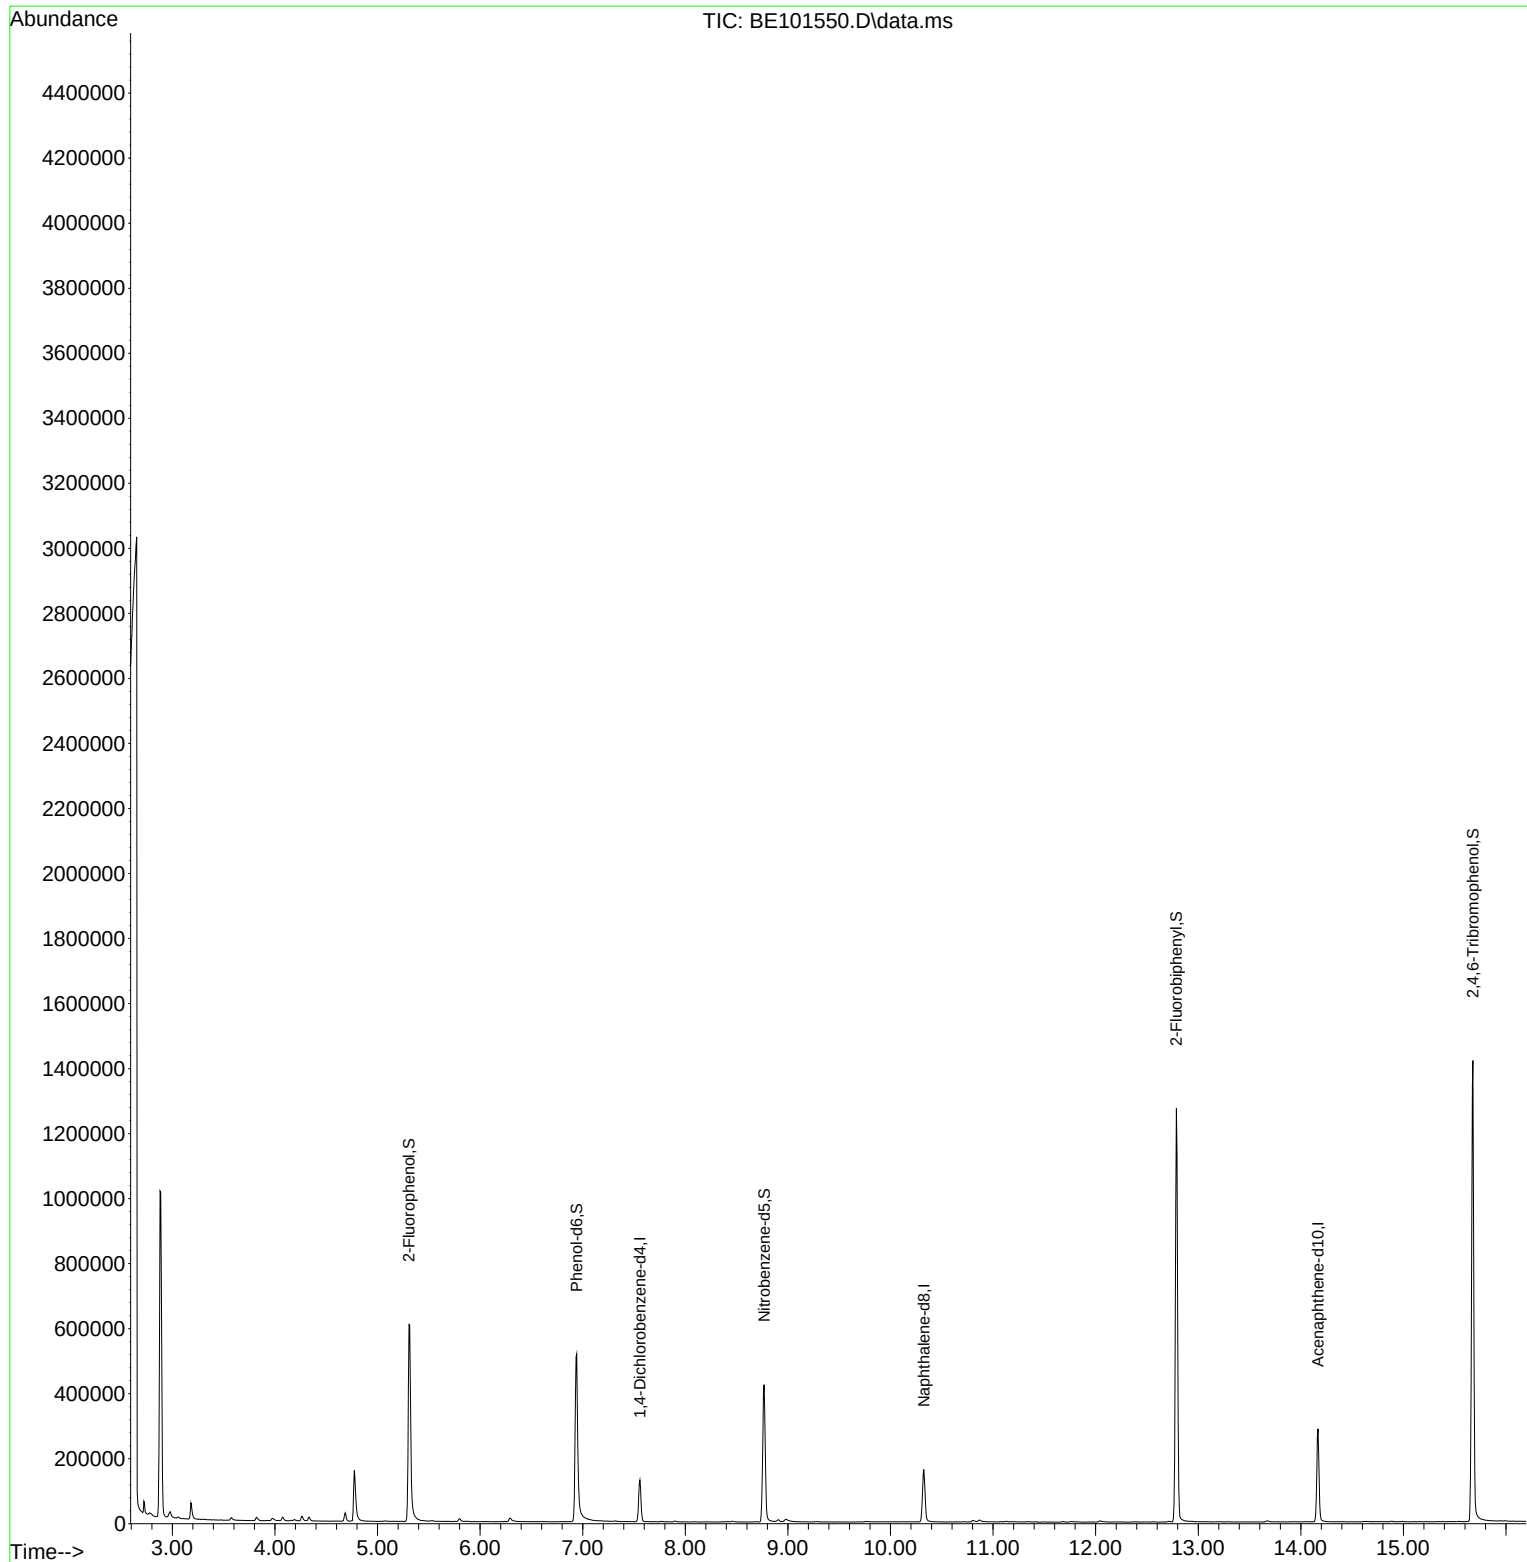

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101550.D
Acq On : 8 Nov 2024 13:56
Operator : RC/JU
Sample : P4694-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-04

Quant Time: Nov 08 13:48:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

