

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101553.D
 Acq On : 8 Nov 2024 15:44
 Operator : RC/JU
 Sample : P4739-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-G2

Quant Time: Nov 08 15:28:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.555	152	37151	20.000	ng	0.00
21) Naphthalene-d8	10.323	136	149942	20.000	ng	0.00
39) Acenaphthene-d10	14.165	164	100255	20.000	ng	0.00
64) Phenanthrene-d10	16.903	188	260781	20.000	ng	0.00
76) Chrysene-d12	21.063	240	352844	20.000	ng	-0.01
86) Perylene-d12	23.348	264	472912	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.311	112	335295	159.581	ng	0.00
7) Phenol-d6	6.938	99	403910	140.210	ng	0.00
23) Nitrobenzene-d5	8.766	82	238937	100.655	ng	0.00
42) 2,4,6-Tribromophenol	15.675	330	322975	171.204	ng	0.00
45) 2-Fluorobiphenyl	12.790	172	603572	98.301	ng	0.00
79) Terphenyl-d14	19.500	244	1854912	116.368	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101553.D
Acq On : 8 Nov 2024 15:44
Operator : RC/JU
Sample : P4739-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G2

Quant Time: Nov 08 15:28:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

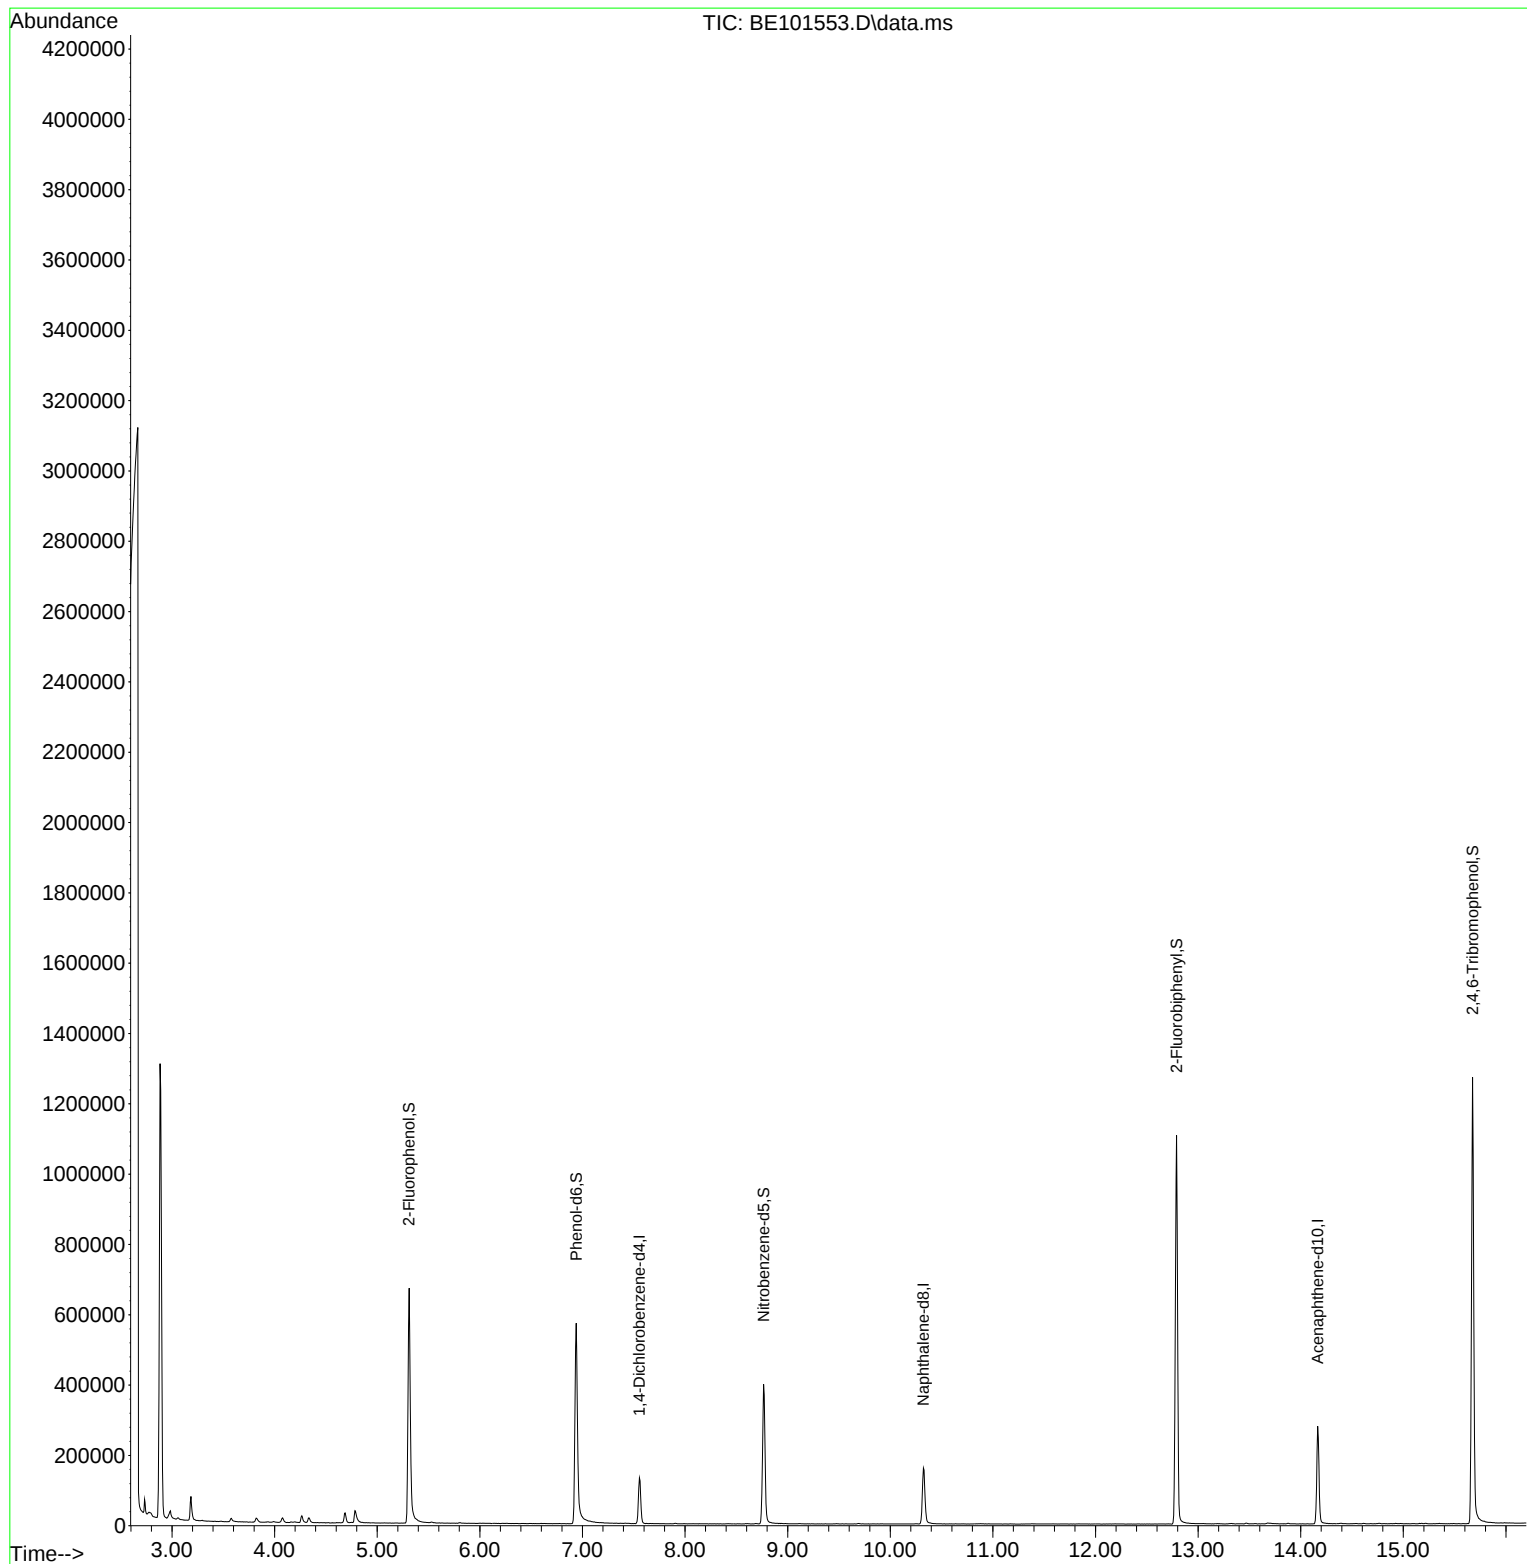

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101553.D
Acq On : 8 Nov 2024 15:44
Operator : RC/JU
Sample : P4739-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-G2

Quant Time: Nov 08 15:28:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

