

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101556.D
 Acq On : 8 Nov 2024 17:31
 Operator : RC/JU
 Sample : P4739-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 TP-14

Quant Time: Nov 08 23:47:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	42587	20.000	ng	-0.01
21) Naphthalene-d8	10.326	136	178340	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	117342	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	286380	20.000	ng	0.00
76) Chrysene-d12	21.067	240	357270	20.000	ng	-0.01
86) Perylene-d12	23.352	264	460355	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.314	112	409750	170.125	ng	0.00
7) Phenol-d6	6.936	99	499007	151.110	ng	-0.01
23) Nitrobenzene-d5	8.769	82	295521	104.668	ng	0.00
42) 2,4,6-Tribromophenol	15.679	330	353414	160.059	ng	0.00
45) 2-Fluorobiphenyl	12.788	172	726189	101.048	ng	-0.01
79) Terphenyl-d14	19.498	244	1747996	108.302	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101556.D
Acq On : 8 Nov 2024 17:31
Operator : RC/JU
Sample : P4739-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-14

Quant Time: Nov 08 23:47:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

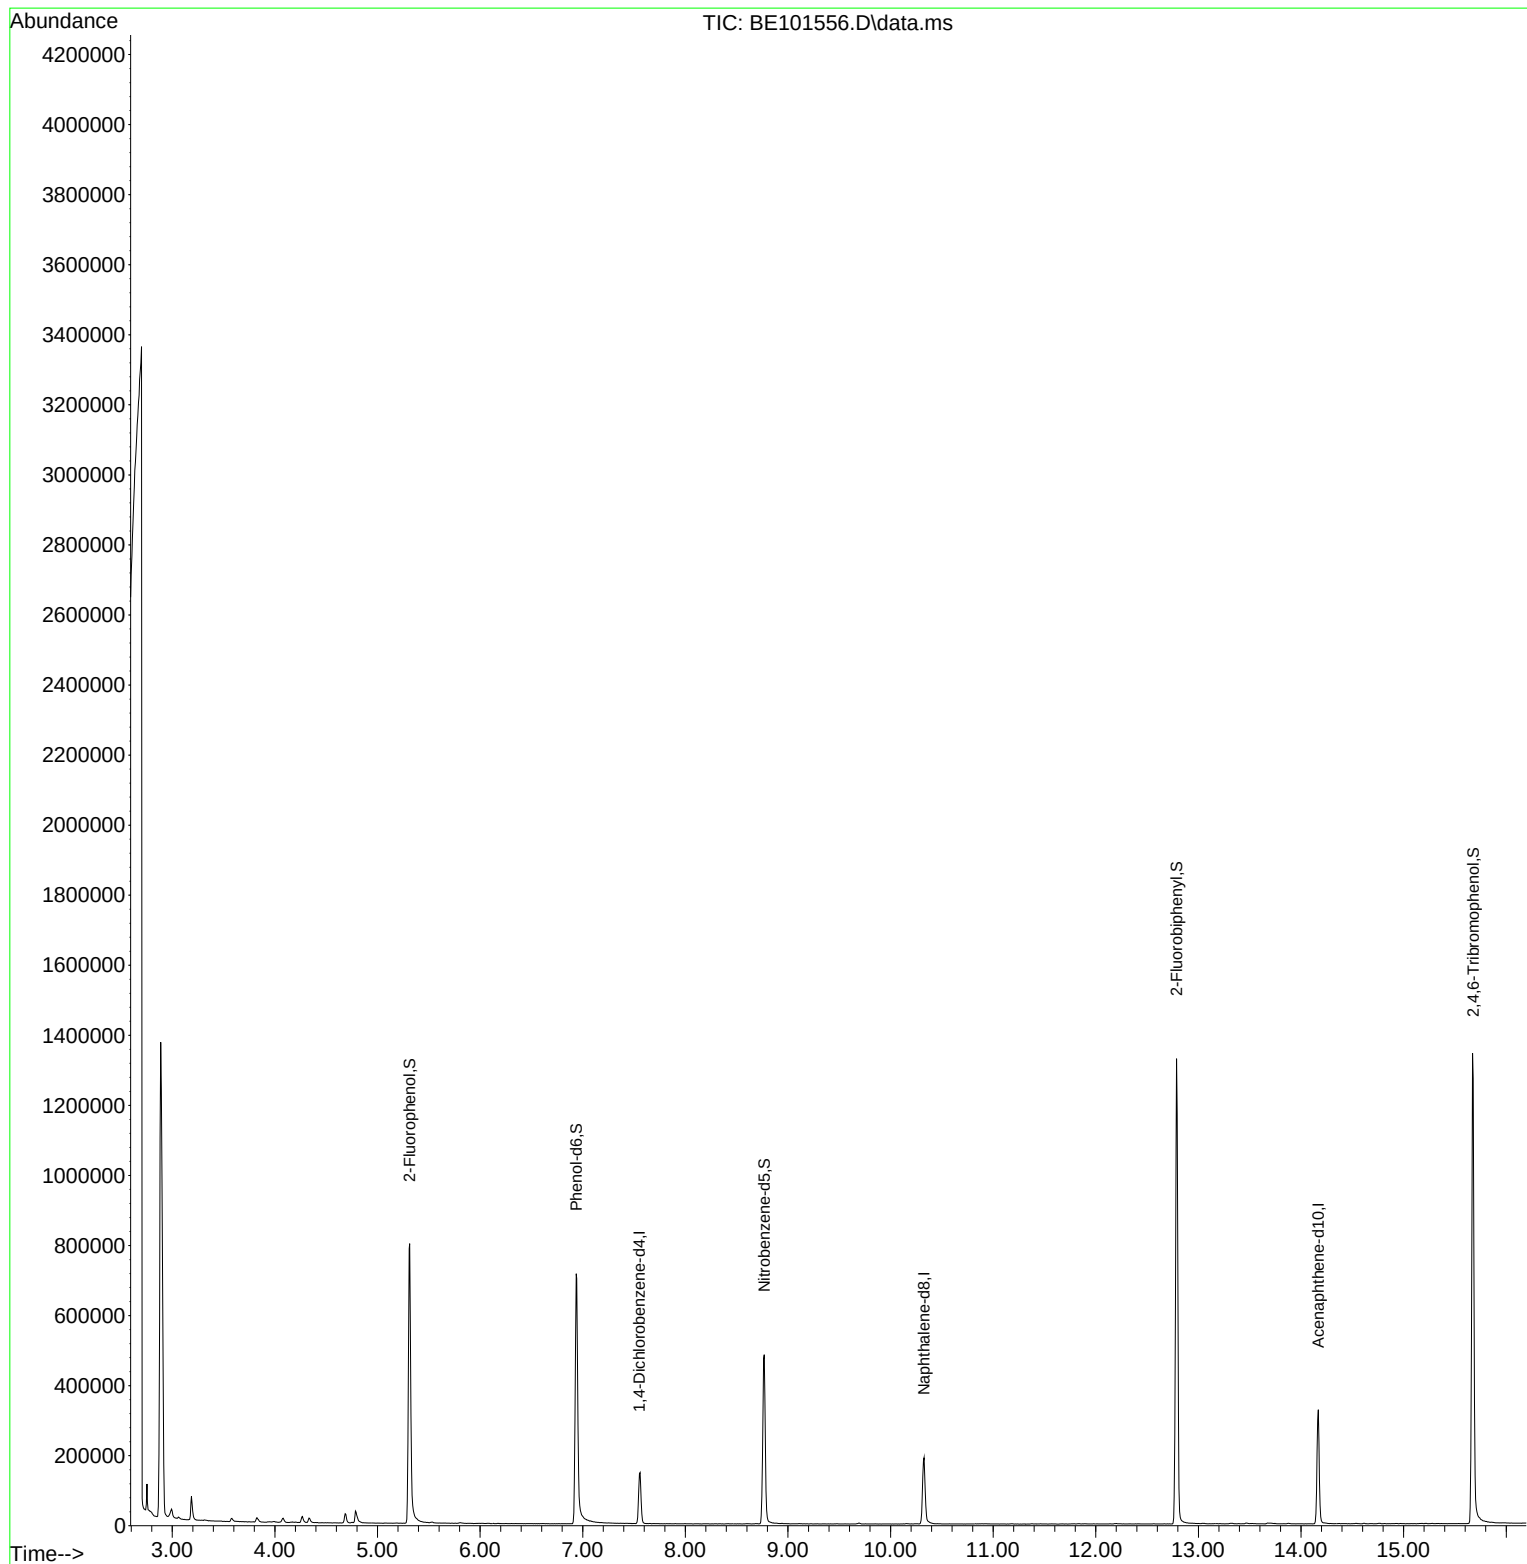

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101556.D
Acq On : 8 Nov 2024 17:31
Operator : RC/JU
Sample : P4739-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-14

Quant Time: Nov 08 23:47:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

