

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110824\  
 Data File : BE101559.D  
 Acq On : 8 Nov 2024 19:19  
 Operator : RC/JU  
 Sample : P4732-02  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 PPE-COMP

Quant Time: Nov 08 23:49:08 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 07 00:01:20 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.557  | 152  | 48513    | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.325 | 136  | 202387   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.167 | 164  | 136414   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 16.905 | 188  | 328245   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.065 | 240  | 391819   | 20.000  | ng    | -0.01    |
| 86) Perylene-d12            | 23.351 | 264  | 513750   | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.313  | 112  | 419577   | 152.925 | ng    | 0.00     |
| 7) Phenol-d6                | 6.940  | 99   | 514040   | 136.648 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.768  | 82   | 319125   | 99.599  | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.677 | 330  | 392605   | 152.949 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 12.787 | 172  | 780370   | 93.406  | ng    | -0.01    |
| 79) Terphenyl-d14           | 19.502 | 244  | 1966505  | 111.097 | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110824\  
Data File : BE101559.D  
Acq On : 8 Nov 2024 19:19  
Operator : RC/JU  
Sample : P4732-02  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PPE-COMP

Quant Time: Nov 08 23:49:08 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

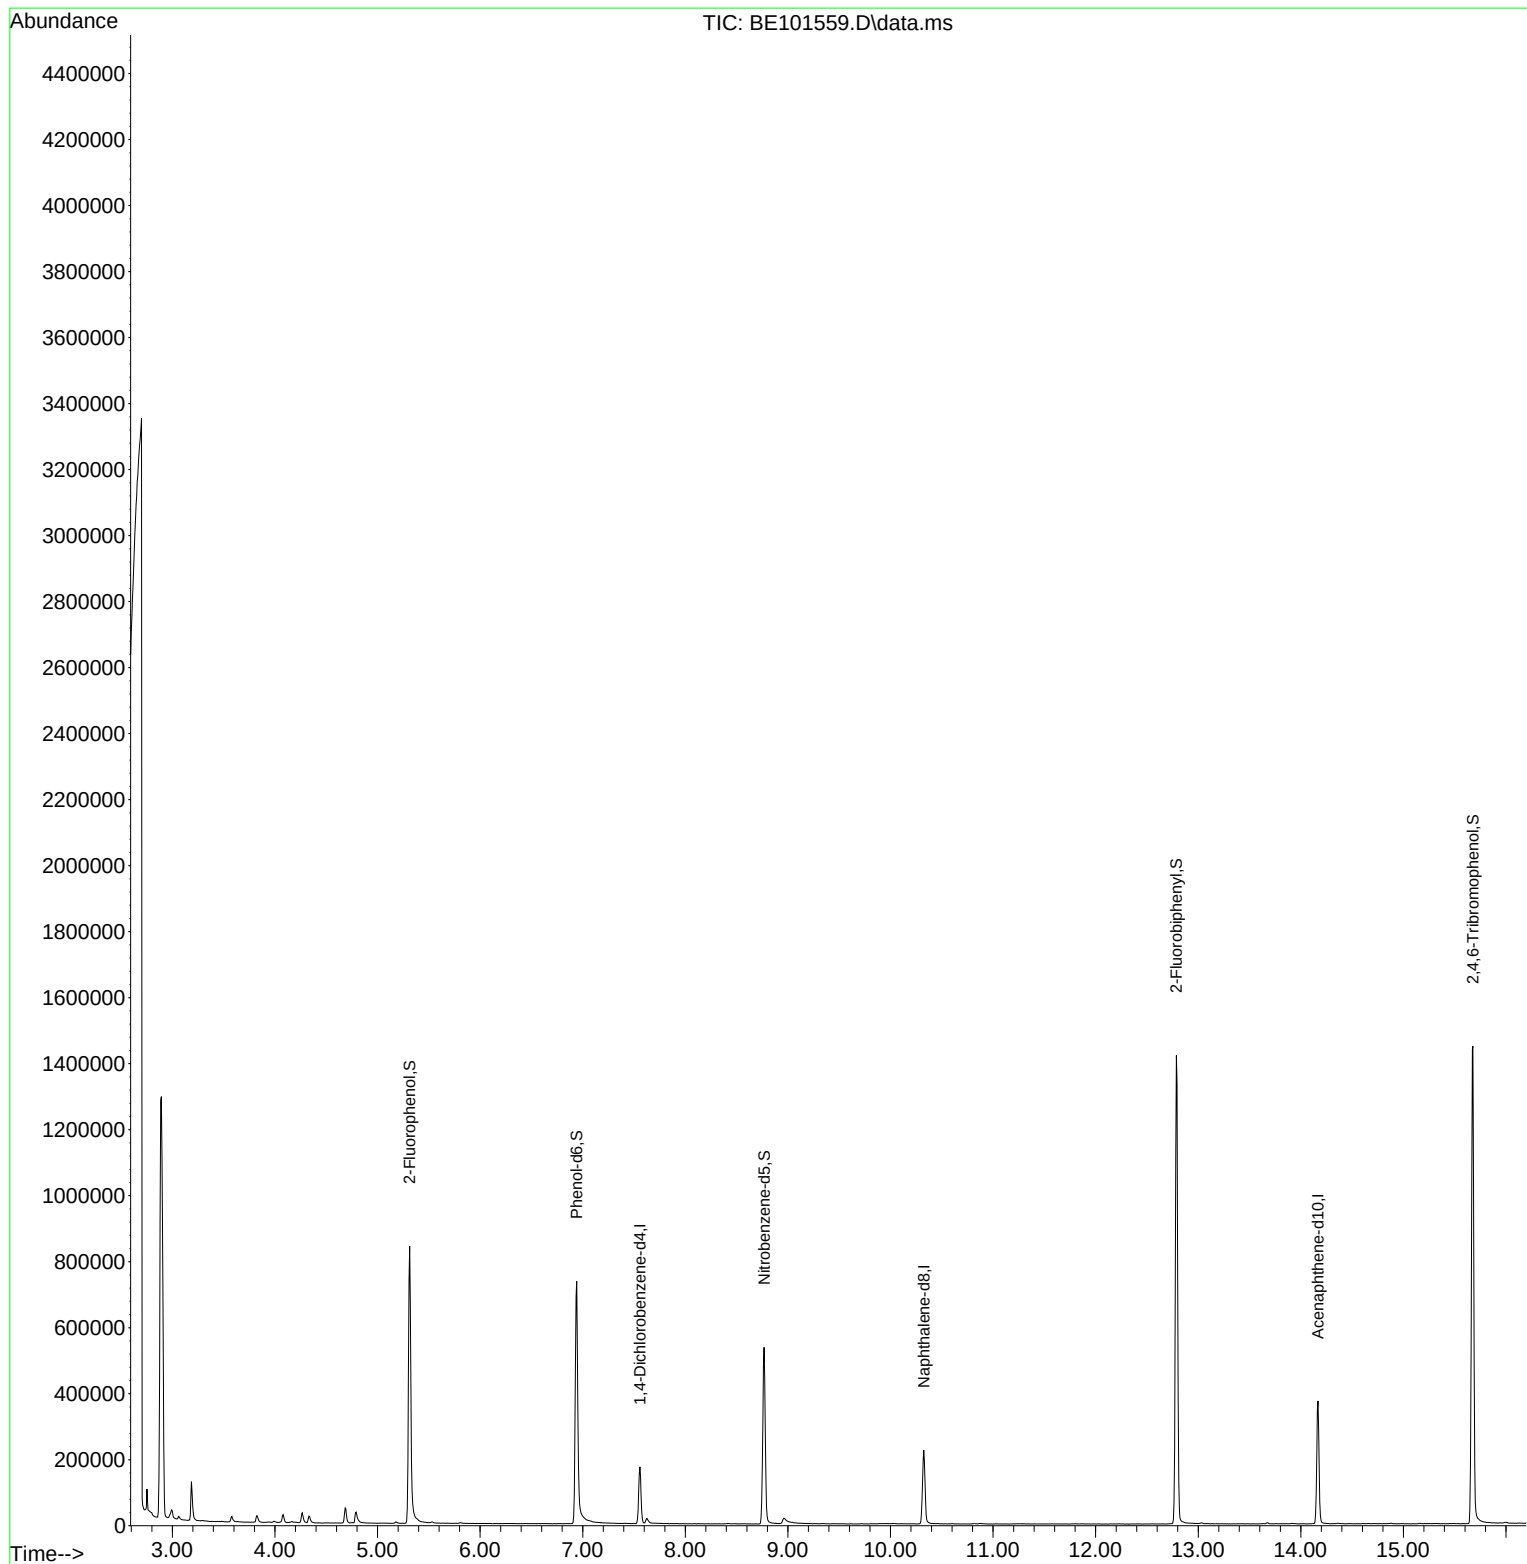

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110824\  
Data File : BE101559.D  
Acq On : 8 Nov 2024 19:19  
Operator : RC/JU  
Sample : P4732-02  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PPE-COMP

Quant Time: Nov 08 23:49:08 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE110624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 07 00:01:20 2024  
Response via : Initial Calibration

