

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101562.D
 Acq On : 8 Nov 2024 21:06
 Operator : RC/JU
 Sample : P4722-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 WC-1(0-6)

Quant Time: Nov 08 23:50:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	43597	20.000	ng	0.00
21) Naphthalene-d8	10.326	136	181077	20.000	ng	0.00
39) Acenaphthene-d10	14.163	164	121098	20.000	ng	-0.01
64) Phenanthrene-d10	16.901	188	293866	20.000	ng	-0.01
76) Chrysene-d12	21.067	240	362629	20.000	ng	-0.01
86) Perylene-d12	23.346	264	463143	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.309	112	325298	131.932	ng	0.00
7) Phenol-d6	6.936	99	362532	107.239	ng	-0.01
23) Nitrobenzene-d5	8.763	82	276209	96.350	ng	-0.01
42) 2,4,6-Tribromophenol	15.673	330	352080	154.509	ng	-0.01
45) 2-Fluorobiphenyl	12.788	172	700448	94.444	ng	-0.01
79) Terphenyl-d14	19.498	244	1816656	110.892	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101562.D
Acq On : 8 Nov 2024 21:06
Operator : RC/JU
Sample : P4722-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-1(0-6)

Quant Time: Nov 08 23:50:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

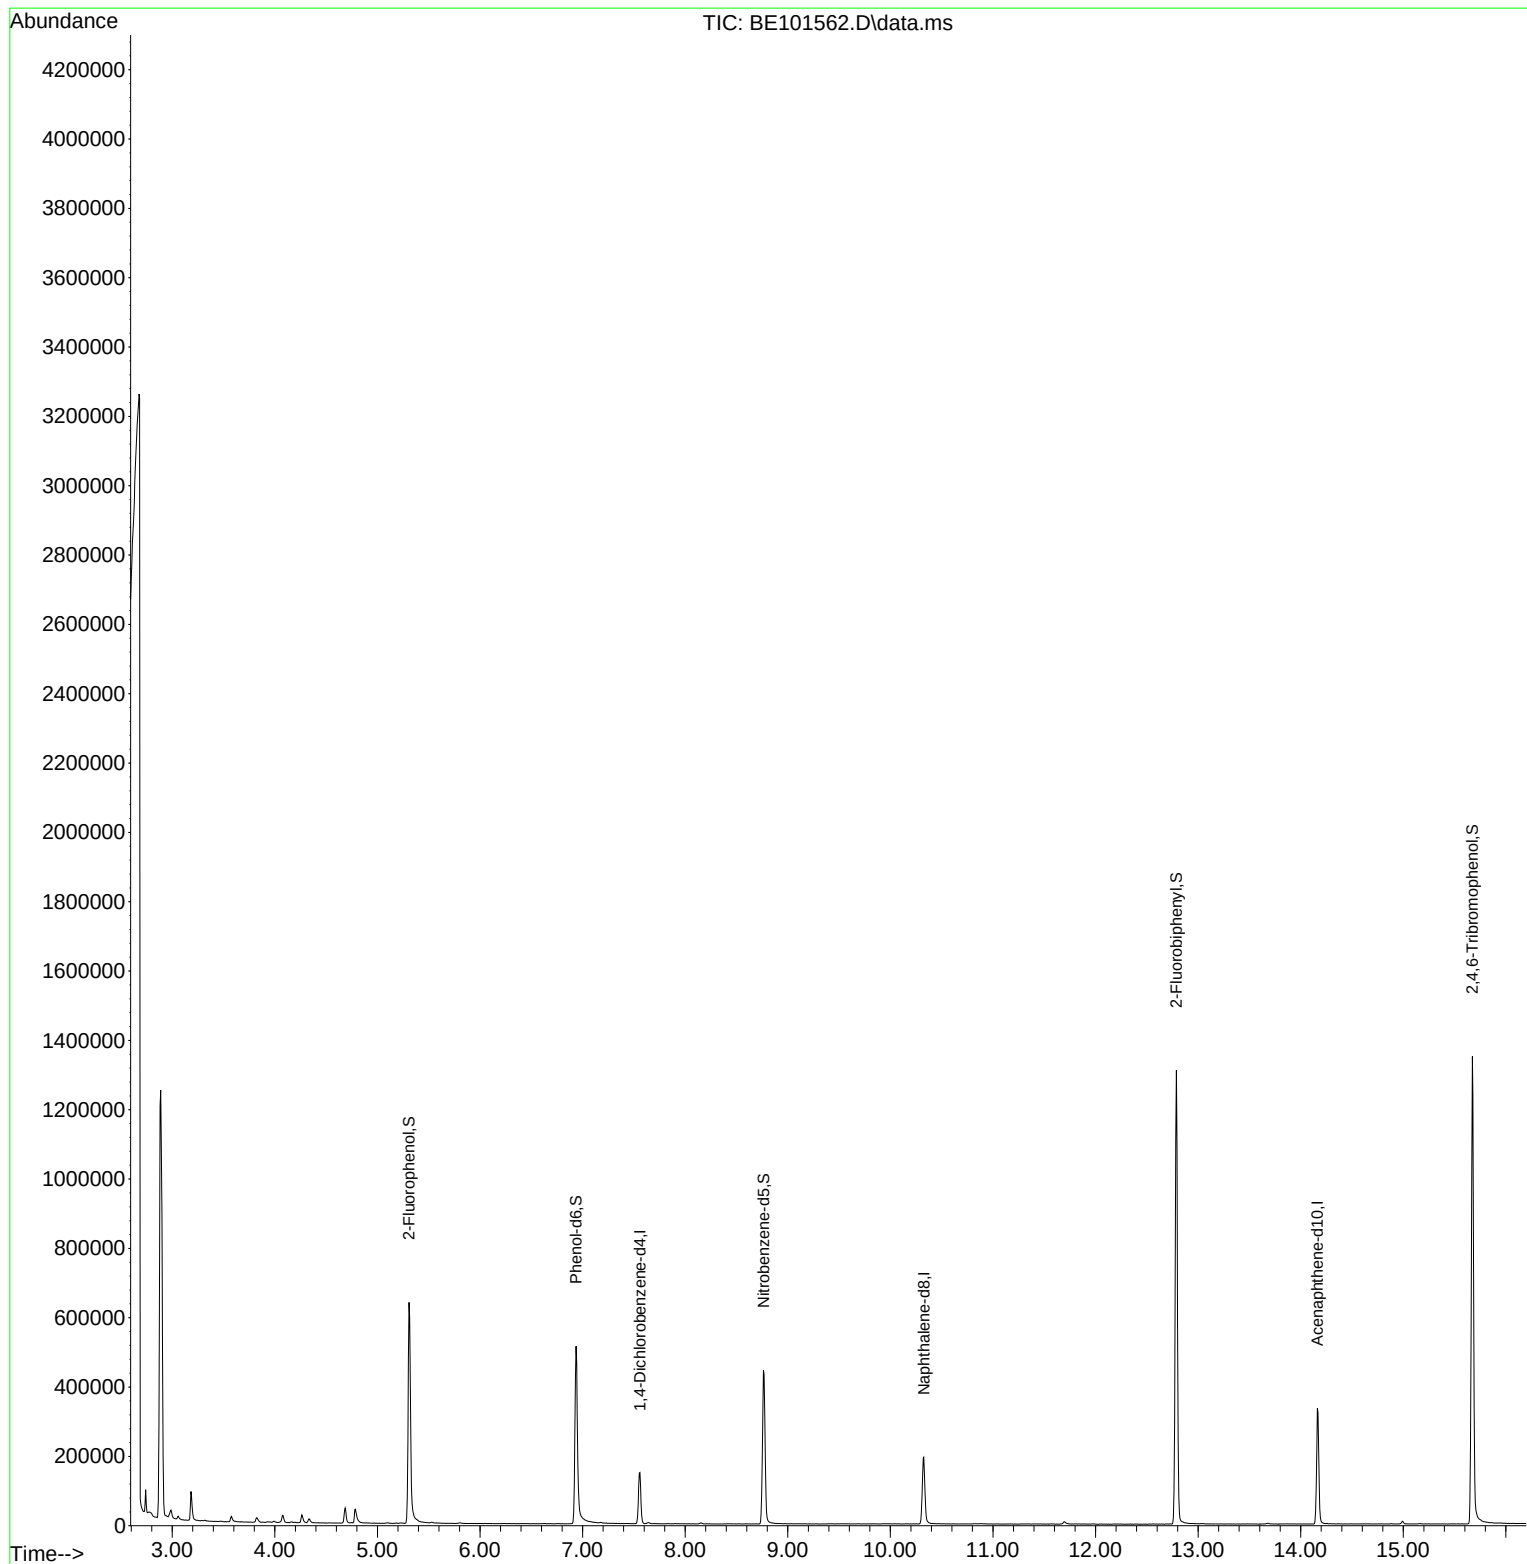

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101562.D
Acq On : 8 Nov 2024 21:06
Operator : RC/JU
Sample : P4722-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-1(0-6)

Quant Time: Nov 08 23:50:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

