
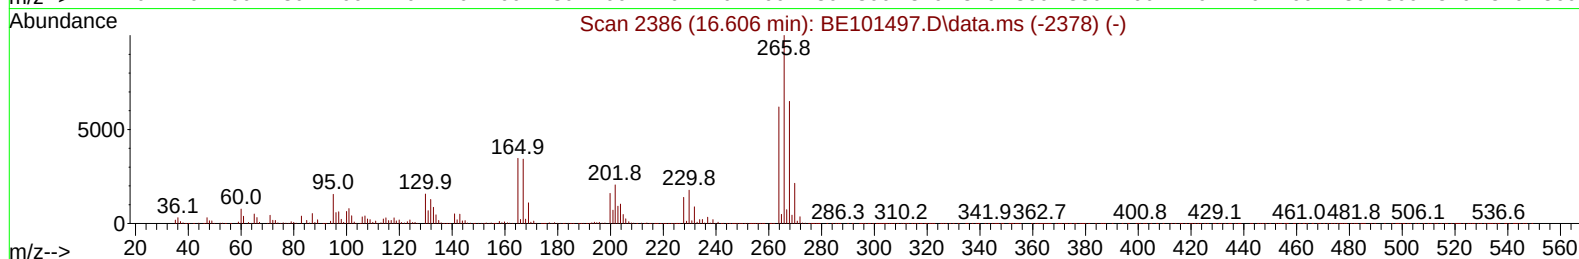
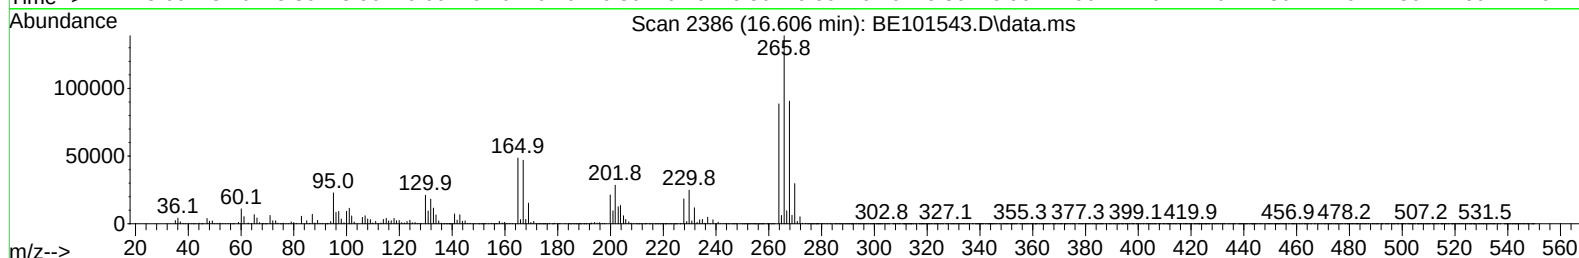


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101543.D
Acq On : 8 Nov 2024 9:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 10:13:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

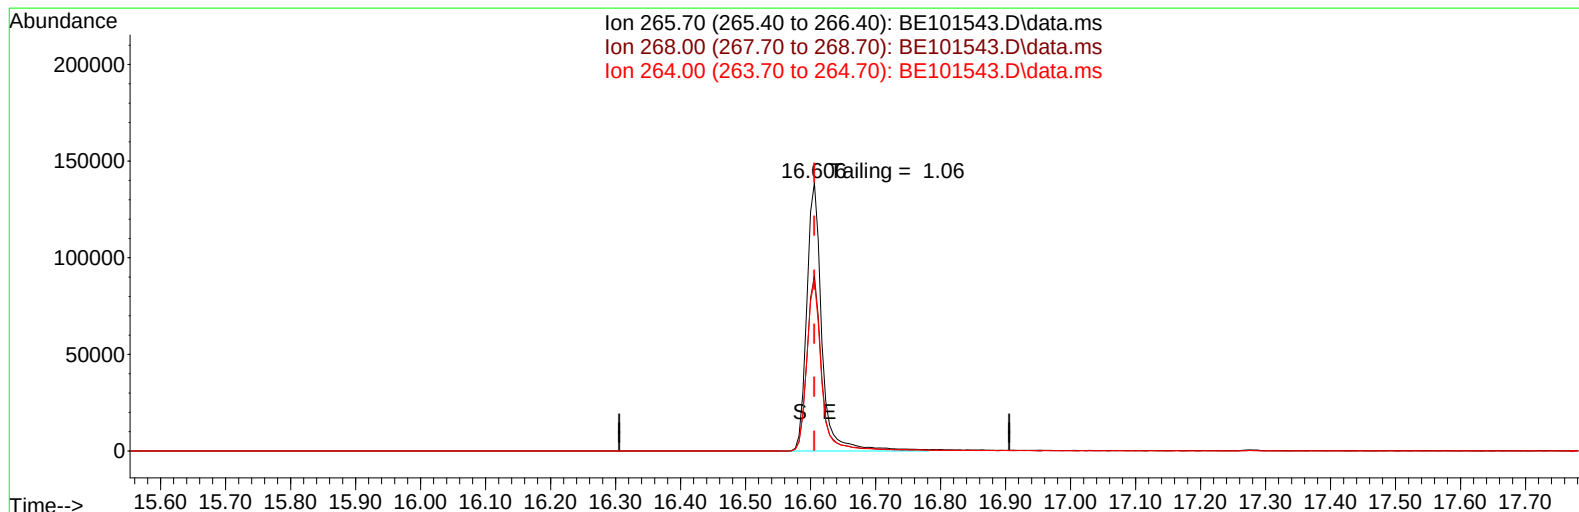

TIC: BE101543.D\data.ms

(70) Pentachlorophenol (C)

16.606min (+ 0.000) 216541.97 ng

response **225120**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	65.00	65.21
--------	-------	-------

264.00	62.00	63.72
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101543.D
Acq On : 8 Nov 2024 9:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 10:13:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

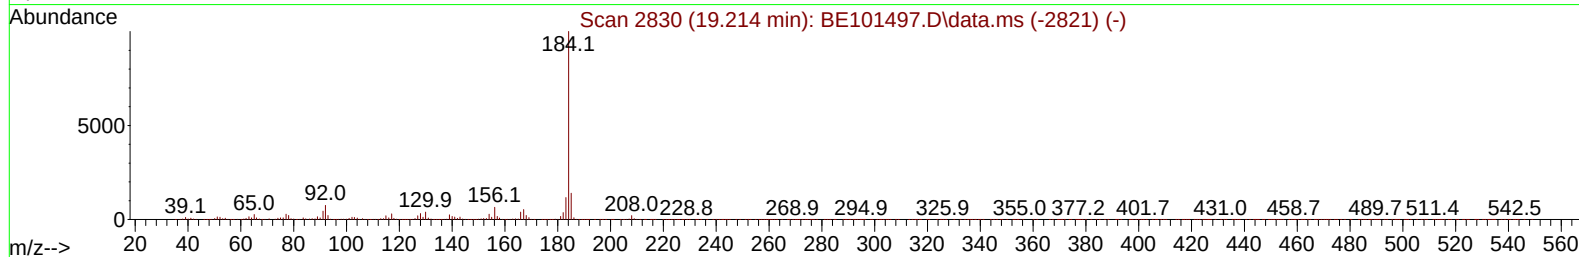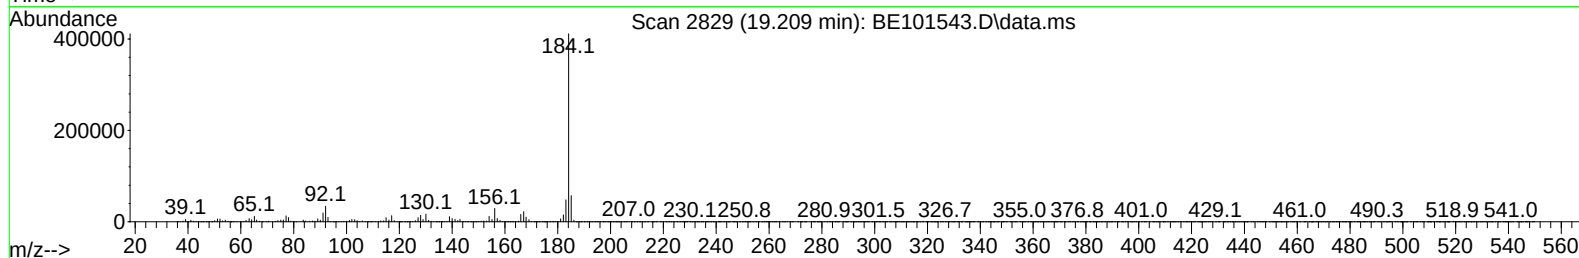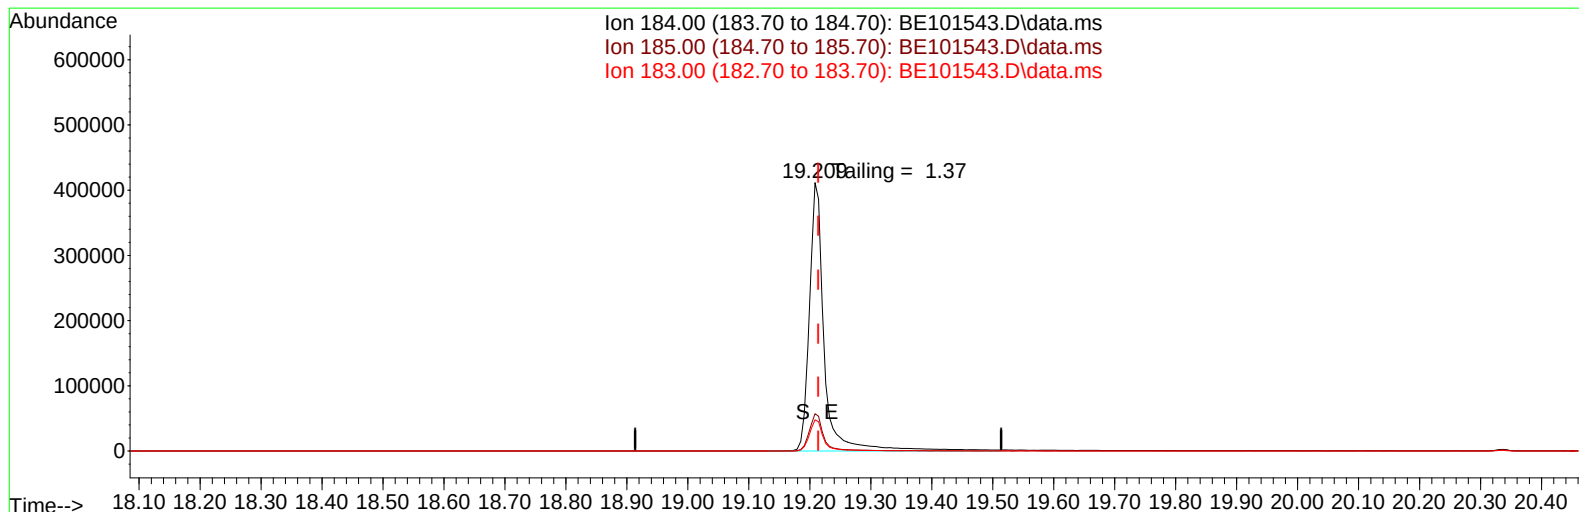

TIC: BE101543.D\data.ms

(77) Benzidine**19.209min (-0.005) 40480.74 ng****response 698261**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	11.70	11.67
0.00	0.00	0.00