

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
 Data File : BE101545.D
 Acq On : 8 Nov 2024 10:51
 Operator : RC/JU
 Sample : PB164750BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164750BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.776	368	372	386	rBV	78306	127628	3.54%	0.962%
2	5.311	456	463	489	rBV	637933	1086917	30.14%	8.193%
3	6.938	733	740	778	rBV	572137	1101458	30.55%	8.303%
4	7.555	839	845	858	rBV	117425	192549	5.34%	1.451%
5	8.765	1043	1051	1072	rBV	379365	678248	18.81%	5.113%
6	10.328	1309	1317	1334	rBV	151020	281898	7.82%	2.125%
7	12.790	1728	1736	1759	rBV	1114358	1711360	47.46%	12.900%
8	14.171	1964	1971	1986	rBV	247860	397095	11.01%	2.993%
9	15.675	2218	2227	2266	rBV	1044614	1624255	45.05%	12.244%
10	16.909	2430	2437	2450	rBV	343082	537705	14.91%	4.053%
11	19.500	2872	2878	2896	rBV	2879895	3605651	100.00%	27.179%
12	21.069	3139	3145	3155	rBV	609639	818377	22.70%	6.169%
13	23.354	3526	3534	3542	rBV2	544469	1103114	30.59%	8.315%




Sum of corrected areas: 13266255

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101545.D
Acq On : 8 Nov 2024 10:51
Operator : RC/JU
Sample : PB164750BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164750BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

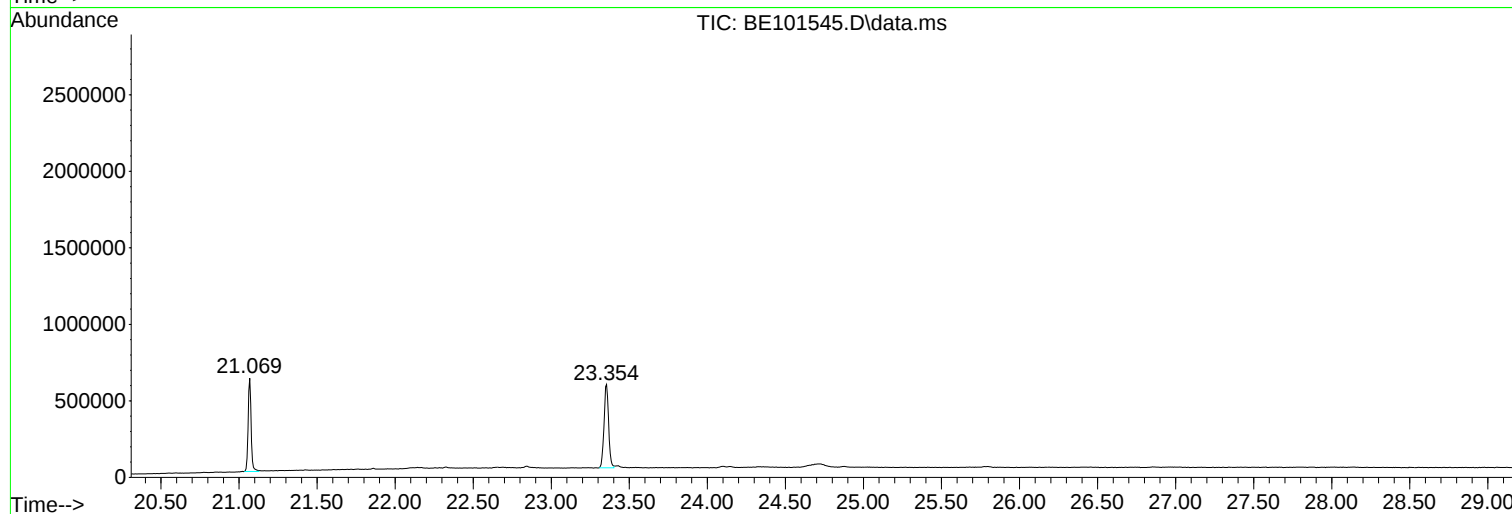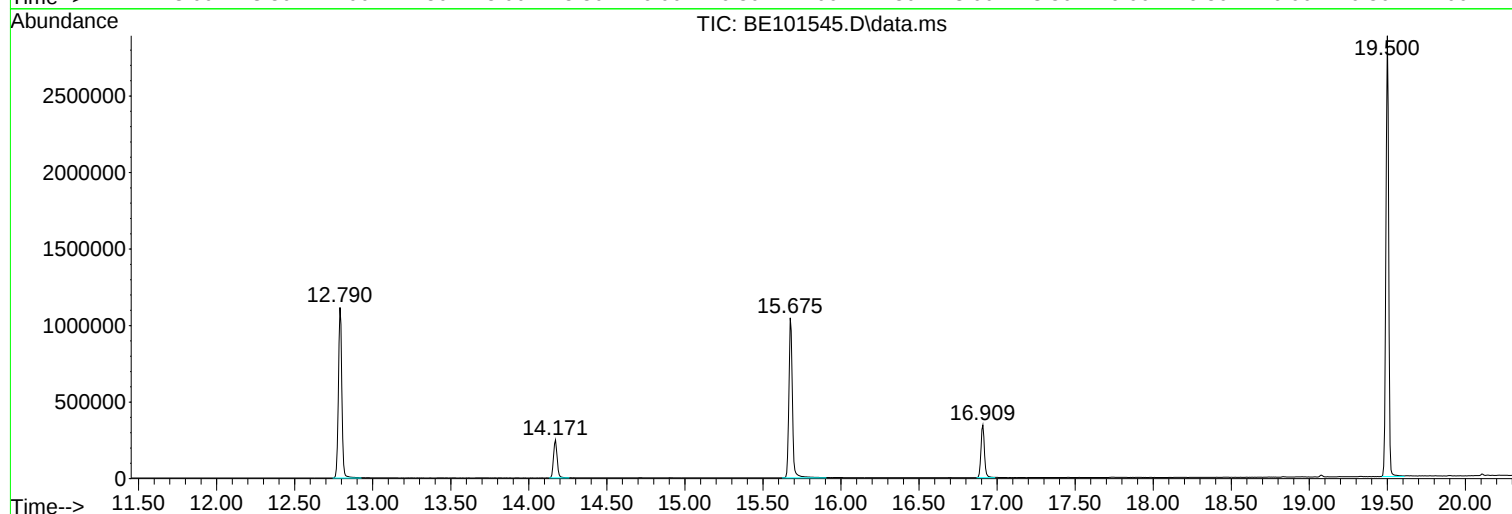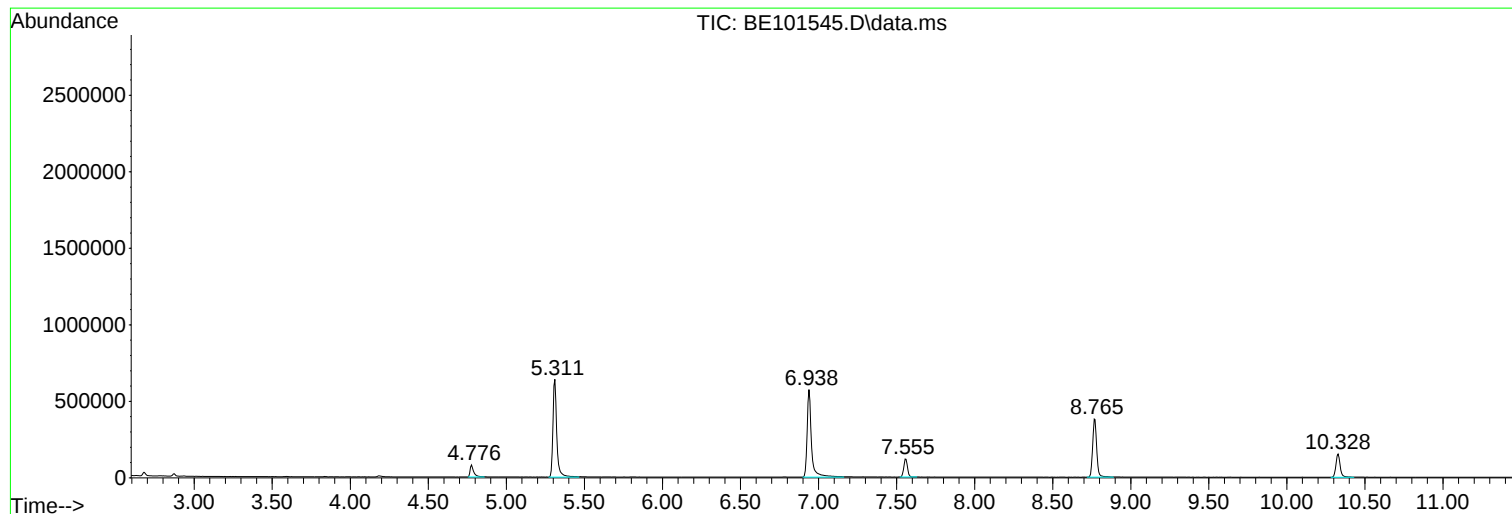

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101545.D
Acq On : 8 Nov 2024 10:51
Operator : RC/JU
Sample : PB164750BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164750BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.776	13.26 ng	127628	1,4-Dichlorobenzene-d4	7.555

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

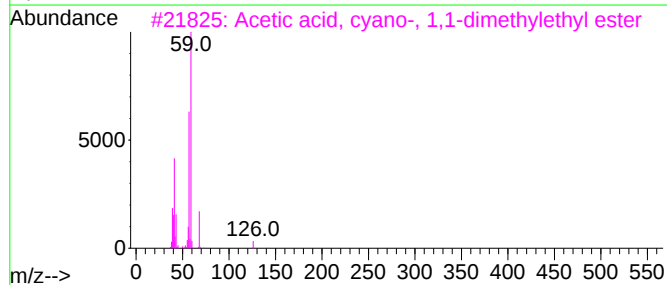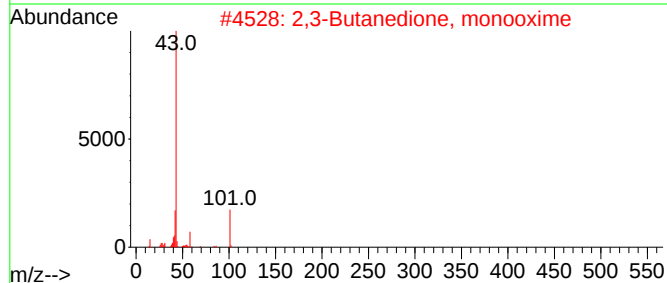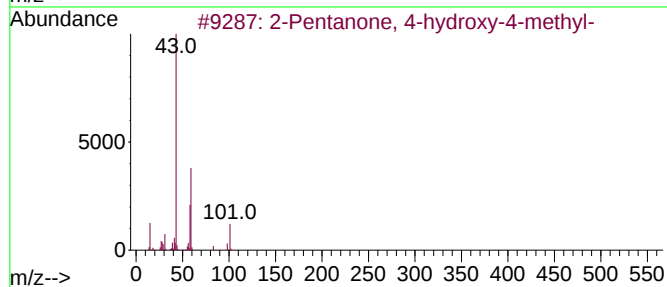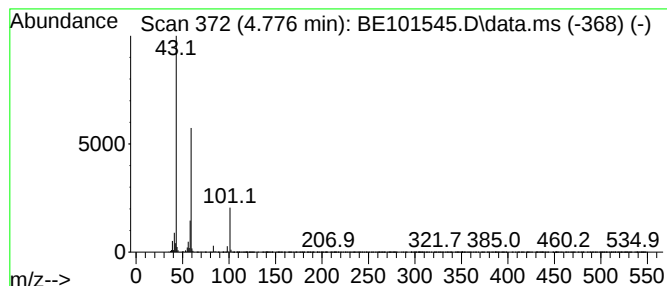

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110824\
Data File : BE101545.D
Acq On : 8 Nov 2024 10:51
Operator : RC/JU
Sample : PB164750BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164750BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.776	13.3	ng	127628	1	7.555	192549	20.0