
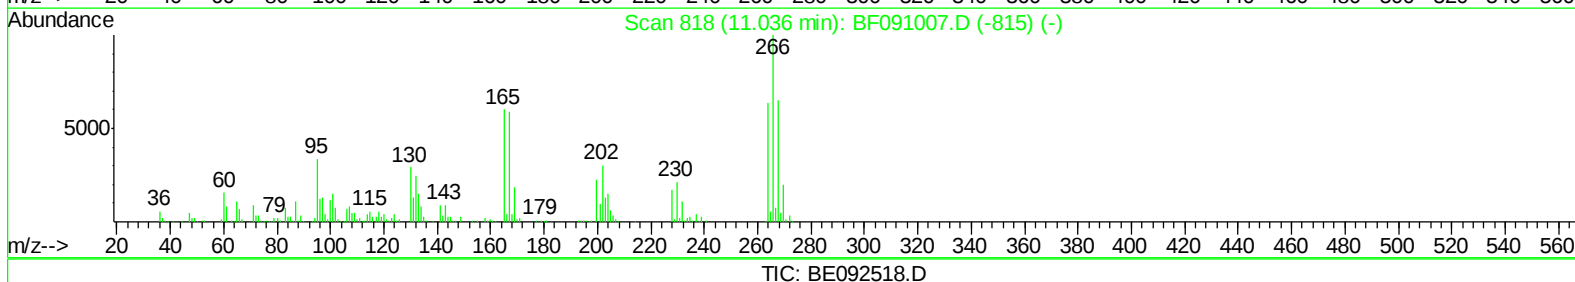
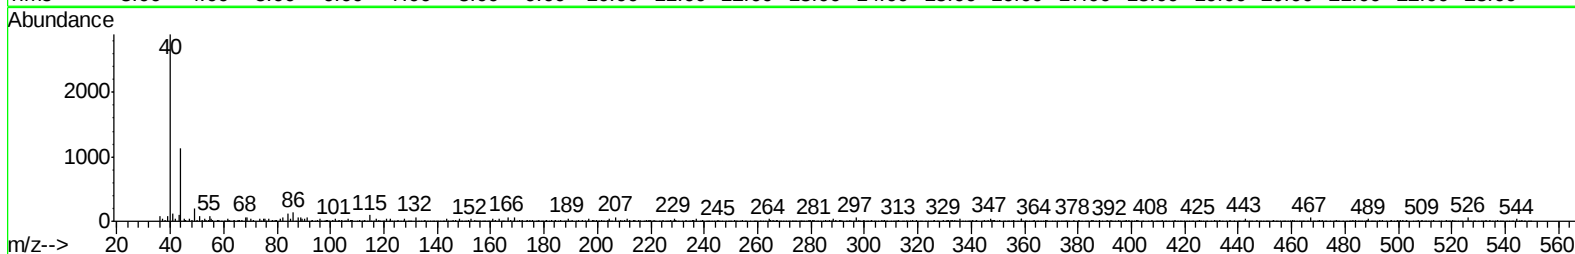


Data Path : Z:\HPCHEM1\BNA E\DATA\BE110916\
Data File : BE092518.D
Acq On : 9 Nov 2016 9:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:44:06 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

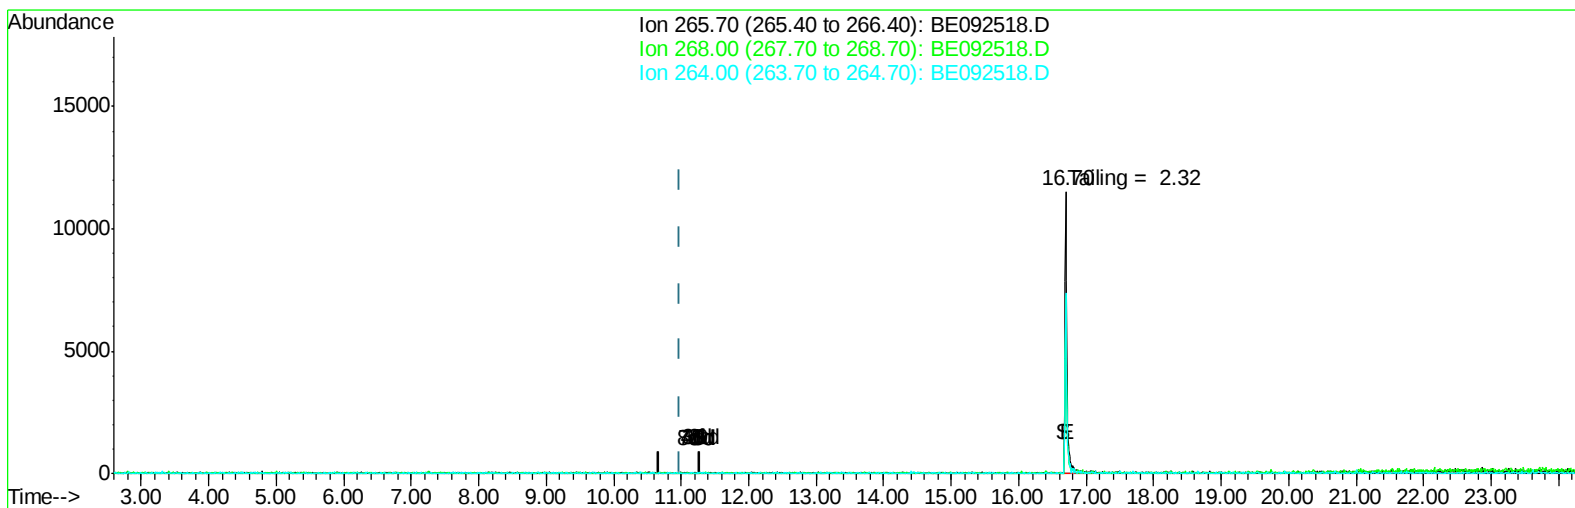

TIC: BE092518.D

(69) Pentachlorophenol (C)




11.249min (+0.258) 144.33ng

response 22

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	18.18#
264.00	63.90	100.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110916\
Data File : BE092518.D
Acq On : 9 Nov 2016 9:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:44:06 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

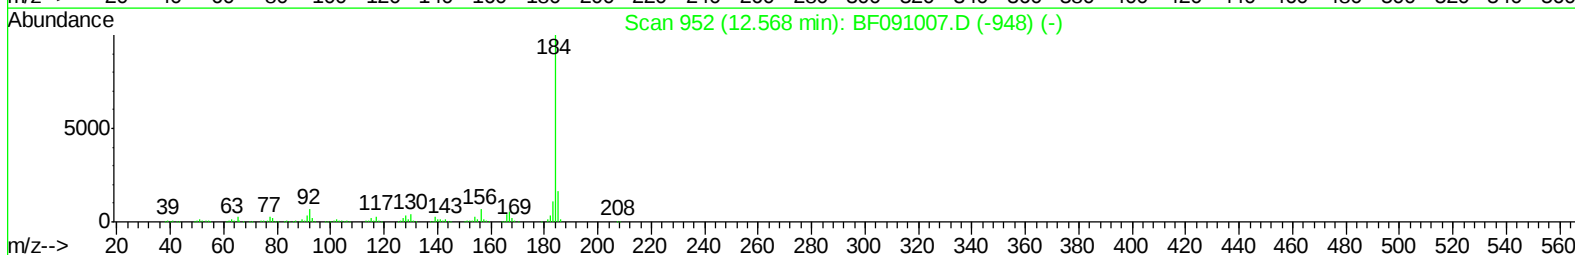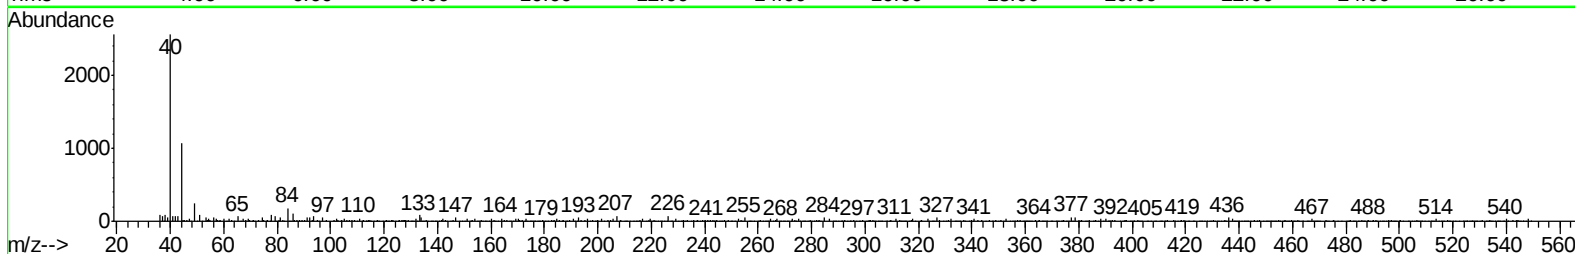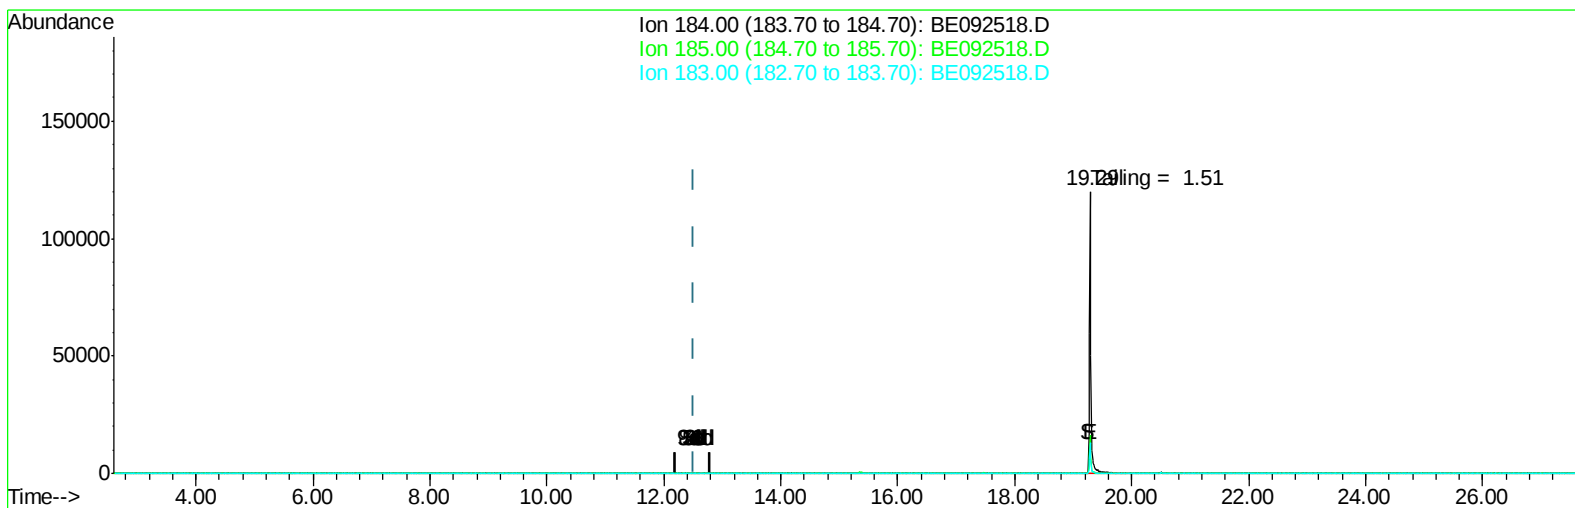

TIC: BE092518.D

(76) Benzidine

12.594min (+0.084) 138.76ng

response 31

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	33.96#
183.00	10.90	64.15#
0.00	0.00	0.00