


Data Path : Z:\HPCHEM1\BNA E\DATA\BE110916\
Data File : BE092518.D
Acq On : 9 Nov 2016 9:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE110816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 08 16:27:22 2016

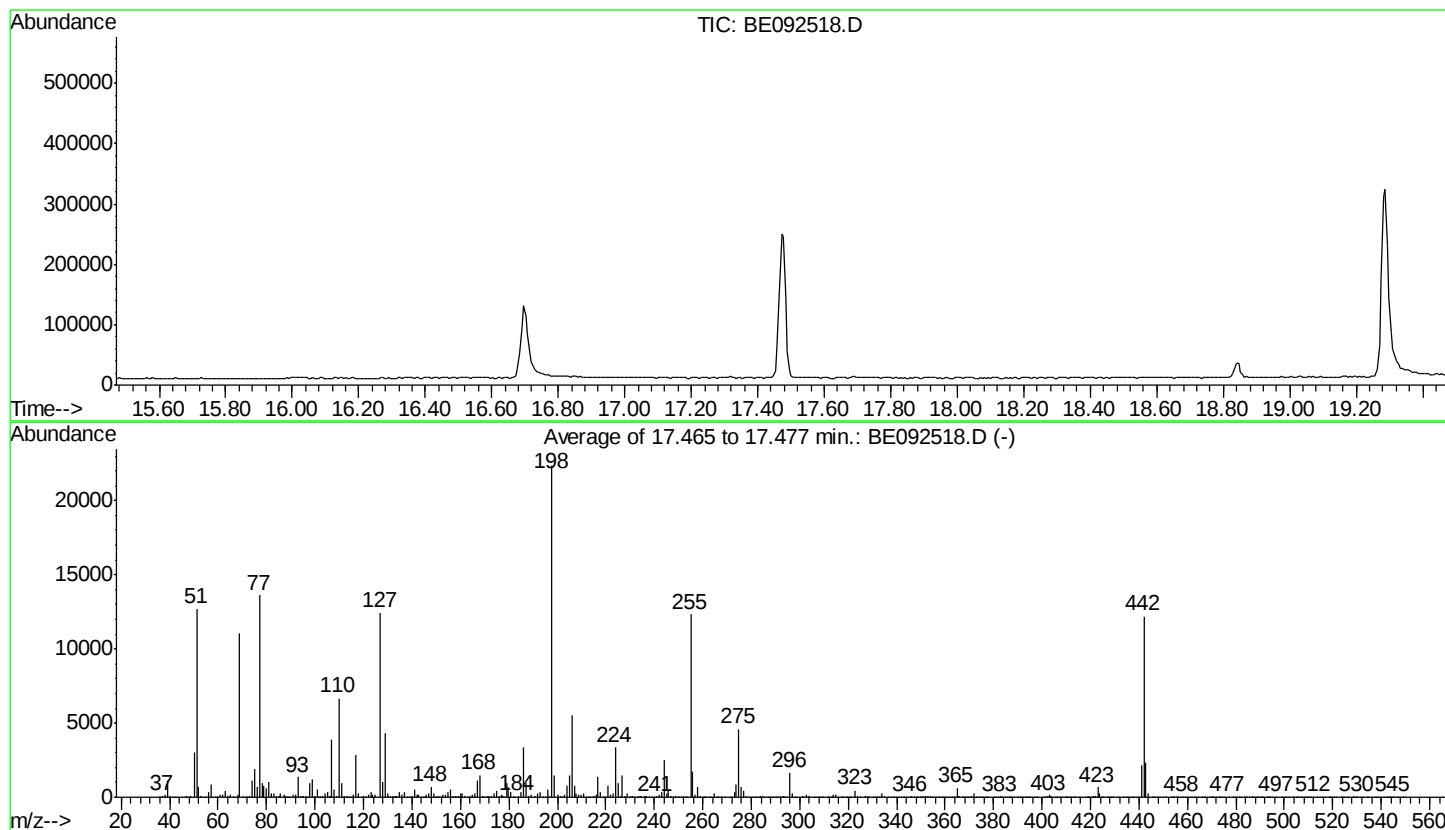

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	12732	PASS
68	69	0.00	2	1.8	199	PASS
69	198	0.00	100	49.3	11013	PASS
70	69	0.00	2	0.2	24	PASS
127	198	10	80	55.7	12459	PASS
197	198	0.00	2	0.4	87	PASS
198	198	100	100	100.0	22356	PASS
199	198	5	9	6.7	1487	PASS
275	198	10	60	20.6	4609	PASS
365	198	1	100	2.8	629	PASS
441	442	0.01	24	17.9	2191	PASS
442	198	50	100	54.6	12214	PASS
443	442	15	24	19.4	2372	PASS