


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE110917\
Data File : BE094783.D
Acq On : 8 Nov 2017 15:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 23 22:40:47 2017

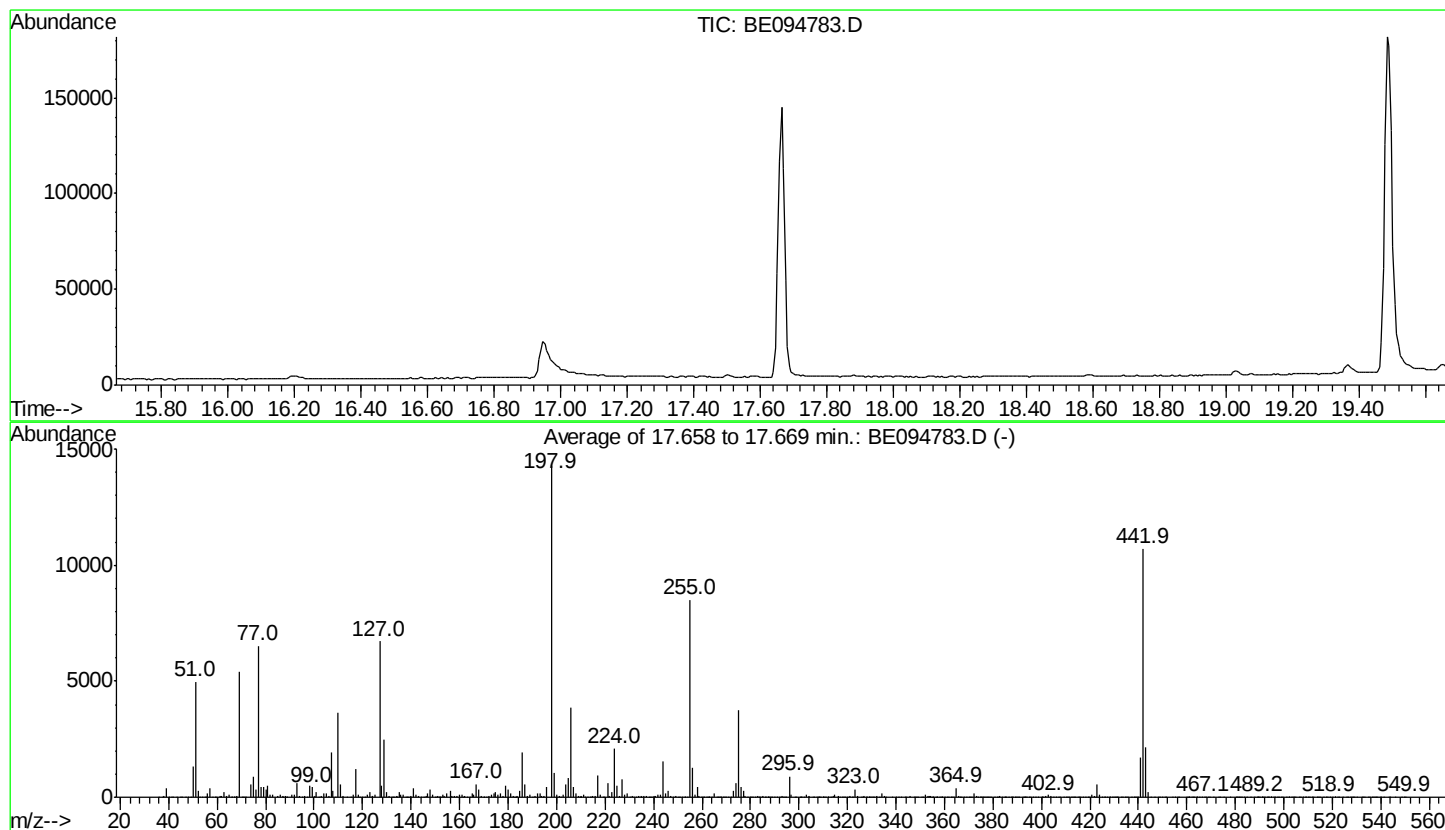

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	4983	PASS
68	69	0.00	2	0.6	30	PASS
69	198	0.00	100	37.7	5381	PASS
70	69	0.00	2	0.5	28	PASS
127	198	10	80	47.1	6725	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14289	PASS
199	198	5	9	7.3	1047	PASS
275	198	10	60	26.4	3769	PASS
365	198	1	100	2.7	389	PASS
441	442	0.01	24	15.8	1692	PASS
442	198	50	100	75.0	10720	PASS
443	442	15	24	20.1	2159	PASS