

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
 Data File : BE091110.D
 Acq On : 11 Nov 2015 00:23
 Operator : UM/NP
 Sample : G4308-16MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KR2MSD

Quant Time: Nov 13 14:06:21 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3371	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	19246	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	11753	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1653871	0.40	ng/ul	0.08
18) Chrysene-d12	20.29	240	34042	0.40	ng/ul	0.00
22) Perylene-d12	22.07	264	1882113	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.96	96	5258	2.17	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.07	152	7595	0.29	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	21191	0.00	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.62	128	2434	0.05	ng/ul#	85
19) Pyrene	18.51	202	12902	0.03	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091110.D
Acq On : 11 Nov 2015 00:23
Operator : UM/NP
Sample : G4308-16MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MSD

Quant Time: Nov 13 14:06:21 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

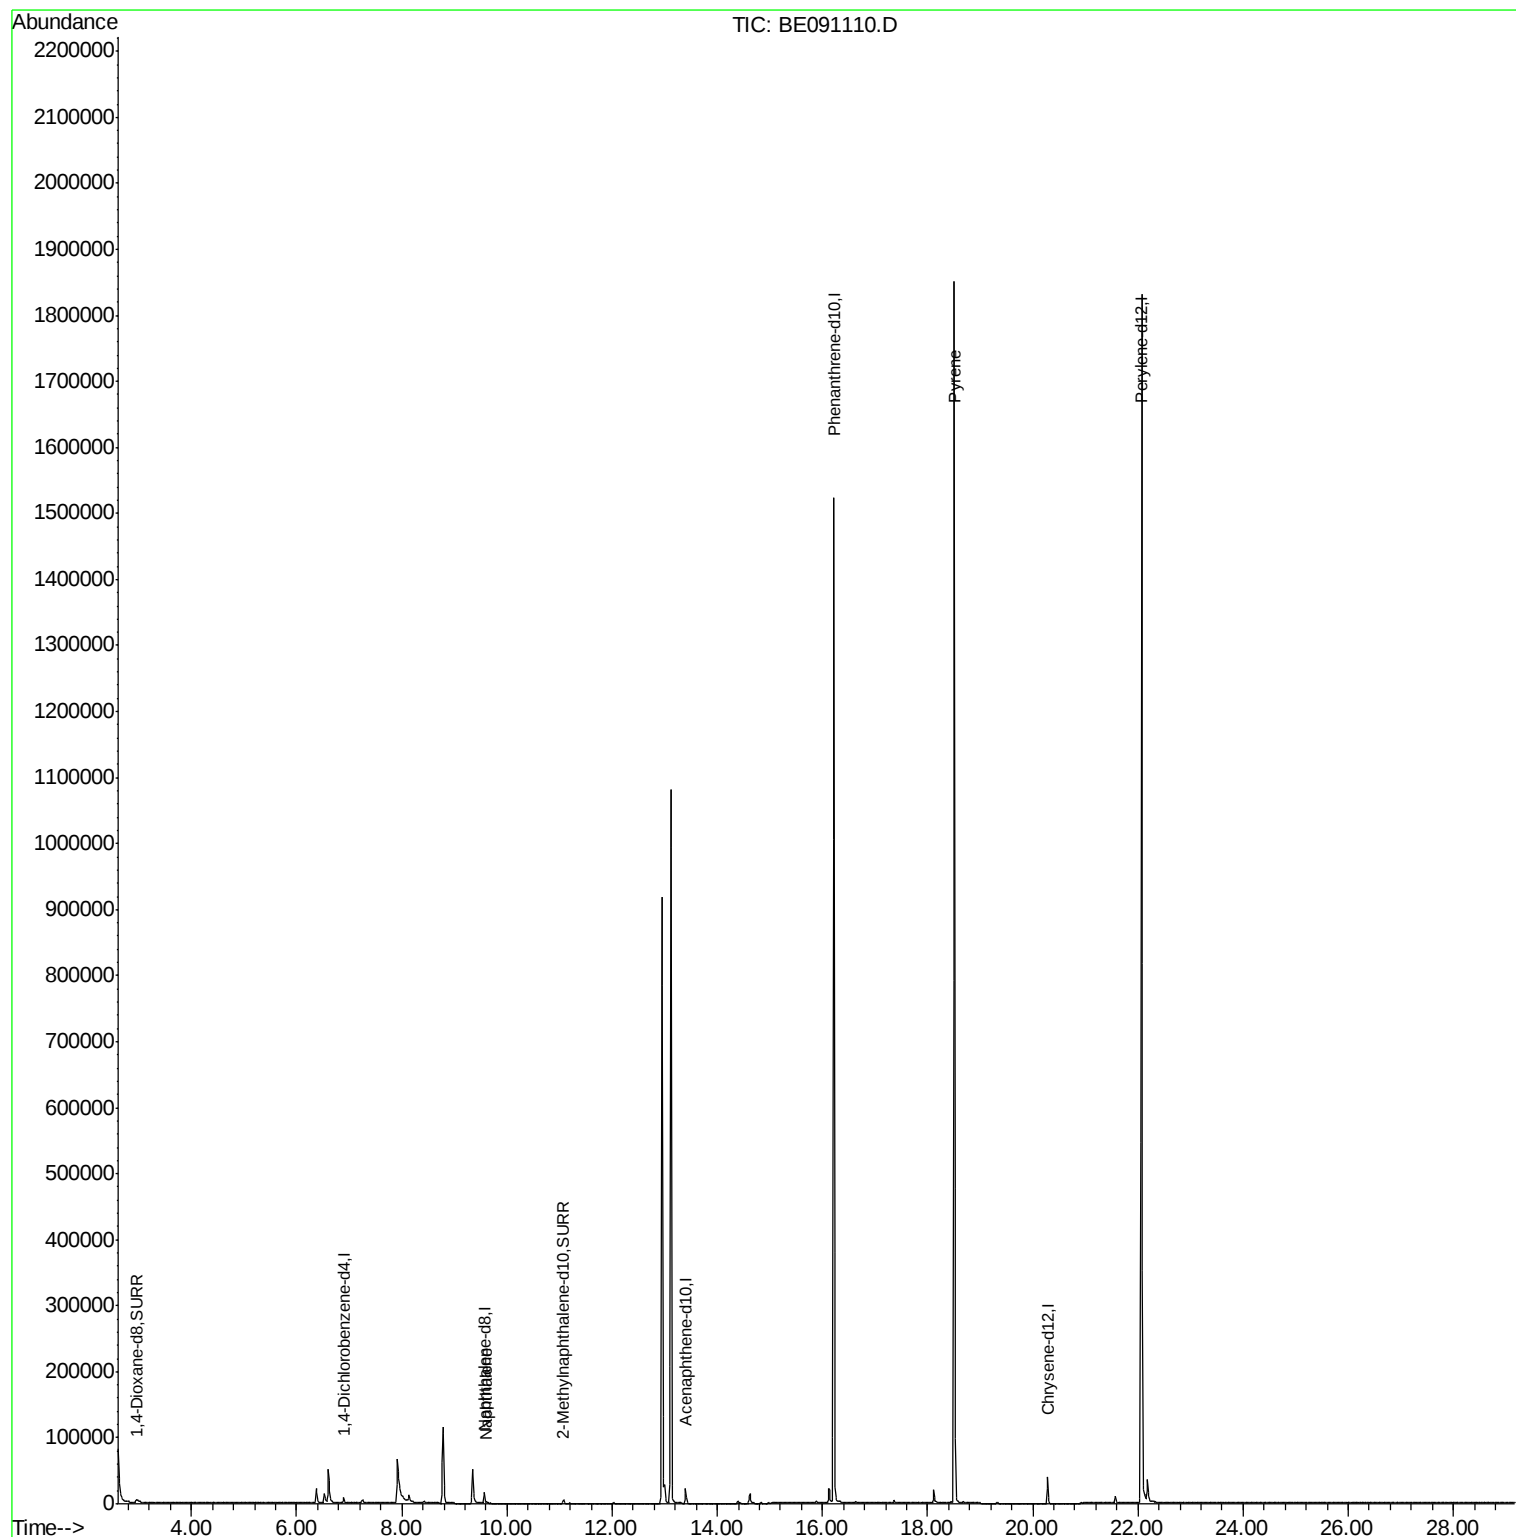

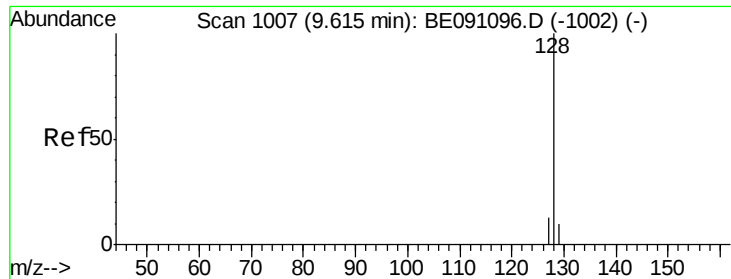

#5

Naphthalene

Concen: 0.05 ng/ul

RT: 9.62 min Scan# 1008

Delta R.T. 0.00 min

Lab File: BE091110.D

Acq: 11 Nov 2015 00:23

Instrument :

BNA_E

ClientSampleId :

D9KR2MSD


Tgt Ion:128 Resp: 2434

Ion Ratio Lower Upper

128 100

129 20.8 9.8 14.8#




127 16.9 10.7 16.1#

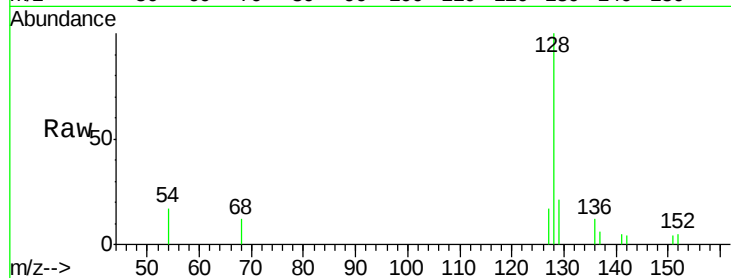

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

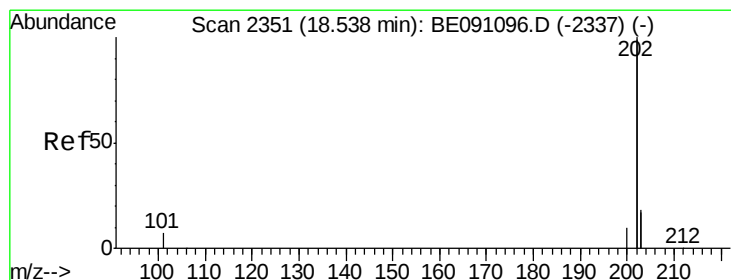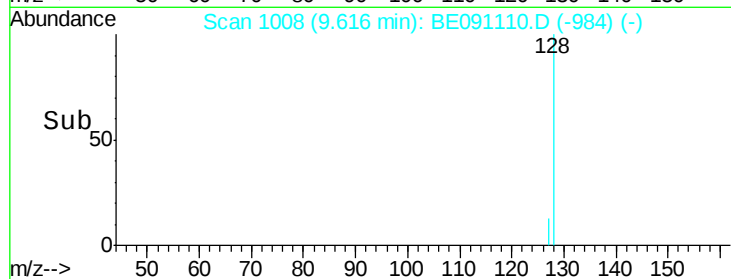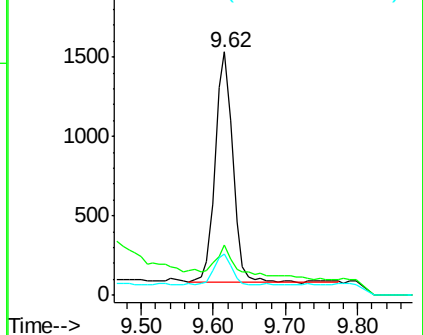

#19

Pyrene

Concen: 0.03 ng/ul

RT: 18.51 min Scan# 2348

Delta R.T. -0.03 min

Lab File: BE091110.D

Acq: 11 Nov 2015 00:23


Tgt Ion:202 Resp: 12902

Ion Ratio Lower Upper

202 100

200 1.8 18.0 27.0#

203 192.9 13.8 20.6#

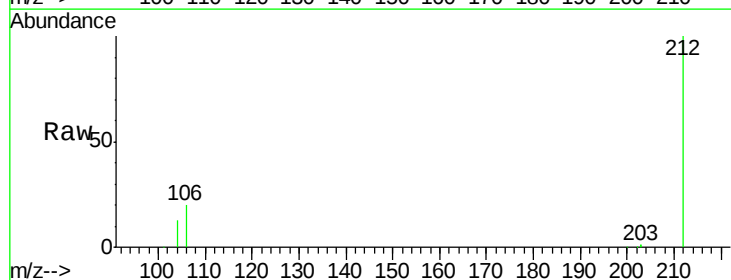

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

