




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091109.D
Acq On : 10 Nov 2015 23:47
Operator : UM/NP
Sample : G4308-15MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MS

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:46 PM

Quant Time: Nov 13 14:06:15 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

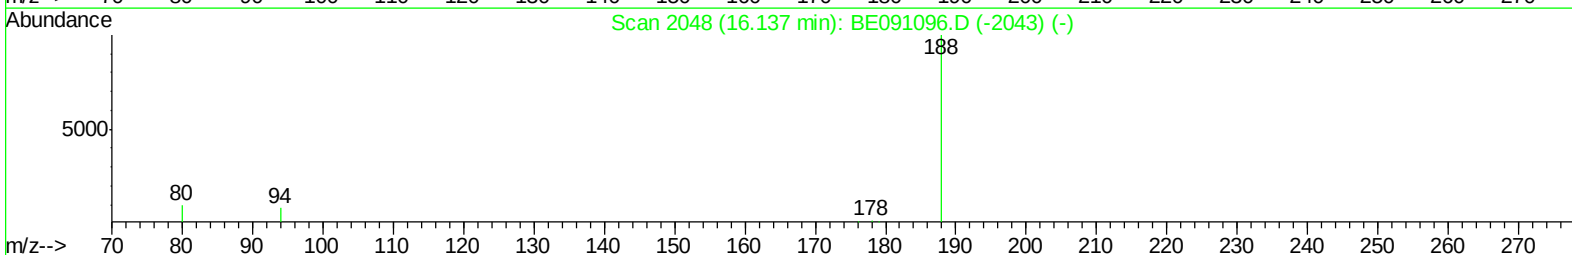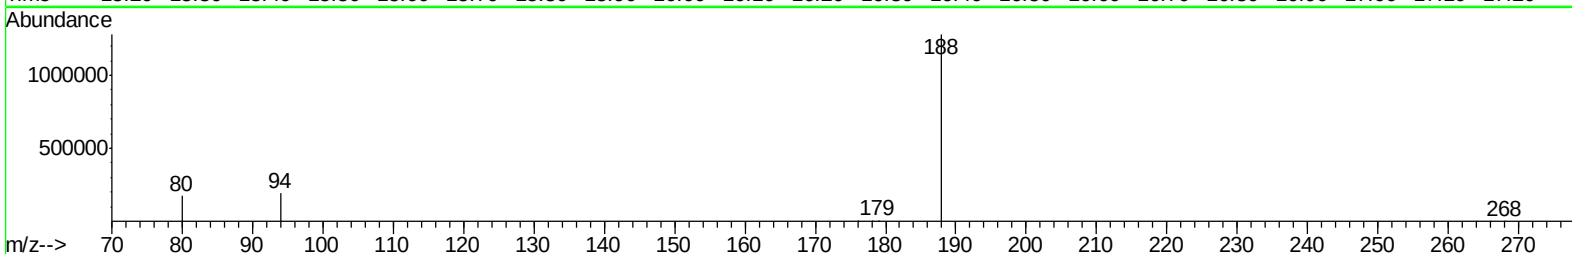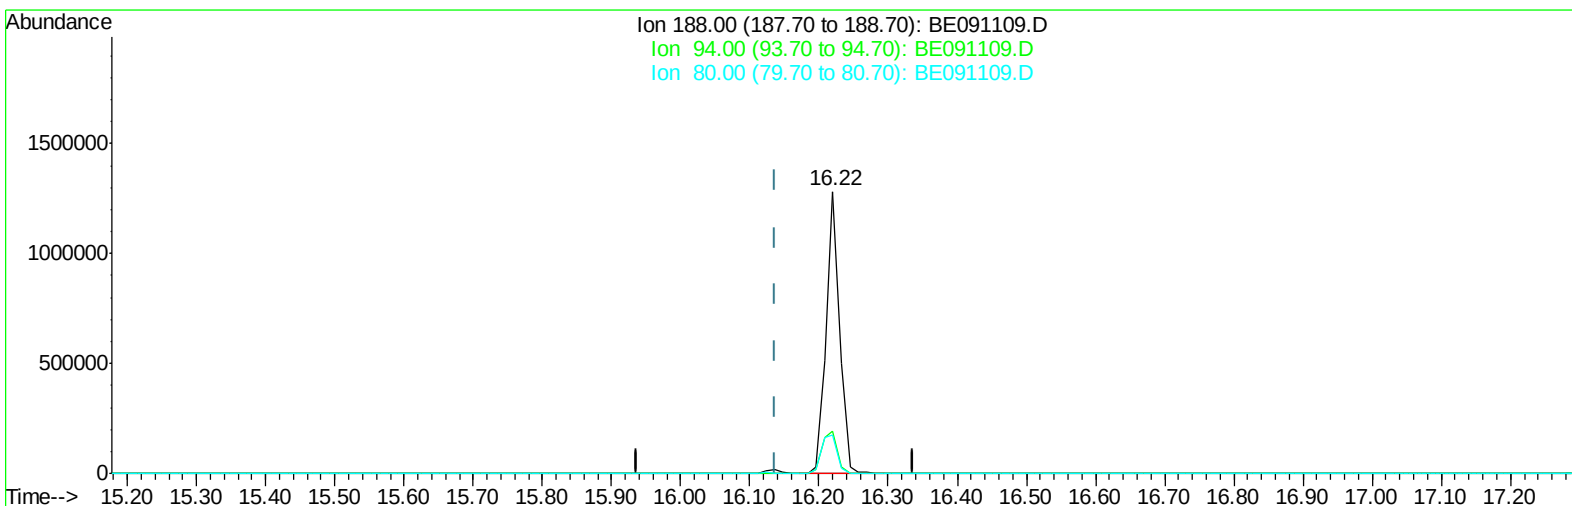

TIC: BE091109.D

(12) Phenanthrene-d10 (I)

16.220min (+0.083) 0.40ng/ul

response 1718160

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	14.94#
80.00	8.90	13.62#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091109.D
Acq On : 10 Nov 2015 23:47
Operator : UM/NP
Sample : G4308-15MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MS

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:46 PM

Quant Time: Nov 13 14:06:15 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

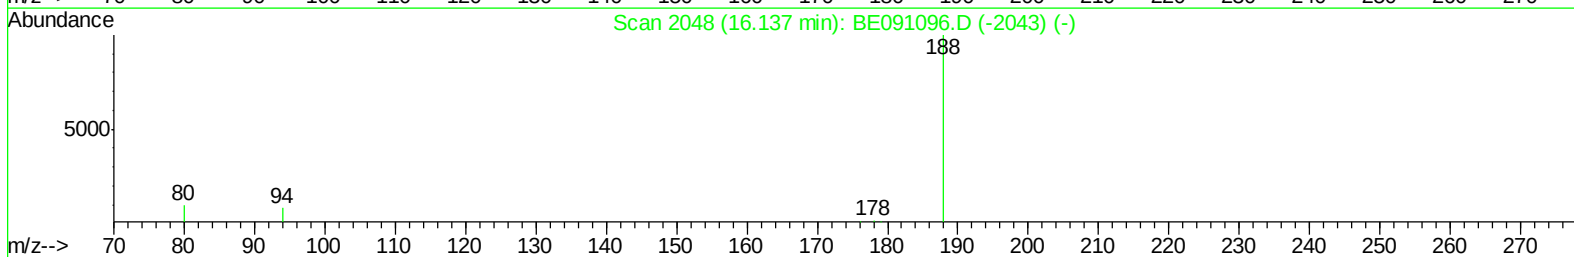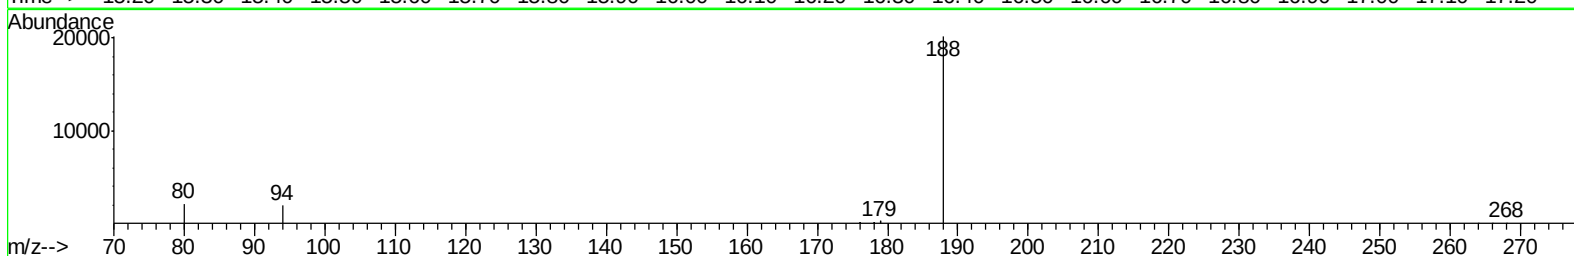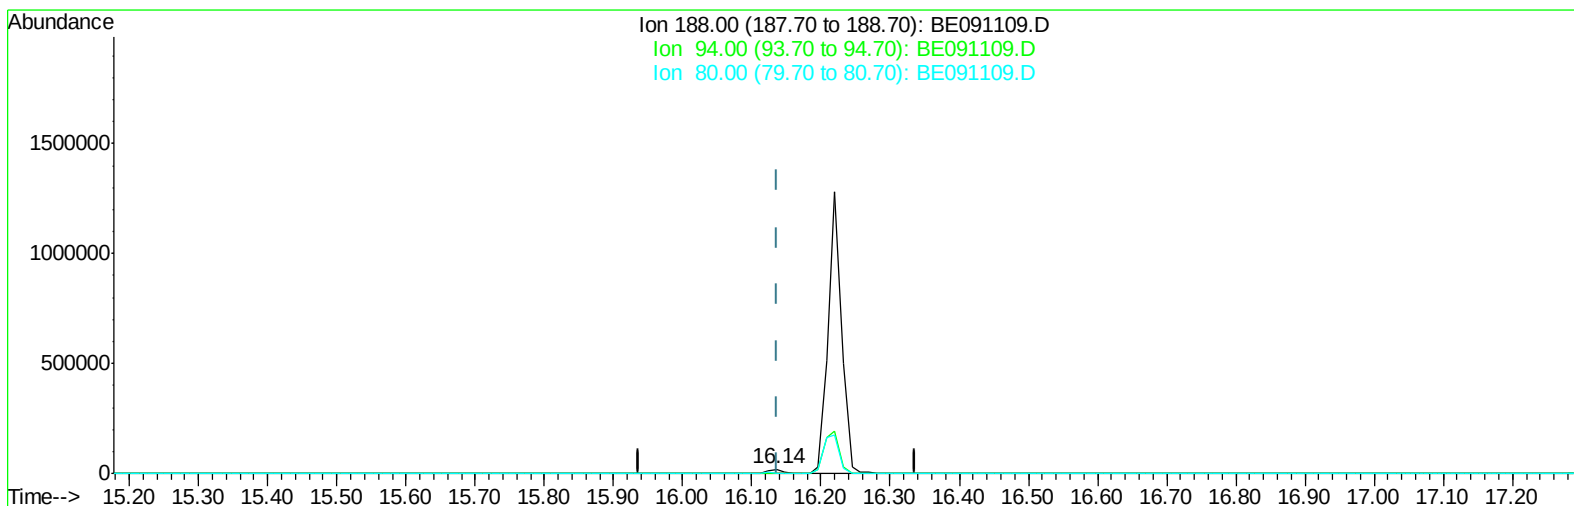

TIC: BE091109.D

(12) Phenanthrene-d10 (I)

16.136min (-0.002) 0.40ng/ul m

response 28766

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	9.78
80.00	8.90	10.86#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091109.D
Acq On : 10 Nov 2015 23:47
Operator : UM/NP
Sample : G4308-15MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MS

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:46 PM

Quant Time: Nov 13 15:01:35 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

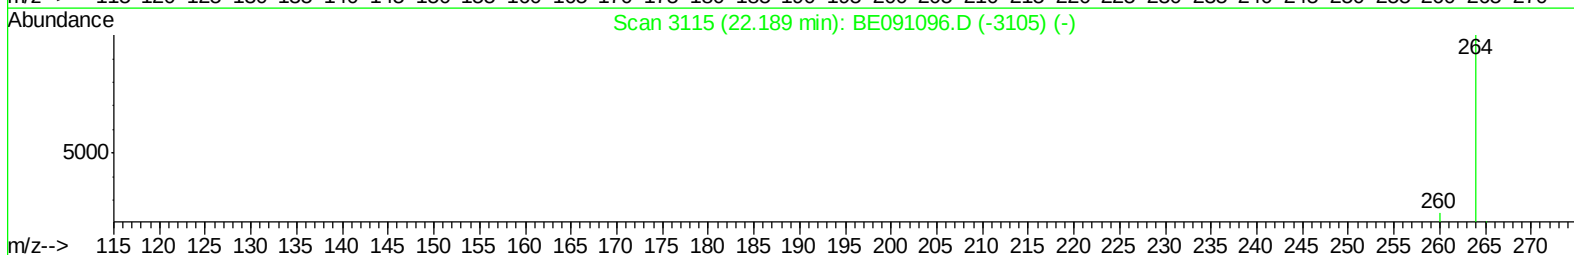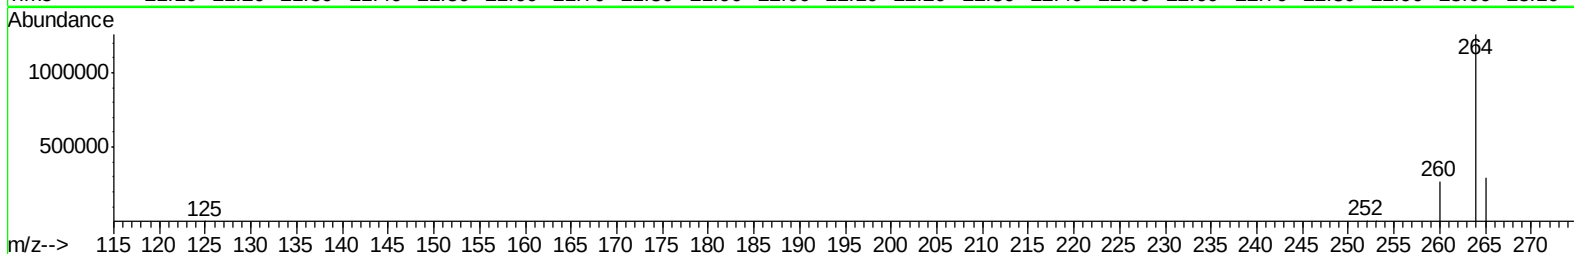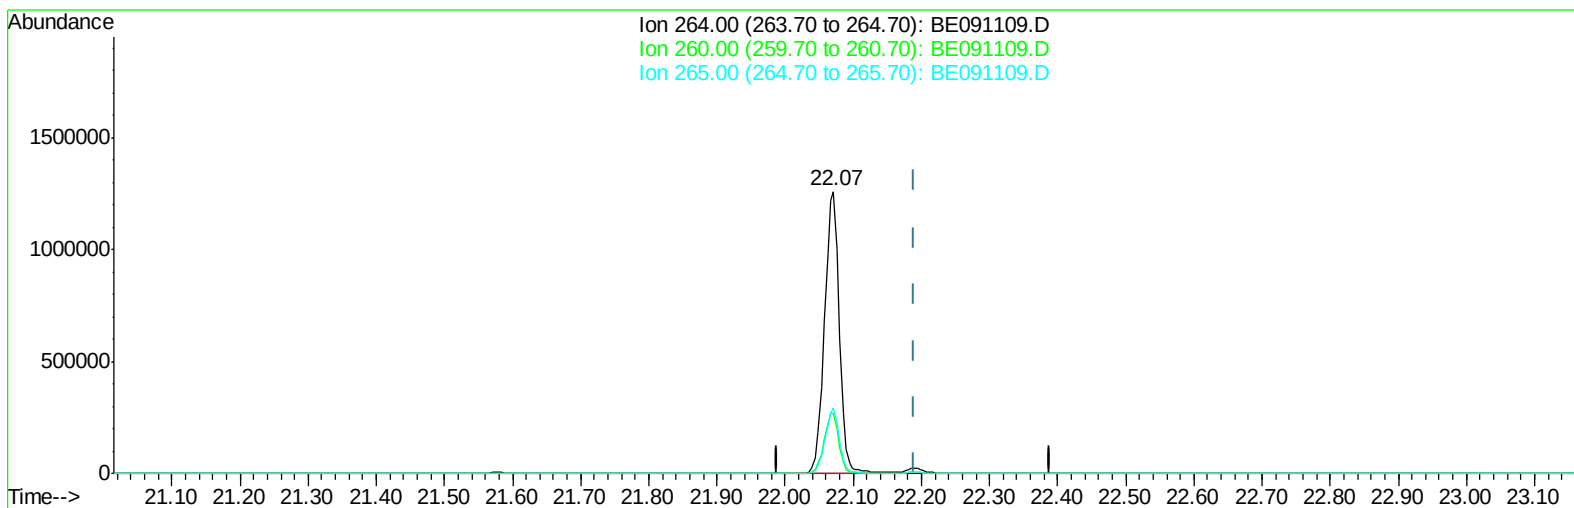

TIC: BE091109.D

(22) Perylene-d12 (I)

22.071min (-0.118) 0.40ng/ul

response 1902030

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	21.30#
265.00	34.70	23.21#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091109.D
Acq On : 10 Nov 2015 23:47
Operator : UM/NP
Sample : G4308-15MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MS

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:46 PM

Quant Time: Nov 13 15:01:35 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

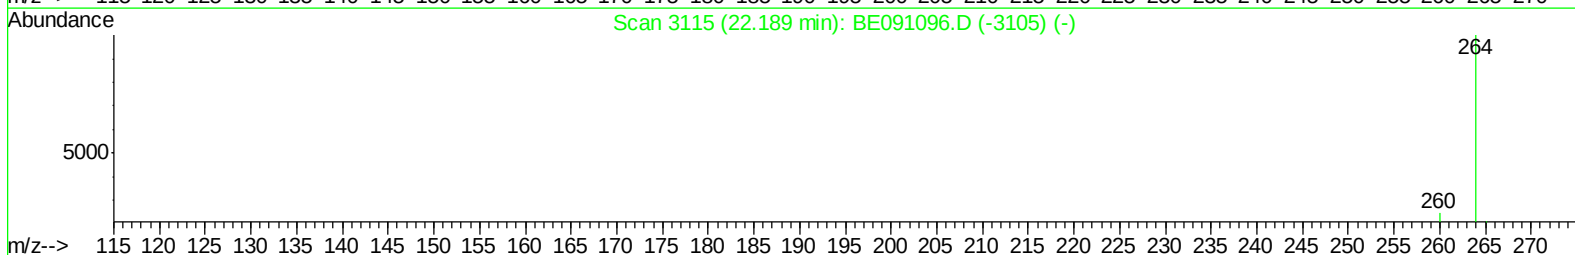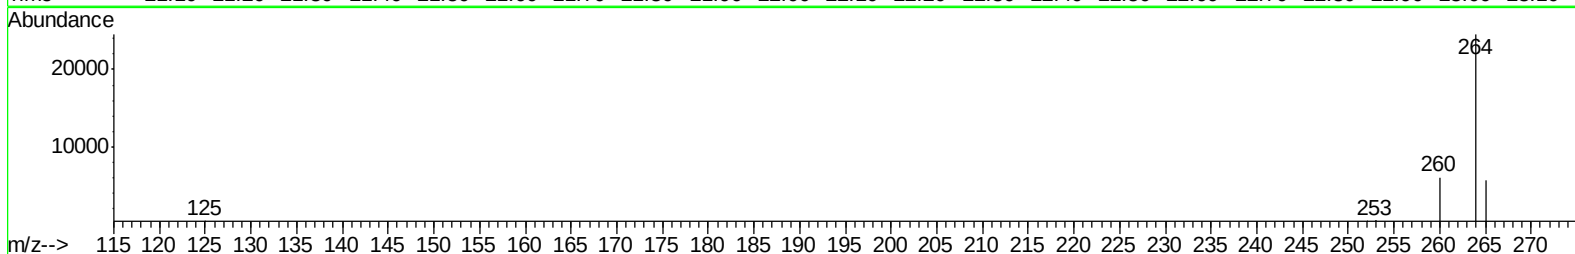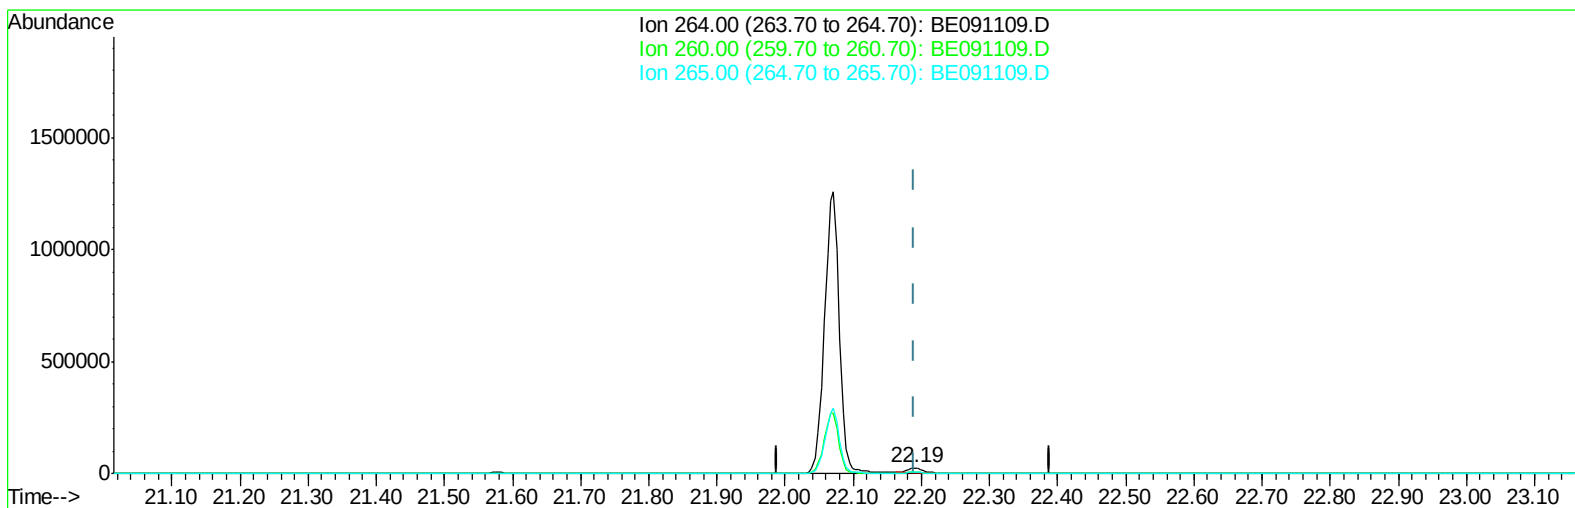

TIC: BE091109.D

(22) Perylene-d12 (I)

22.190min (+0.000) 0.40ng/ul m

response 29486

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	24.55
265.00	34.70	22.82#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111015\
Data File : BE091110.D
Acq On : 11 Nov 2015 00:23
Operator : UM/NP
Sample : G4308-16MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR2MS

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:46 PM

Quant Time: Nov 13 14:06:21 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

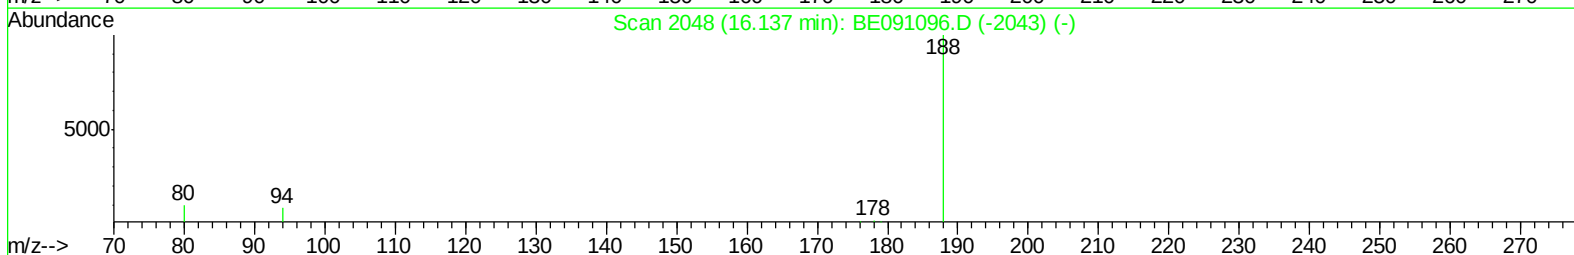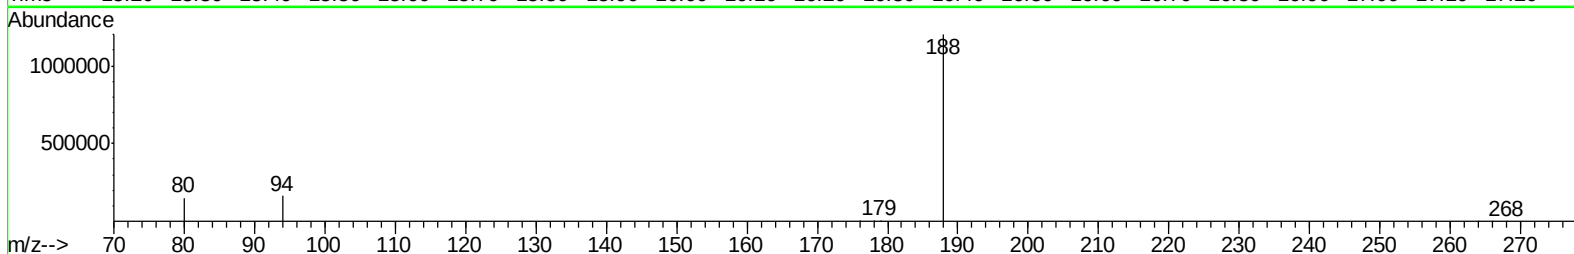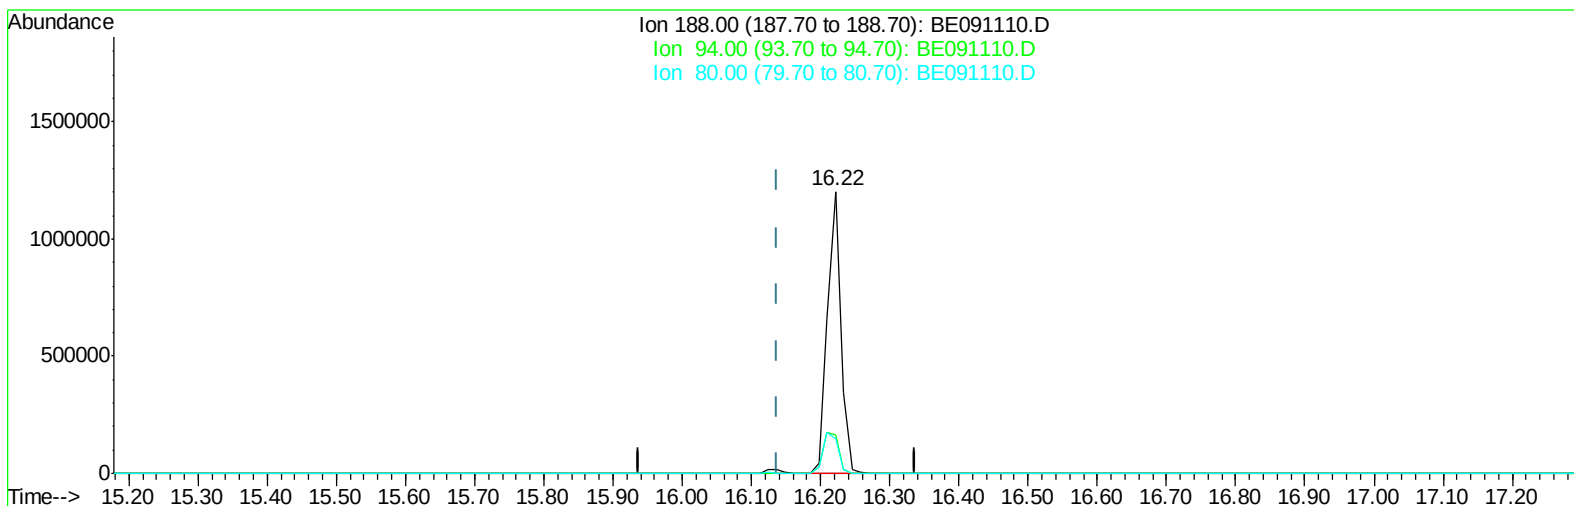

TIC: BE091110.D

(12) Phenanthrene-d10 (I)

16.221min (+0.084) 0.40ng/ul

response 1653871

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	13.66#
80.00	8.90	12.34#
0.00	0.00	0.00