

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111015\
 Data File : BE091101.D
 Acq On : 10 Nov 2015 18:55
 Operator : UM/NP
 Sample : G4308-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KR6

Manual Integrations
 APPROVED

Mmdadoda
 11/13/2015 6:29:32 PM

Quant Time: Nov 13 14:39:06 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3412	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	19333	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	11956	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.14	188	28595m	0.40	ng/ul	0.00
18) Chrysene-d12	20.28	240	34300	0.40	ng/ul	0.00
22) Perylene-d12	22.19	264	31448m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.96	96	4895	1.99	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.07	152	7610	0.29	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	21910	0.27	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.62	128	2070	0.04	ng/ul#	Ovalue 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111015\
Data File : BE091101.D
Acq On : 10 Nov 2015 18:55
Operator : UM/NP
Sample : G4308-07
Misc :
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
D9KR6

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:32 PM

Quant Time: Nov 13 14:39:06 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

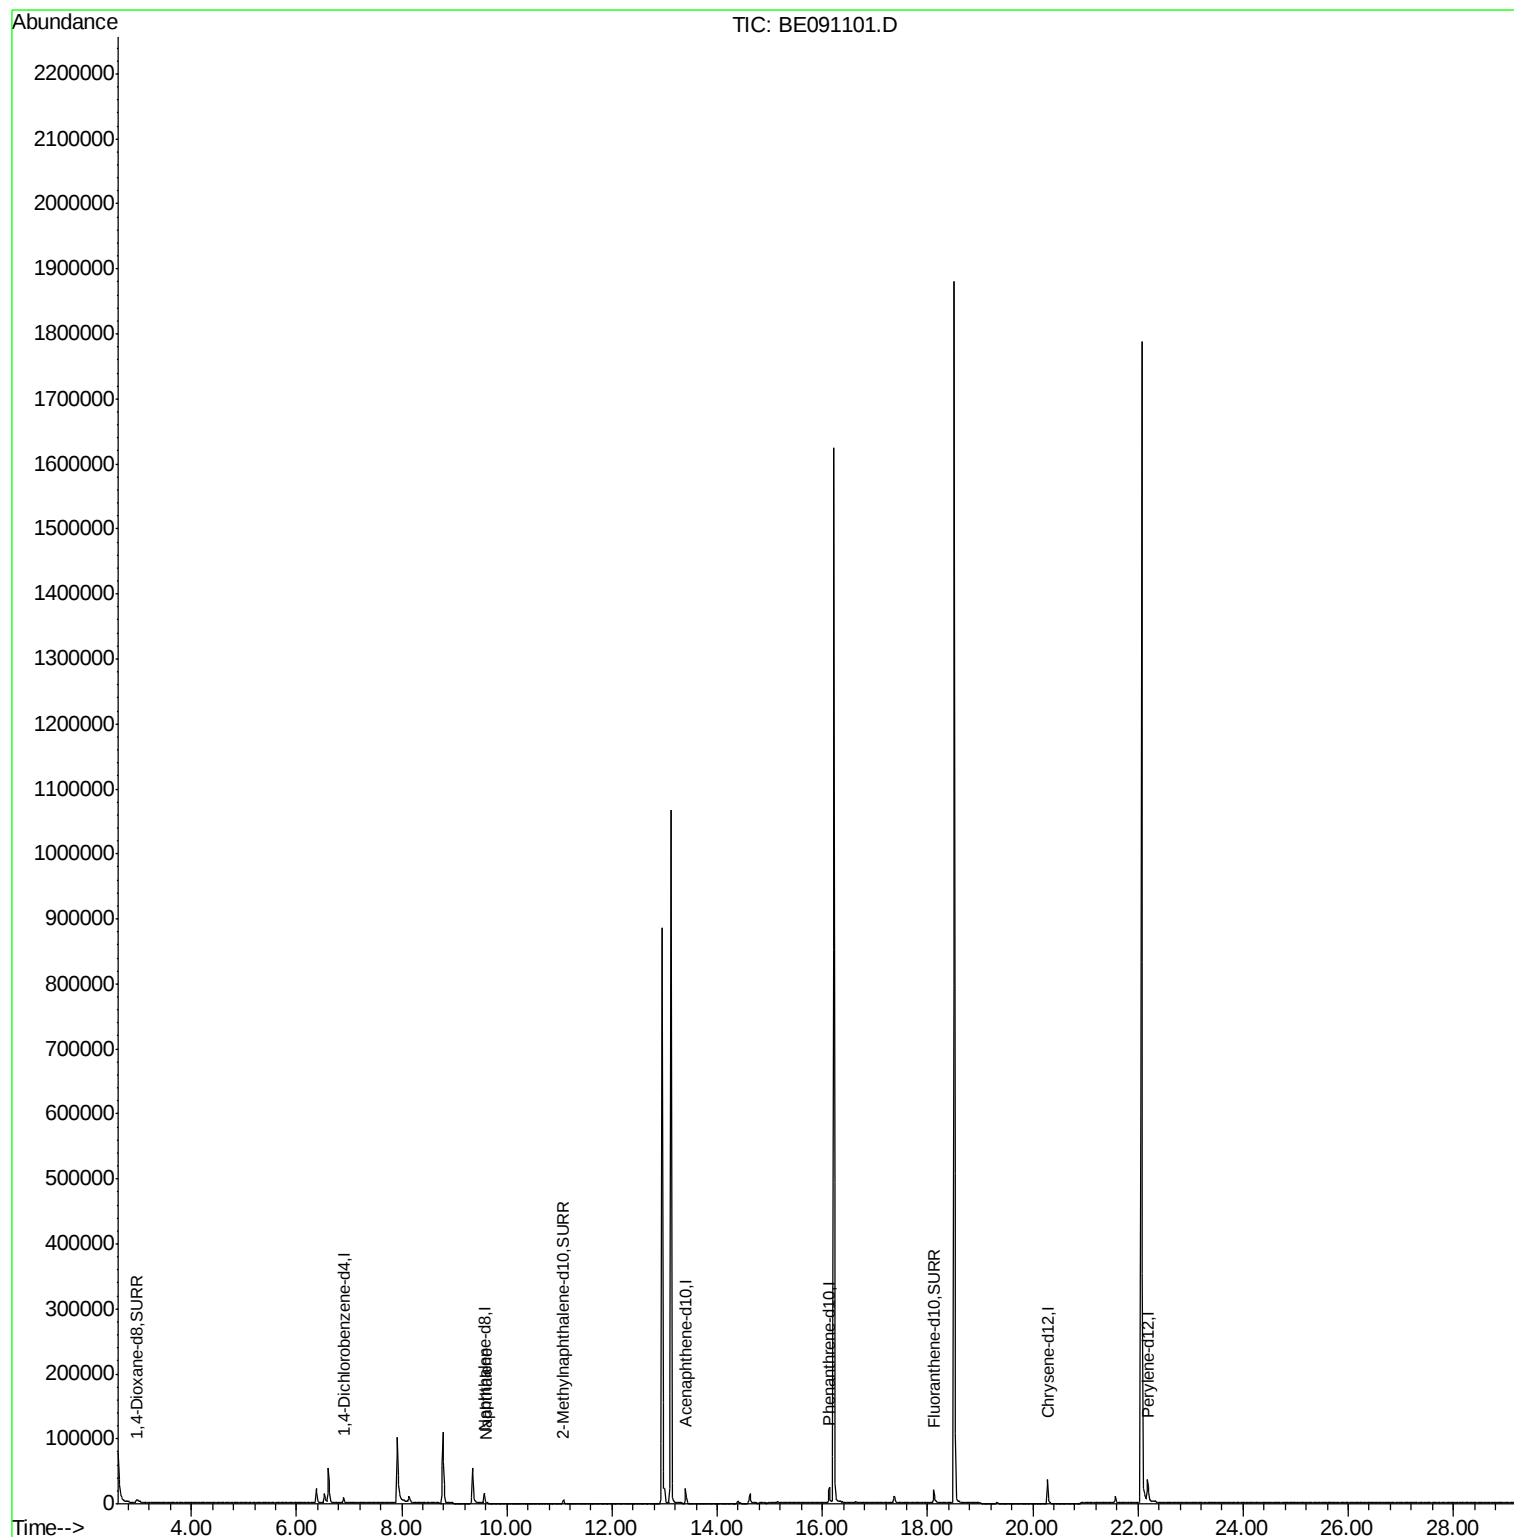

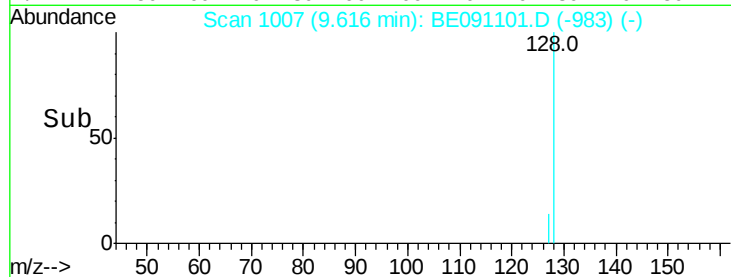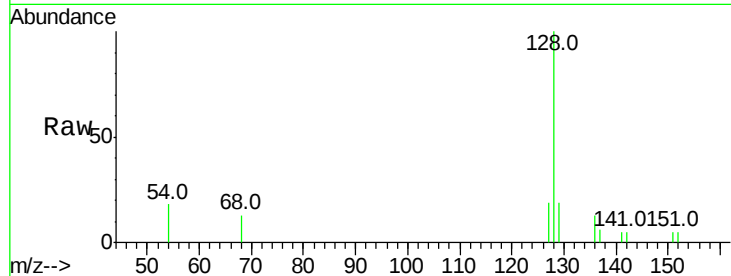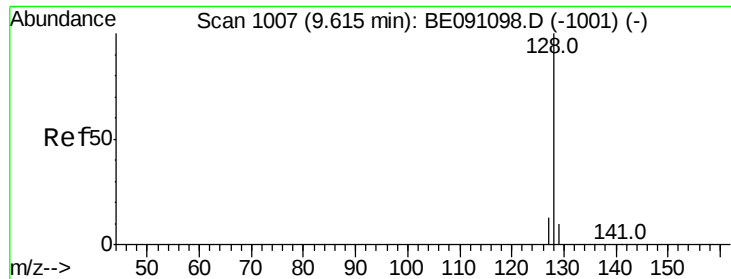

#5

Naphthalene

Concen: 0.04 ng/ul

RT: 9.62 min Scan# 1007

Delta R.T. 0.00 min

Lab File: BE091101.D

Acq: 10 Nov 2015 18:55

Tot Ion:	128	Resp:	2070
Ion Ratio	Lower	Upper	
128	100		
129	19.3	9.8	14.8#
127	18.8	10.7	16.1#

Instrument :

BNA_E

ClientSampleId :

D9KR6

Manual Integrations
APPROVED

Mmdadoda
11/13/2015 6:29:32 PM

