

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
 Data File : BE094796.D
 Acq On : 9 Nov 2017 9:54
 Operator : SJ/JU
 Sample : PB103704BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 09 12:49:22 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 01:37:48 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1336	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	8234	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4772	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.28
16) Chrysene-d12	21.44	240	9521	0.40	ng/ul	0.00
20) Perylene-d12	23.80	264	494827	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	4088	0.31	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	9566	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	920	0.053	ng/ul#	22
17) Pyrene	19.64	202	1139	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 09 12:49:22 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

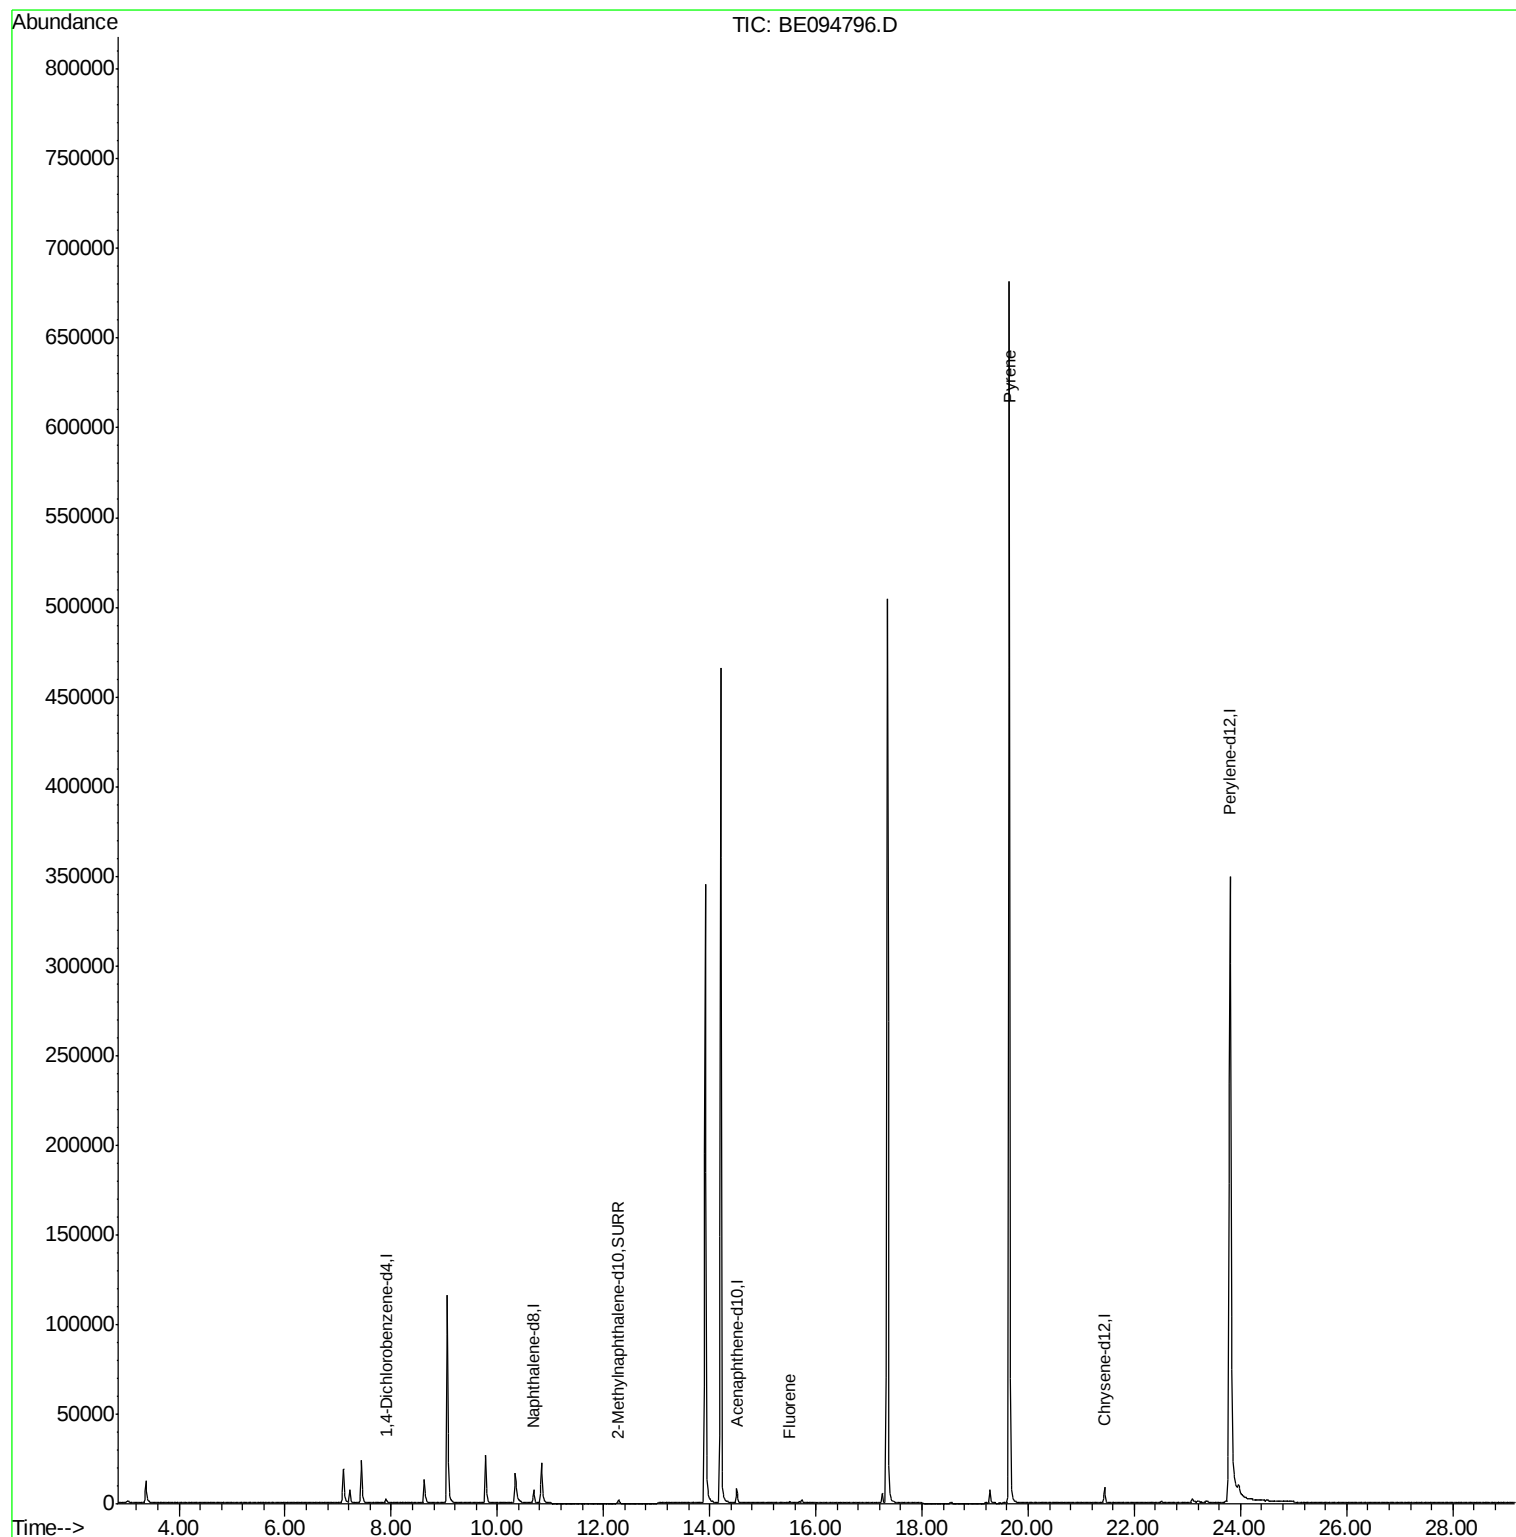

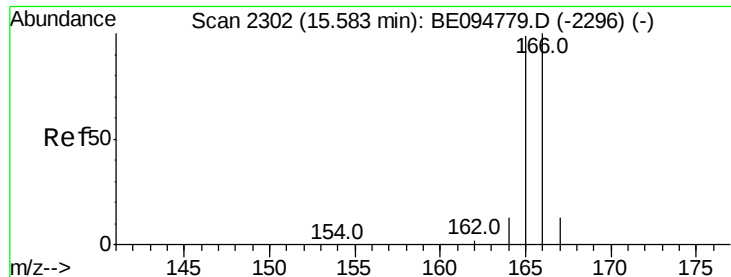

#9

Fluorene

Concen: 0.053 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.08 min

Lab File: BE094796.D

Acq: 9 Nov 2017 9:54

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 920

Ion Ratio Lower Upper


166 100

165 11.2 73.4 110.2#



167 39.5 14.6 22.0#

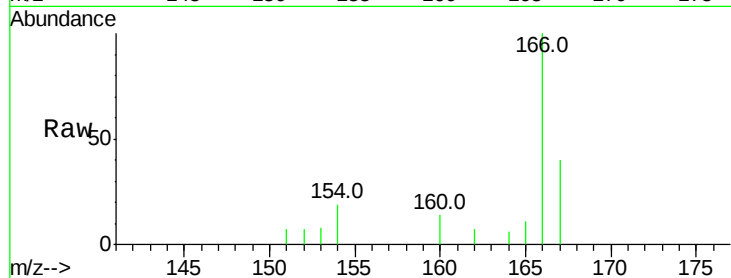

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

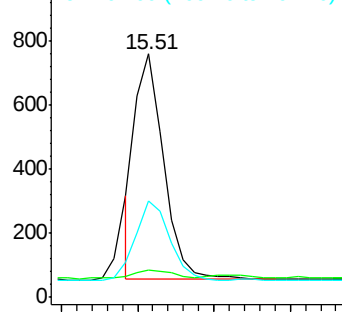

Time--> 15.45 15.50 15.55 15.60

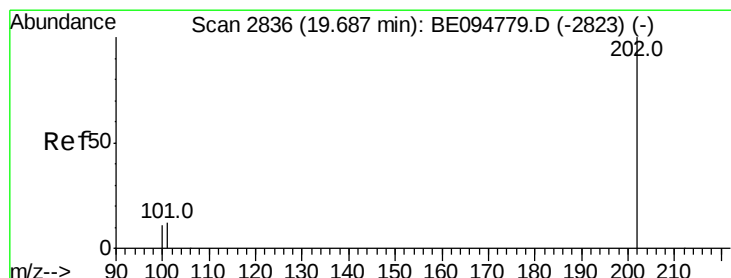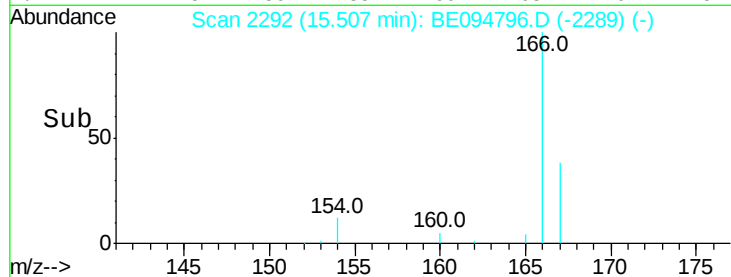

#17

Pyrene

Concen: 0.039 ng/ul

RT: 19.64 min Scan# 2826

Delta R.T. -0.04 min

Lab File: BE094796.D

Acq: 9 Nov 2017 9:54


Tgt Ion:202 Resp: 1139

Ion Ratio Lower Upper


202 100

101 147.7 18.2 27.4#

100 793.9 15.6 23.4#

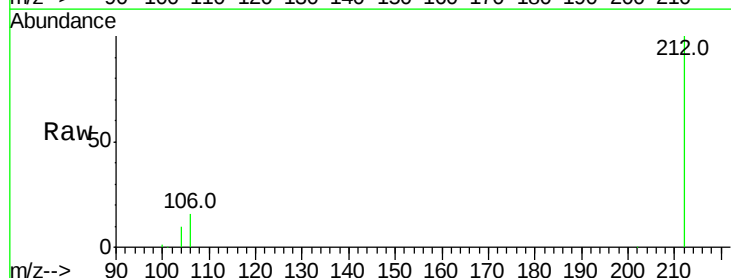

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

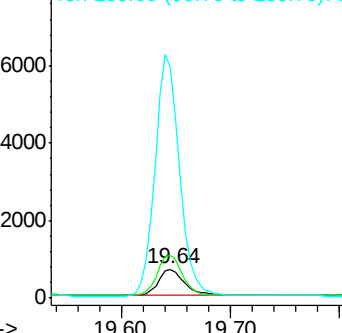

Time--> 19.60 19.70

