

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
 Data File : BE094797.D
 Acq On : 9 Nov 2017 10:29
 Operator : SJ/JU
 Sample : PB103554BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 09 12:49:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 01:37:48 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1198	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	7130	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4179	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.28
16) Chrysene-d12	21.44	240	8171	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	519402	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	4284	0.37	ng/ul	-0.02
14) Fluoranthene-d10	19.28	212	9834	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	920	0.060	ng/ul#	22
17) Pyrene	19.65	202	1164	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094797.D
Acq On : 9 Nov 2017 10:29
Operator : SJ/JU
Sample : PB103554BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 09 12:49:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration




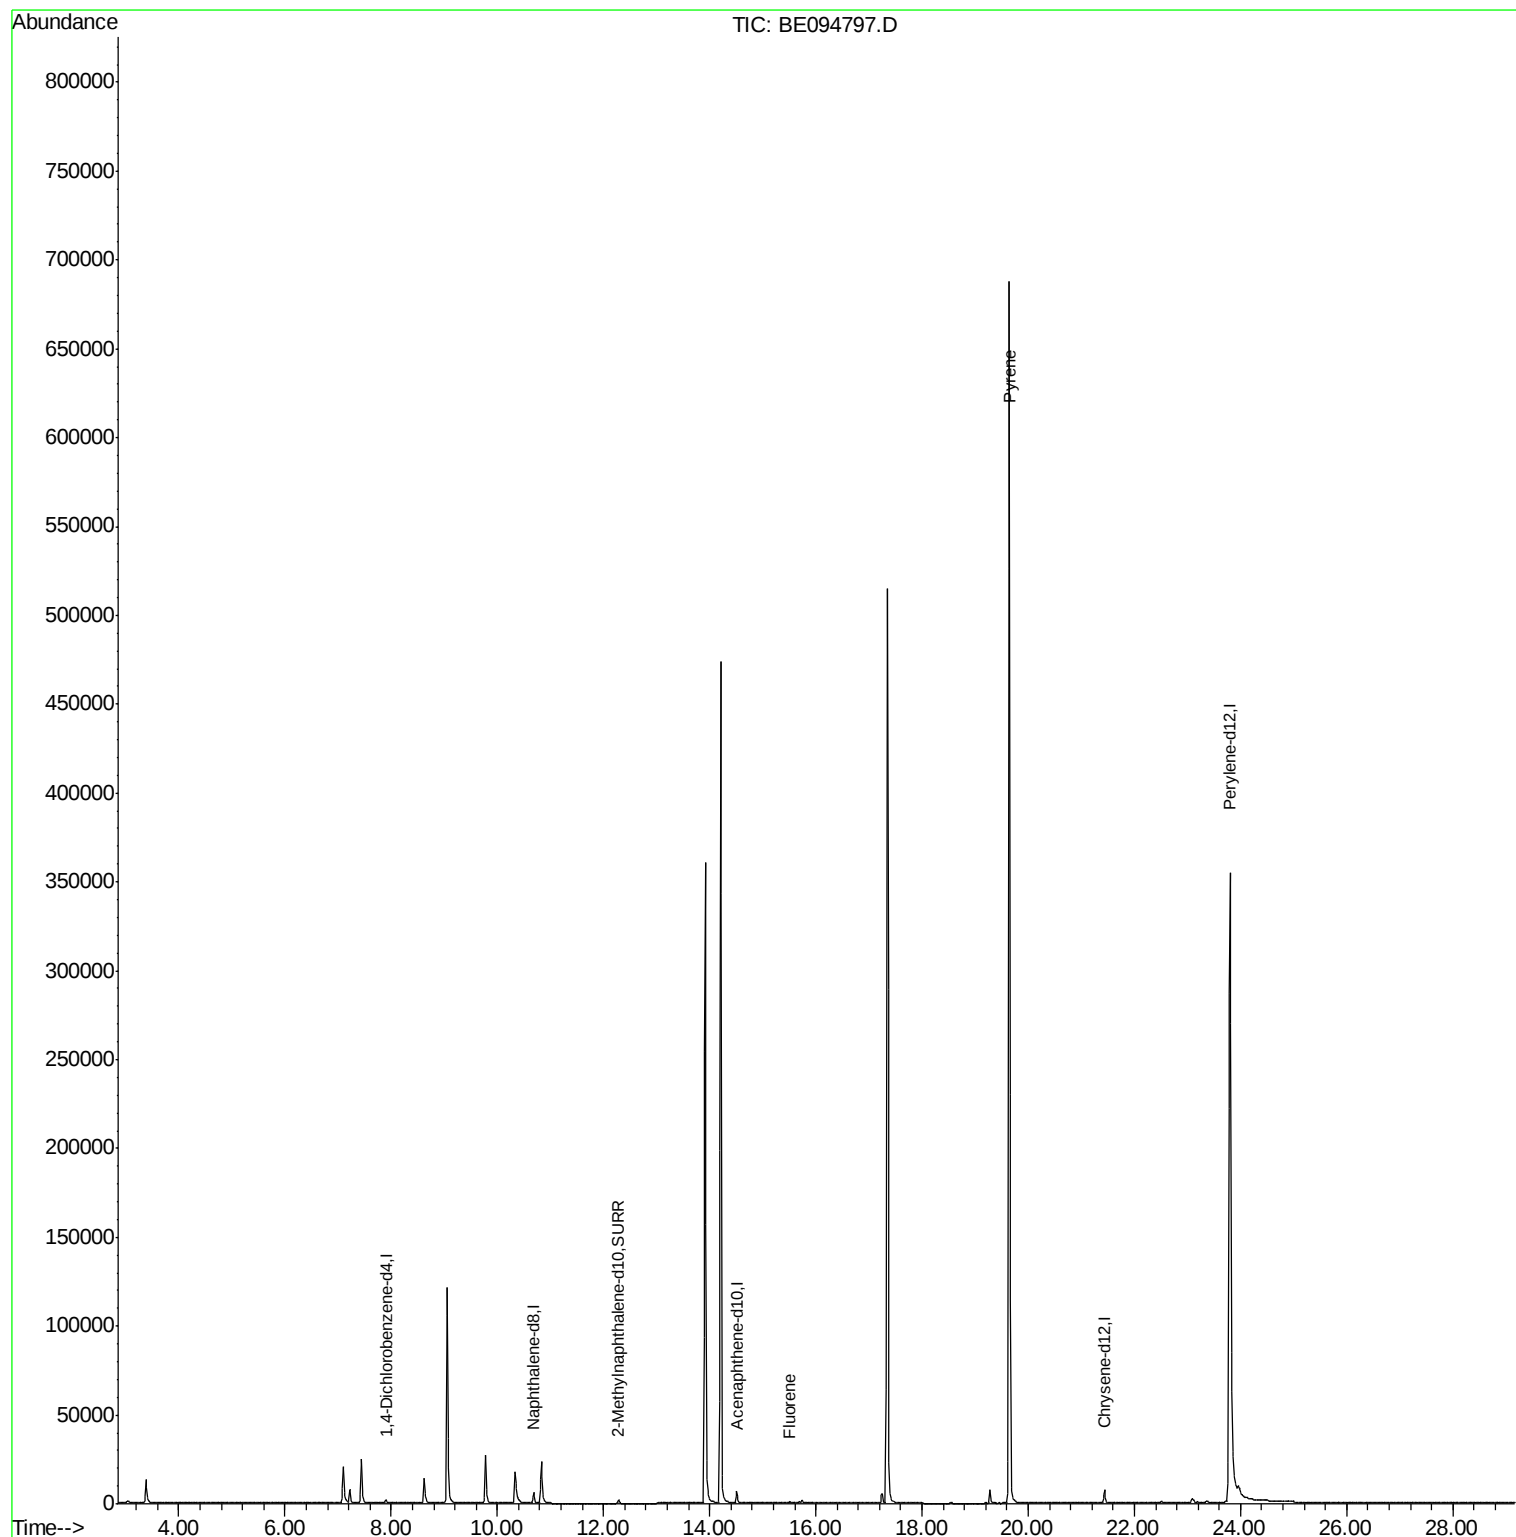


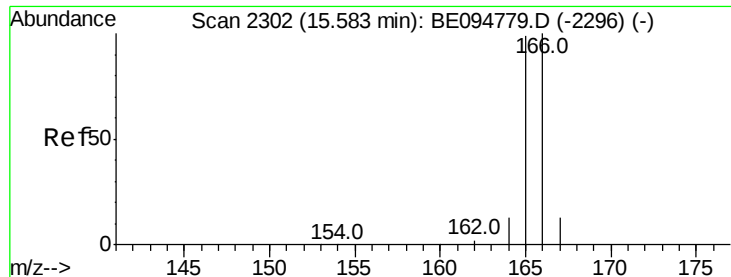

#9
Fluorene
 Concen: 0.060 ng/ul
 RT: 15.51 min Scan# 2292
 Delta R.T. -0.07 min
 Lab File: BE094797.D
 Acq: 9 Nov 2017 10:29

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 920
 Ion Ratio Lower Upper
 166 100
 165 11.8 73.4 110.2#
 167 40.9 14.6 22.0#

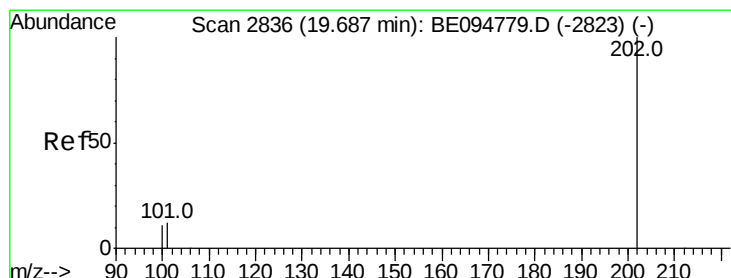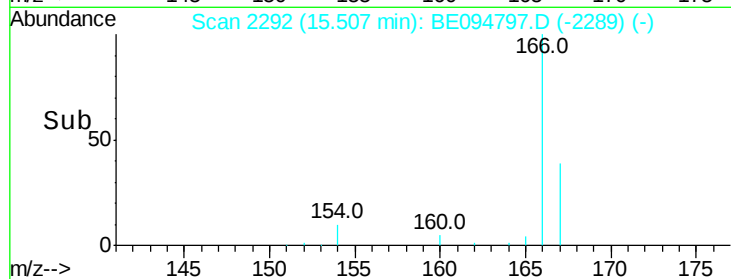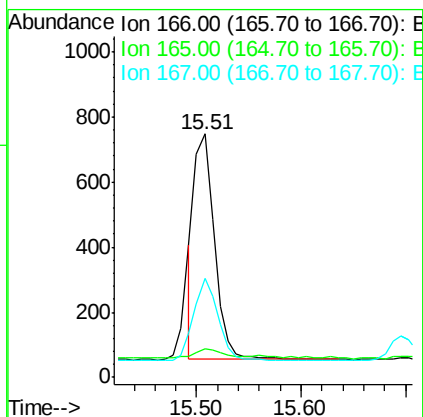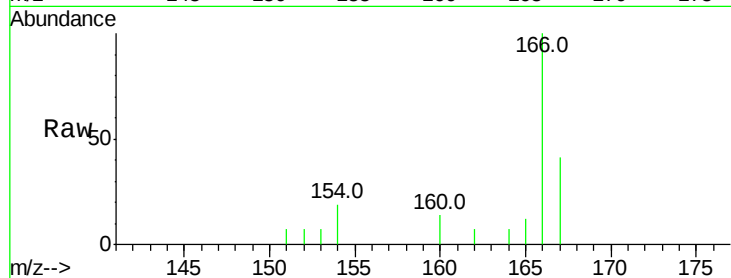

#17
Pyrene
 Concen: 0.046 ng/ul
 RT: 19.65 min Scan# 2827
 Delta R.T. -0.04 min
 Lab File: BE094797.D
 Acq: 9 Nov 2017 10:29

Tgt Ion:202 Resp: 1164
 Ion Ratio Lower Upper
 202 100
 101 155.1 18.2 27.4#
 100 805.8 15.6 23.4#

