

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
 Data File : BE094799.D
 Acq On : 9 Nov 2017 11:41
 Operator : SJ/JU
 Sample : I6120-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 09 12:50:03 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 01:37:48 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1517	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	9215	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	5303	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.26	188	10960	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	11067	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	20871	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3330	0.22	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	7881	0.24	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	1050	0.031	ng/ul#	1
23) Benzo(a)pyrene	23.80	252	1889	0.032	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094799.D
Acq On : 9 Nov 2017 11:41
Operator : SJ/JU
Sample : I6120-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 09 12:50:03 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

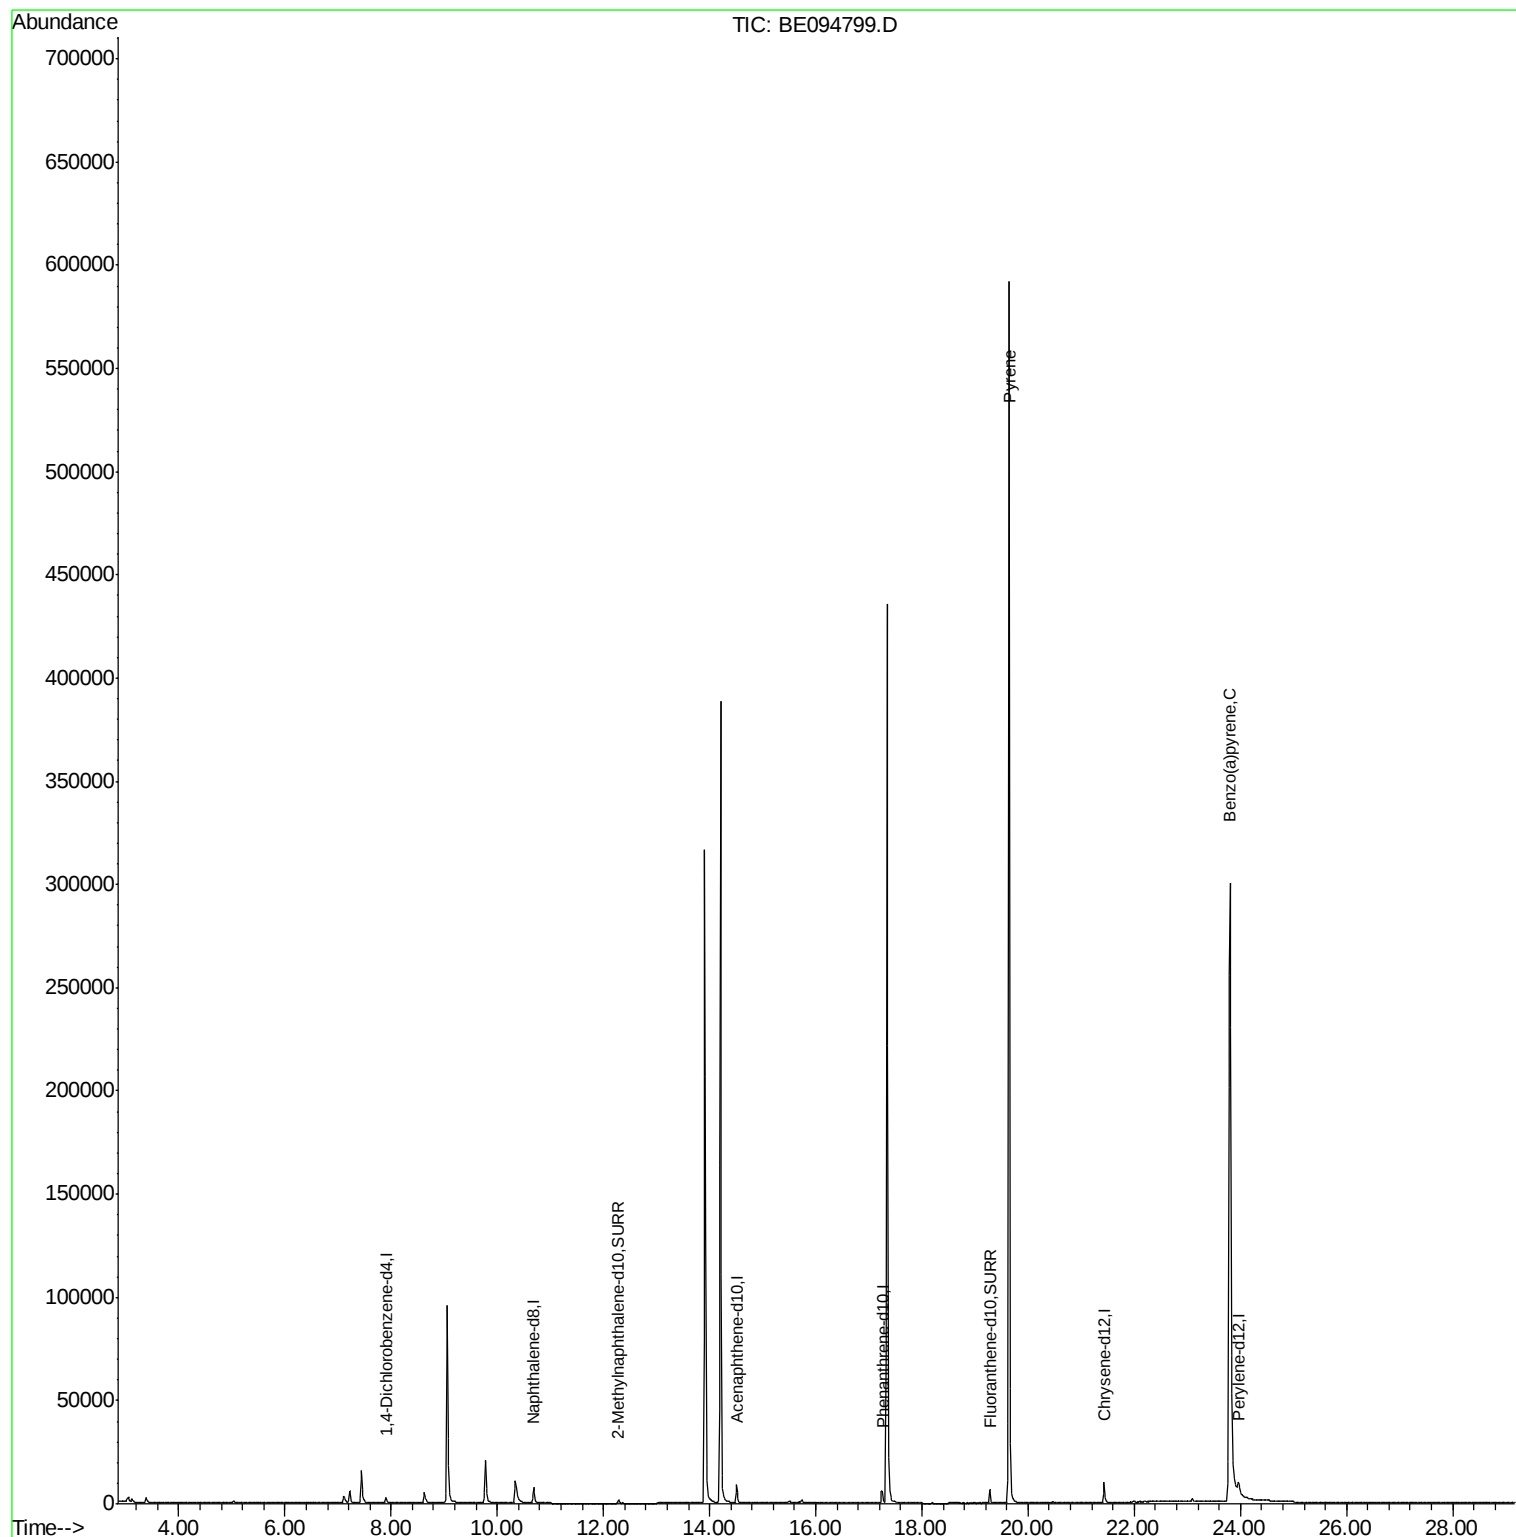

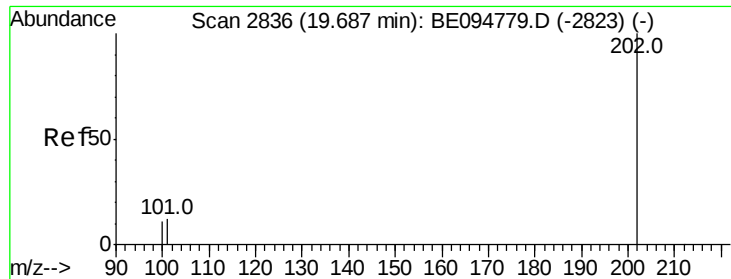

#17

Pvrene

Concen: 0.031 ng/ul

RT: 19.64 min Scan# 2826

Delta R.T. -0.04 min

Lab File: BE094799.D

Acq: 9 Nov 2017 11:41

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 1050

Ion Ratio Lower Upper

202 100

101 152.8 18.2 27.4#




100 819.8 15.6 23.4#

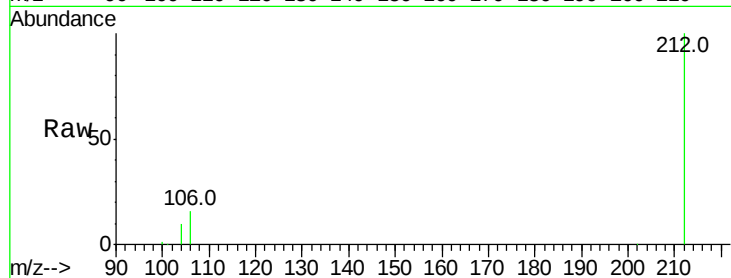

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

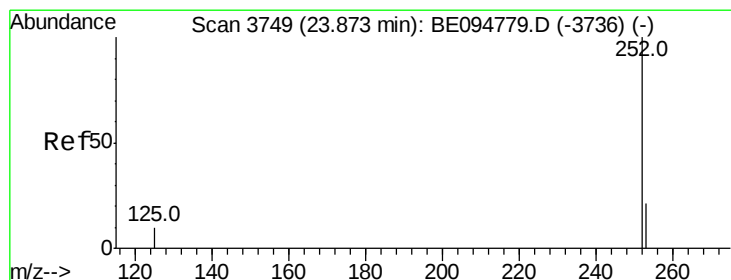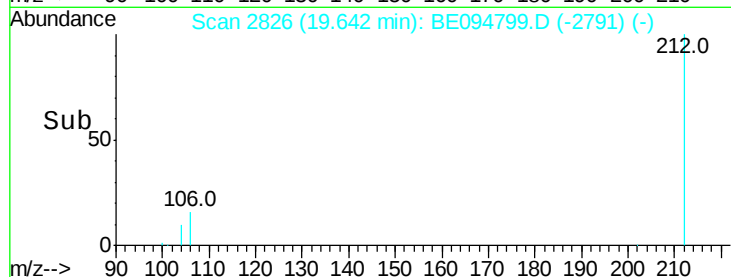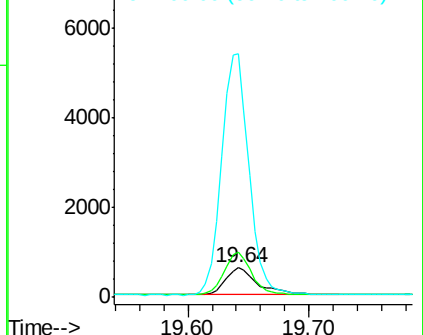

#23

Benzo(a)pyrene

Concen: 0.032 ng/ul

RT: 23.80 min Scan# 3732

Delta R.T. -0.06 min

Lab File: BE094799.D

Acq: 9 Nov 2017 11:41


Tgt Ion:252 Resp: 1889

Ion Ratio Lower Upper

252 100

253 51.0 28.5 42.7#

125 44.6 18.1 27.1#

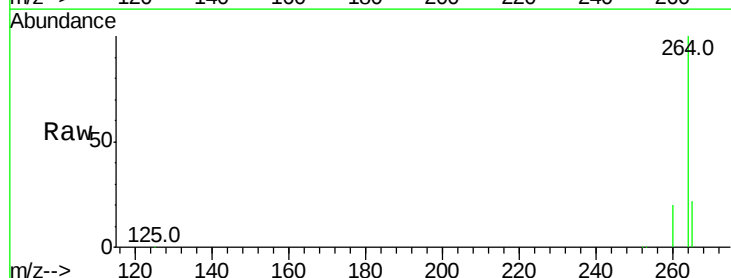

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

