




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 12:49:22 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

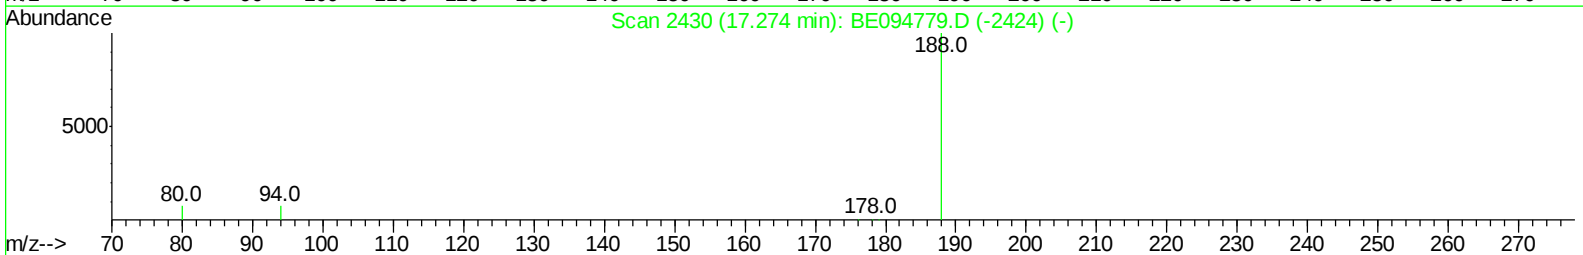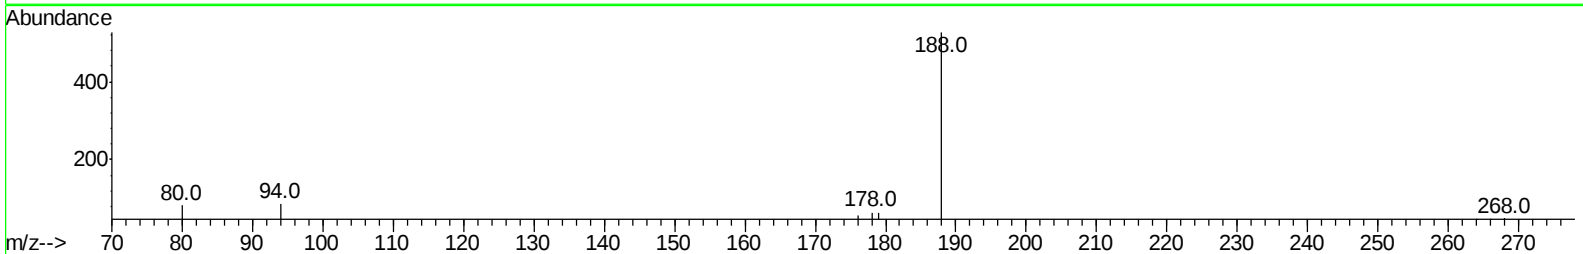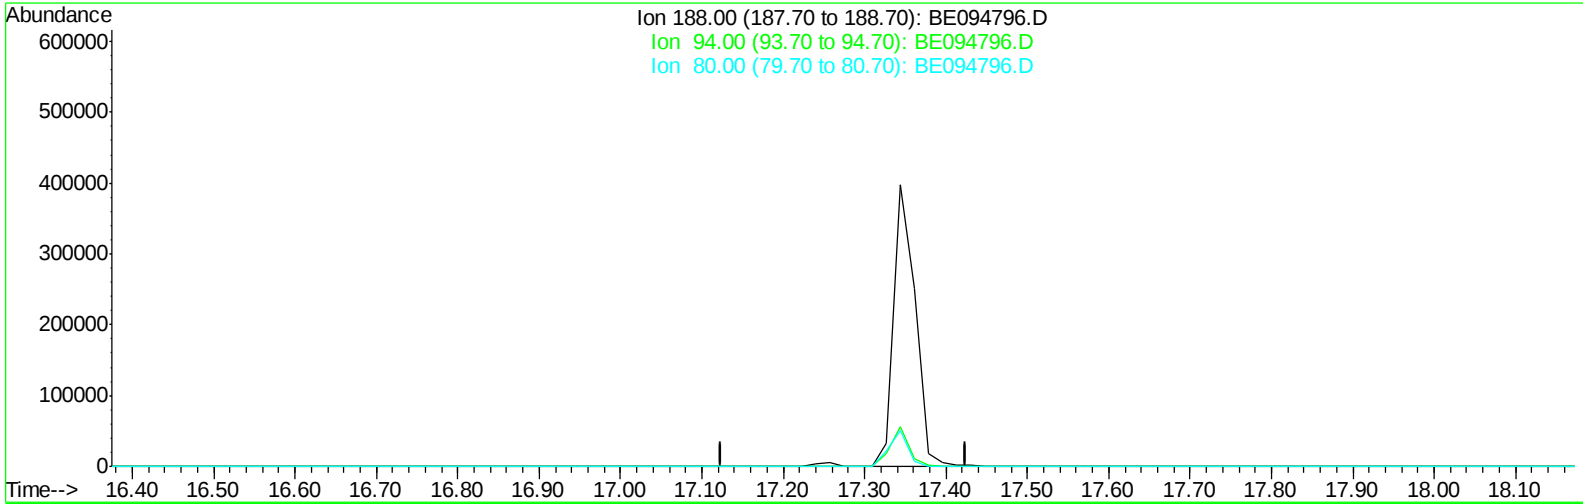

TIC: BE094796.D

(10) Phenanthrene-d10 (I)

17.275min (-17.275) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 12:49:22 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

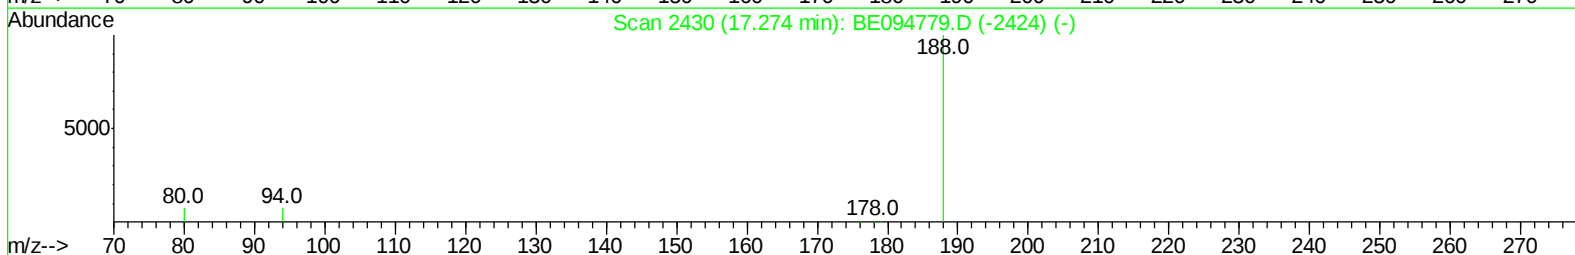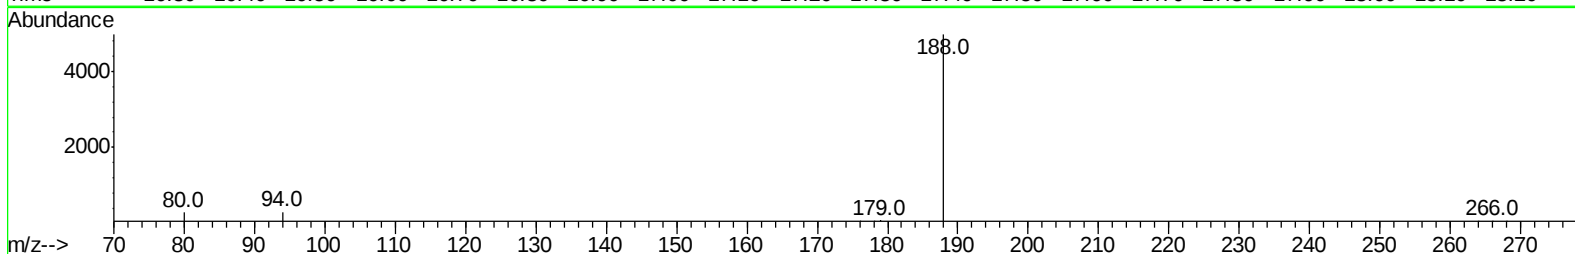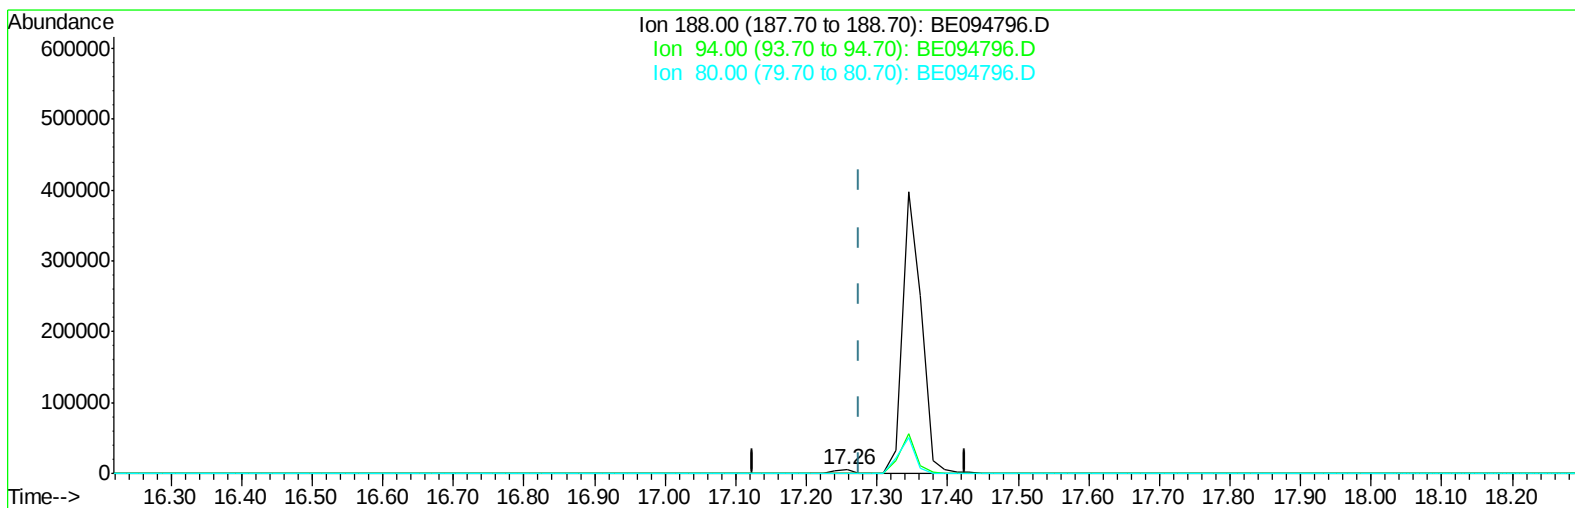

TIC: BE094796.D

(10) Phenanthrene-d10 (I)

17.258min (-0.018) 0.40ng/ul m

response 9904

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.00#
80.00	11.80	5.56#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 12:57:07 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

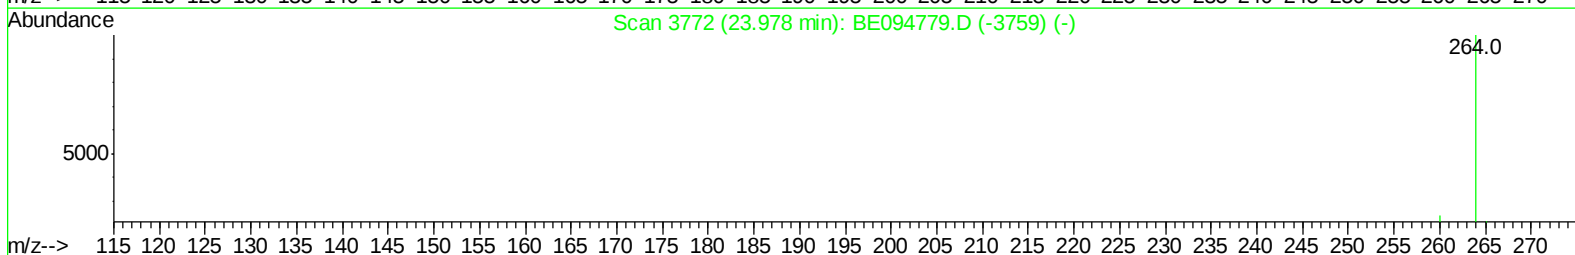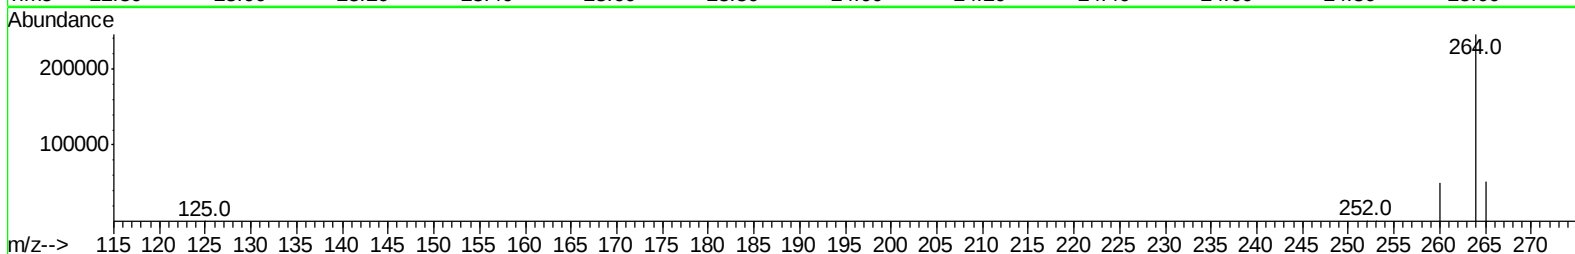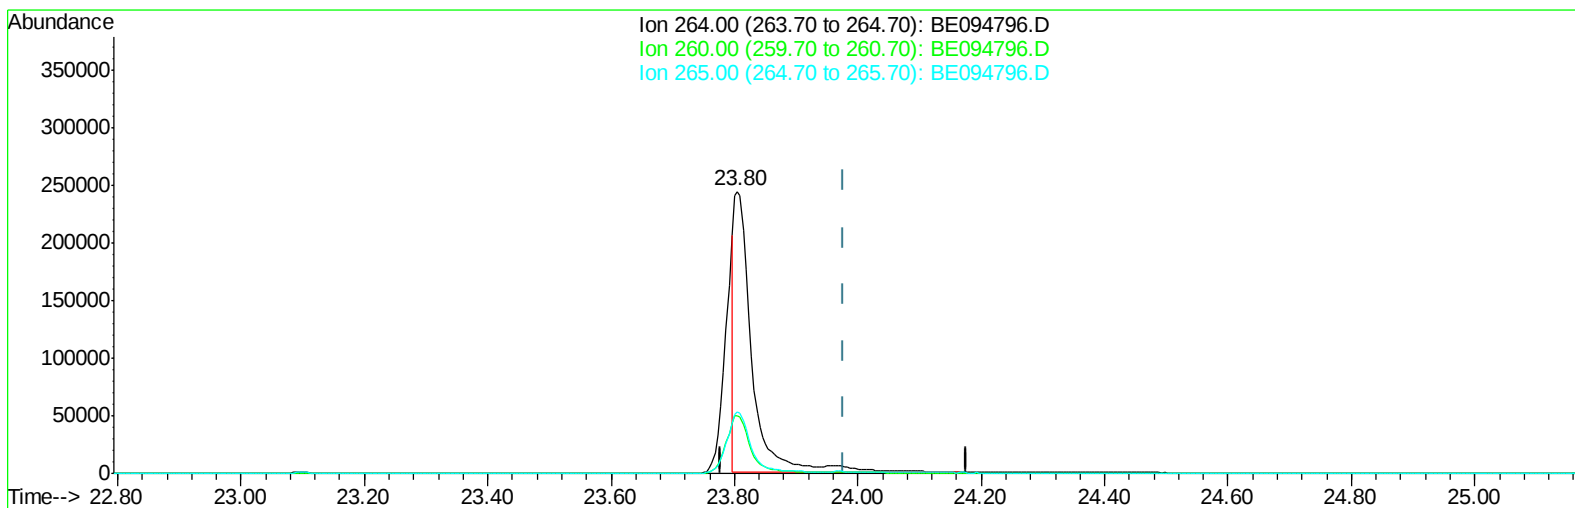

TIC: BE094796.D

(20) Perylene-d12 (I)

23.805min (-0.173) 0.40ng/ul

response 494827

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.51#
265.00	103.50	21.66#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 12:57:07 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

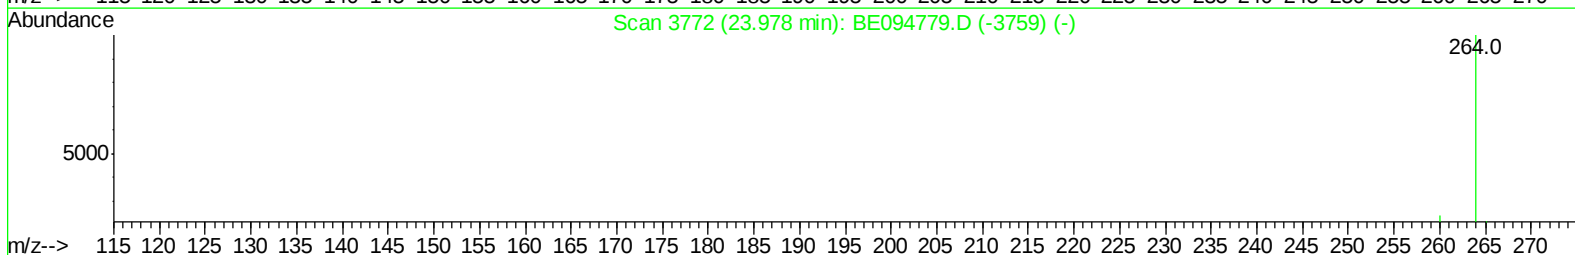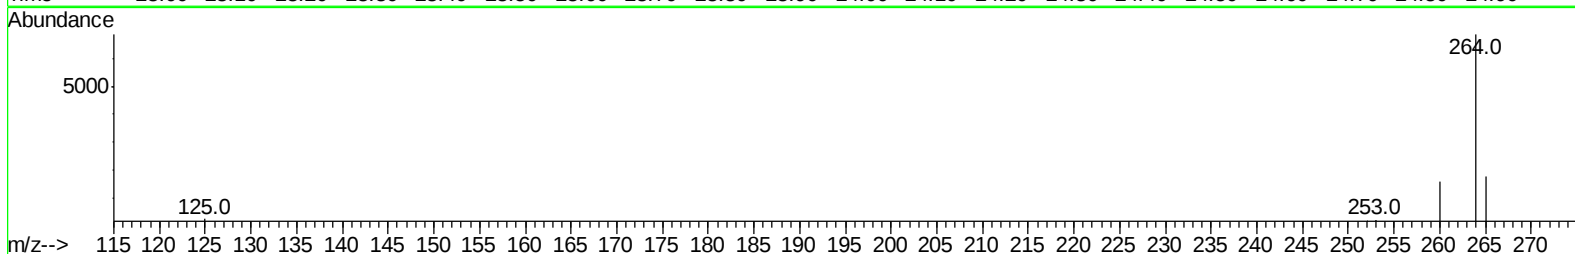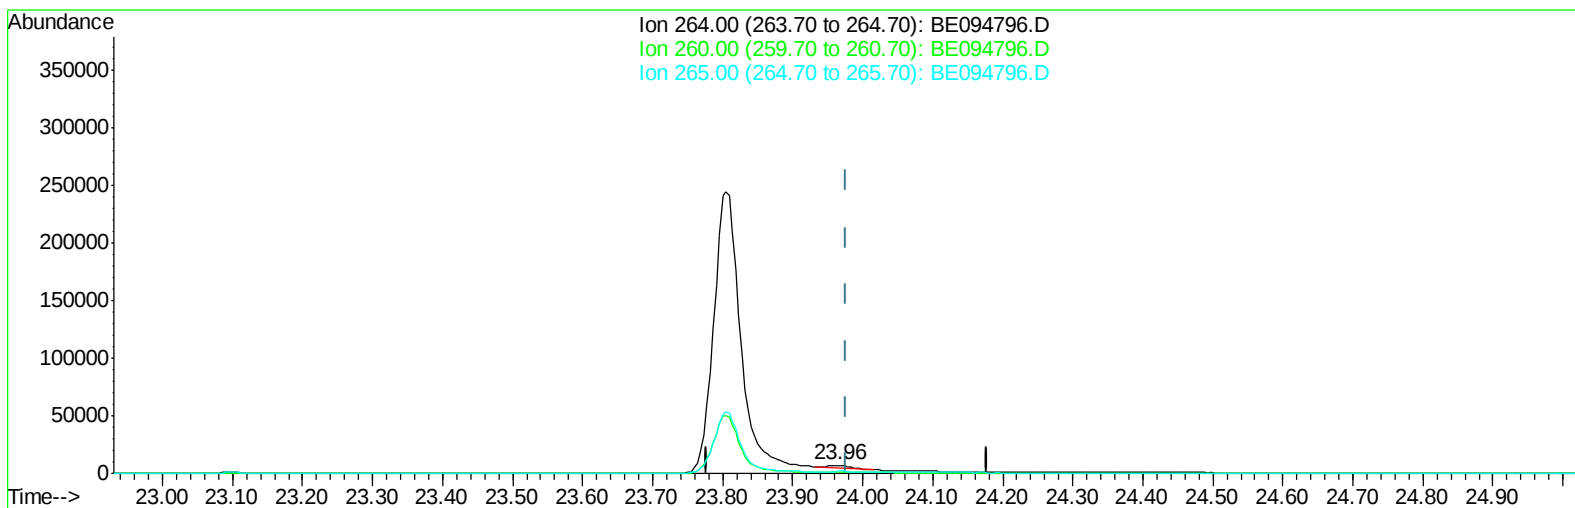

TIC: BE094796.D

(20) Perylene-d12 (I)

23.964min (-0.013) 0.40ng/ul m

response 4720

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.02#
265.00	103.50	25.65#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 13:00:11 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1336	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	8234	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4772	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9904m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	9521	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	4720m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	4088	0.31	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	9566	0.33	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094796.D
Acq On : 9 Nov 2017 9:54
Operator : SJ/JU
Sample : PB103704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK04

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:10 PM

Quant Time: Nov 09 13:00:11 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

