




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 12:49:51 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

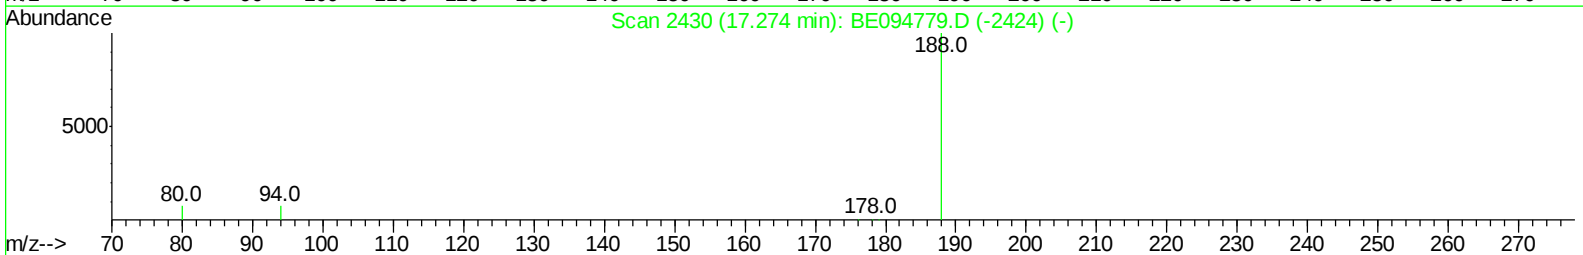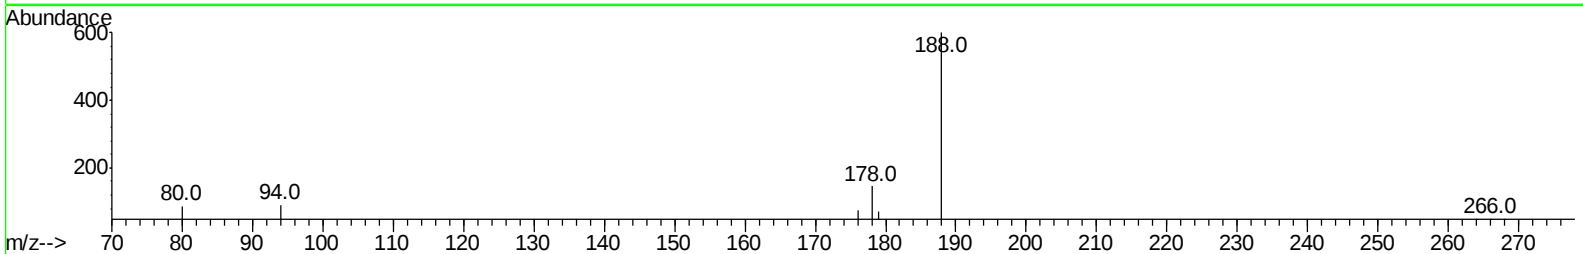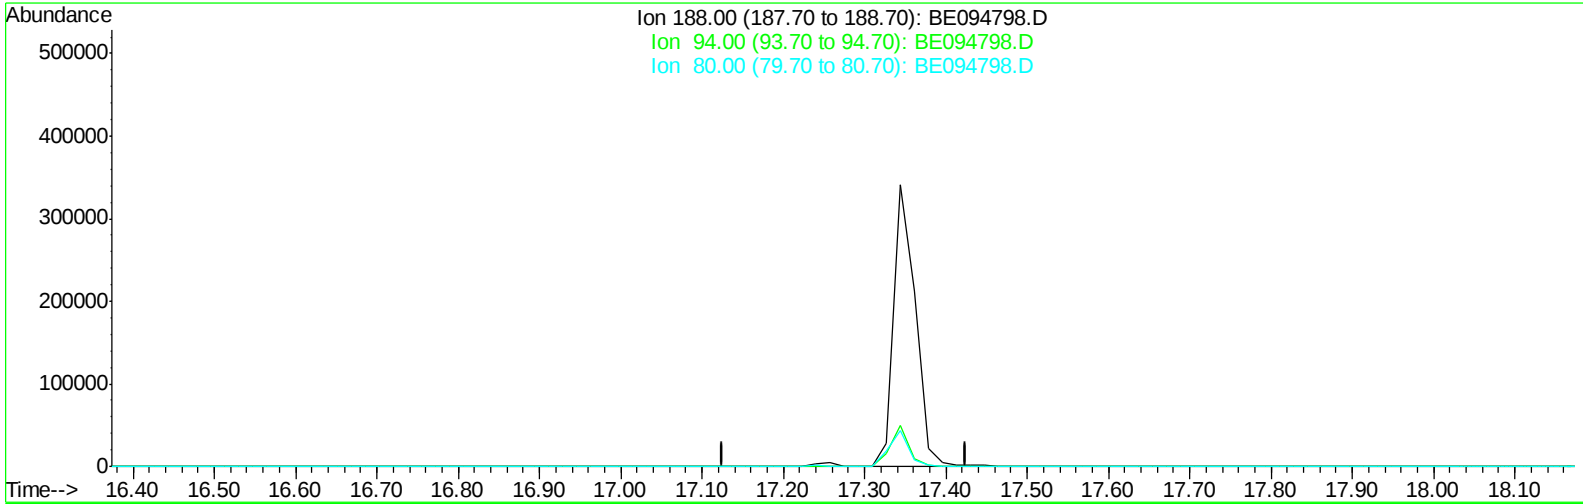

TIC: BE094798.D

(10) Phenanthrene-d10 (I)

17.275min (-17.275) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 12:49:51 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

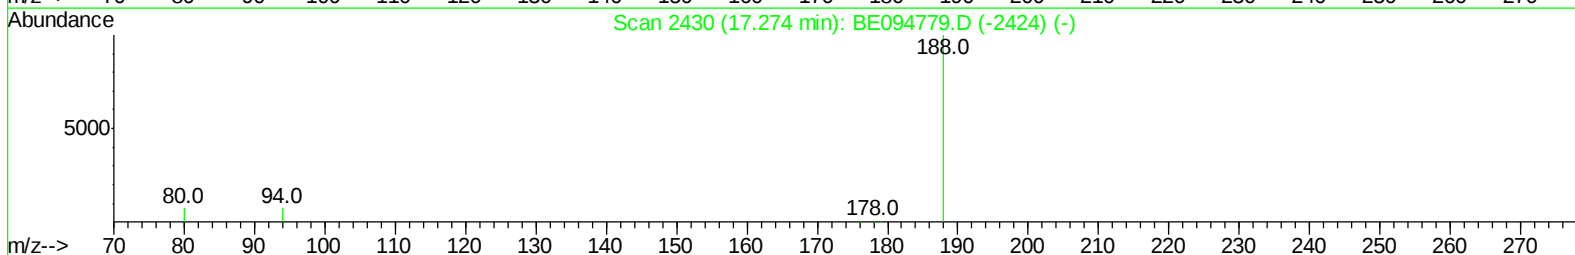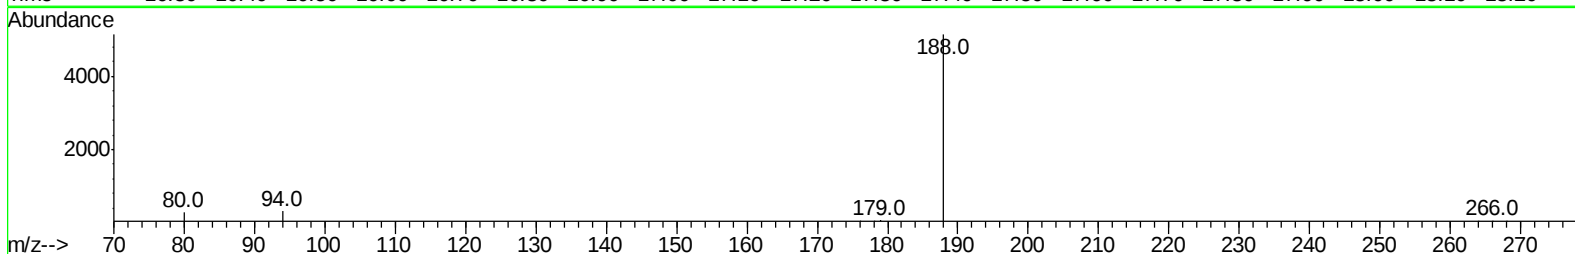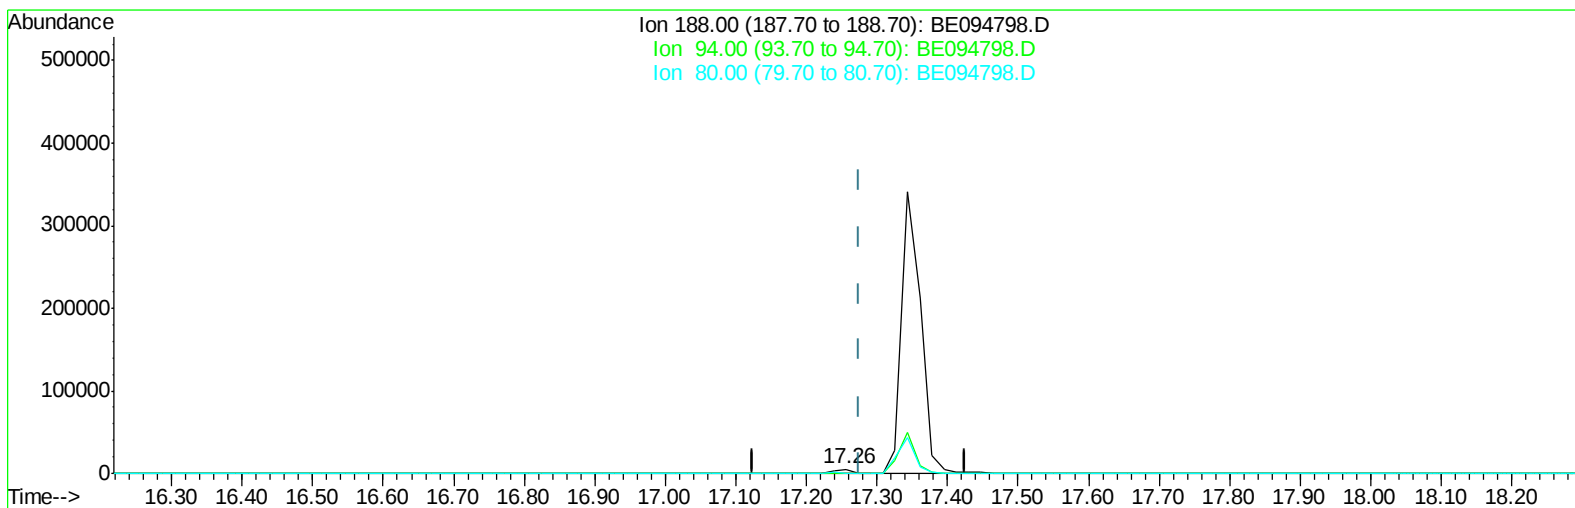

TIC: BE094798.D

(10) Phenanthrene-d10 (I)

17.257min (-0.018) 0.40ng/ul m

response 9726

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.08#
80.00	11.80	5.39#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 13:06:16 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

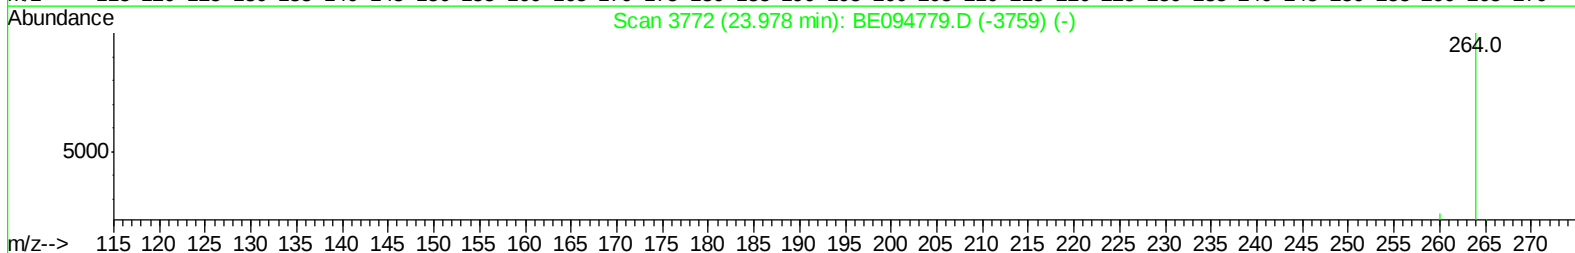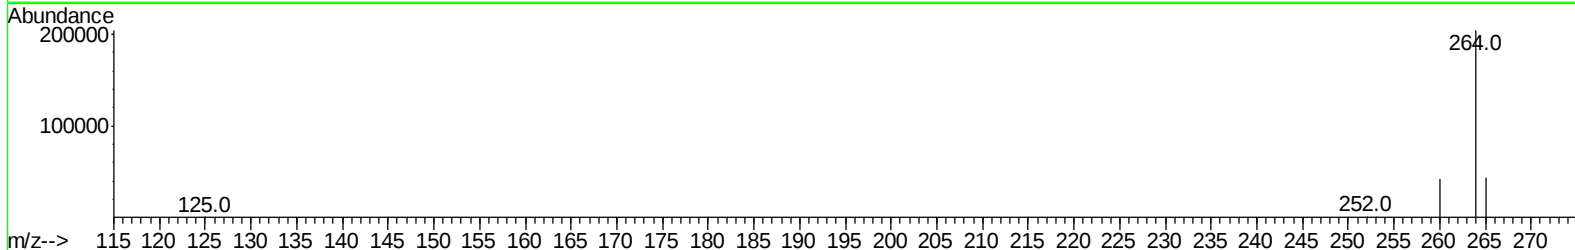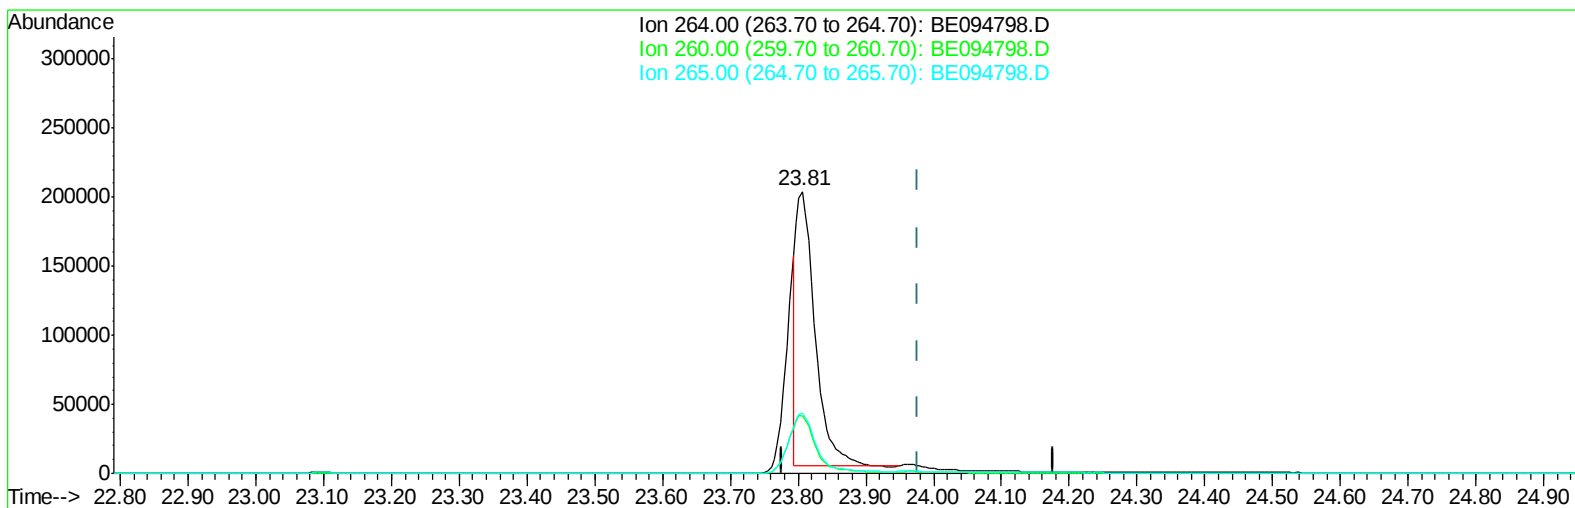

TIC: BE094798.D

(20) Perylene-d12 (I)

23.806min (-0.172) 0.40ng/ul

response 393368

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.46#
265.00	103.50	21.33#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 13:06:16 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

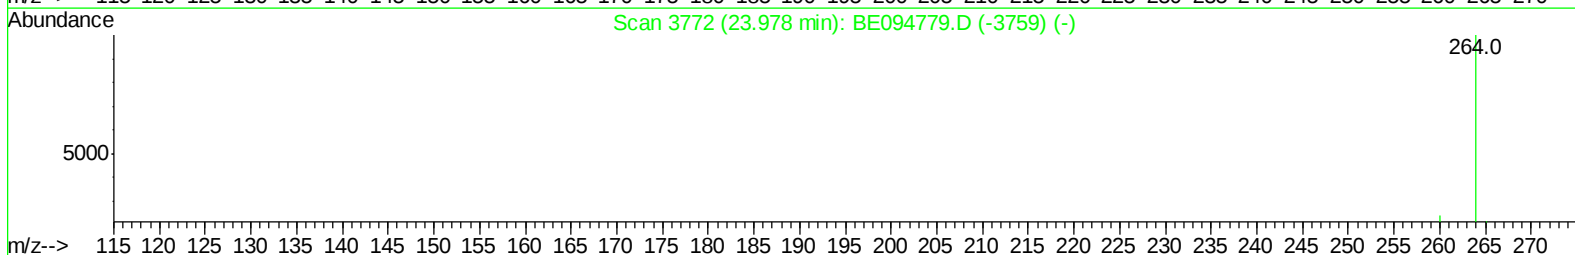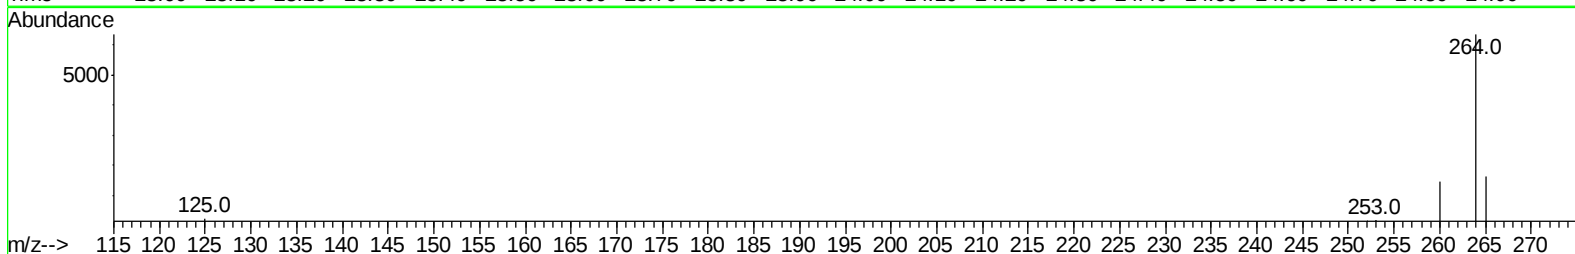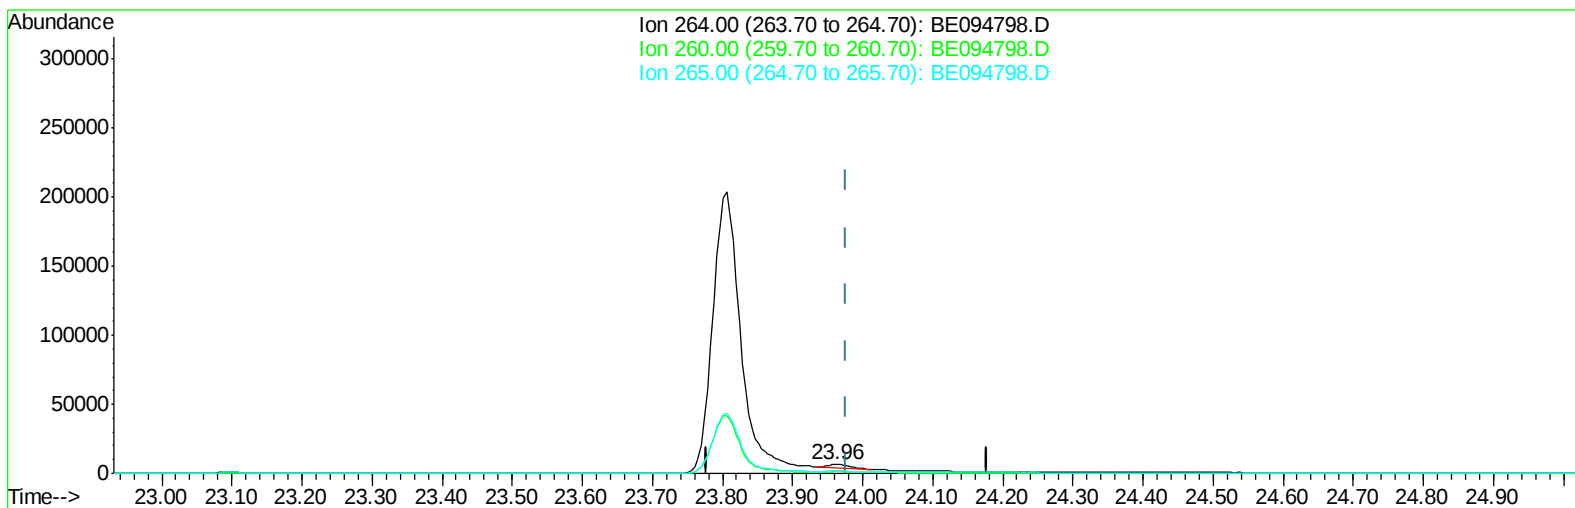

TIC: BE094798.D

(20) Perylene-d12 (I)

23.961min (-0.017) 0.40ng/ul m

response 5281

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.21#
265.00	103.50	25.81#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 13:09:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1386	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	8232	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4769	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9726m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.44	240	9469	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	5281m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3670	0.27	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	8326	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094798.D
Acq On : 9 Nov 2017 11:05
Operator : SJ/JU
Sample : I5976-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-4-101817

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:13 PM

Quant Time: Nov 09 13:09:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

