




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094799.D
Acq On : 9 Nov 2017 11:41
Operator : SJ/JU
Sample : I6120-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-5-102417

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:15 PM

Quant Time: Nov 09 12:50:03 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

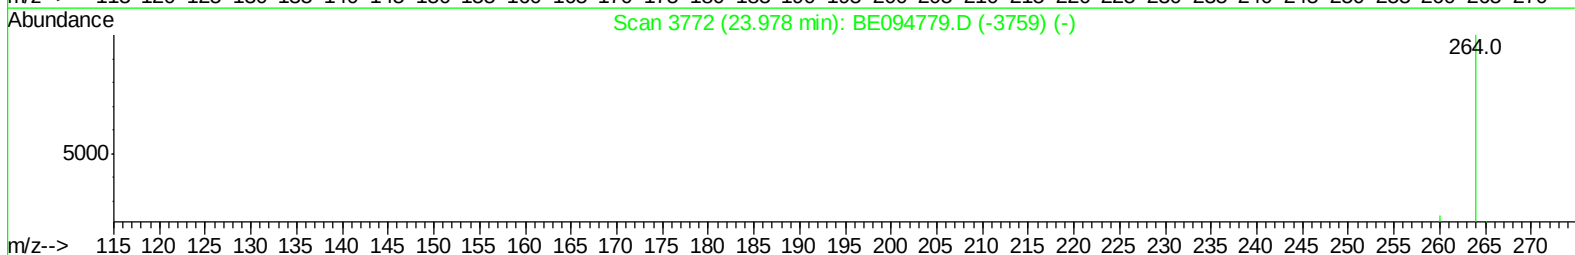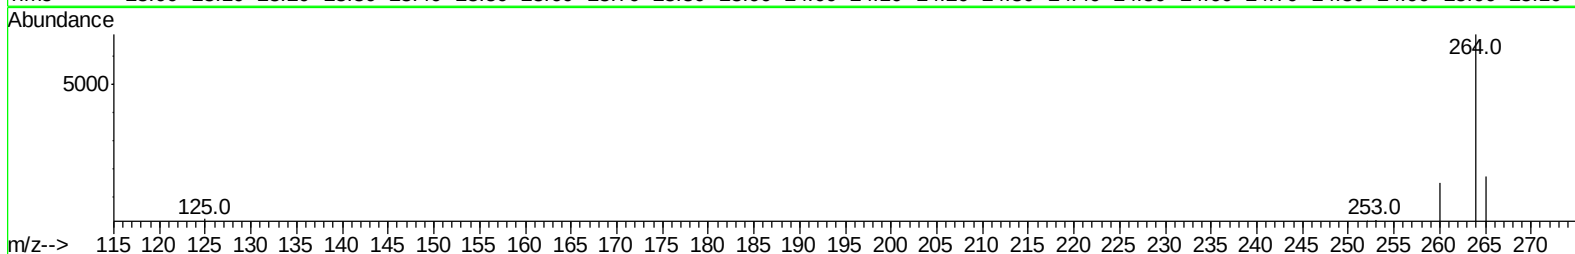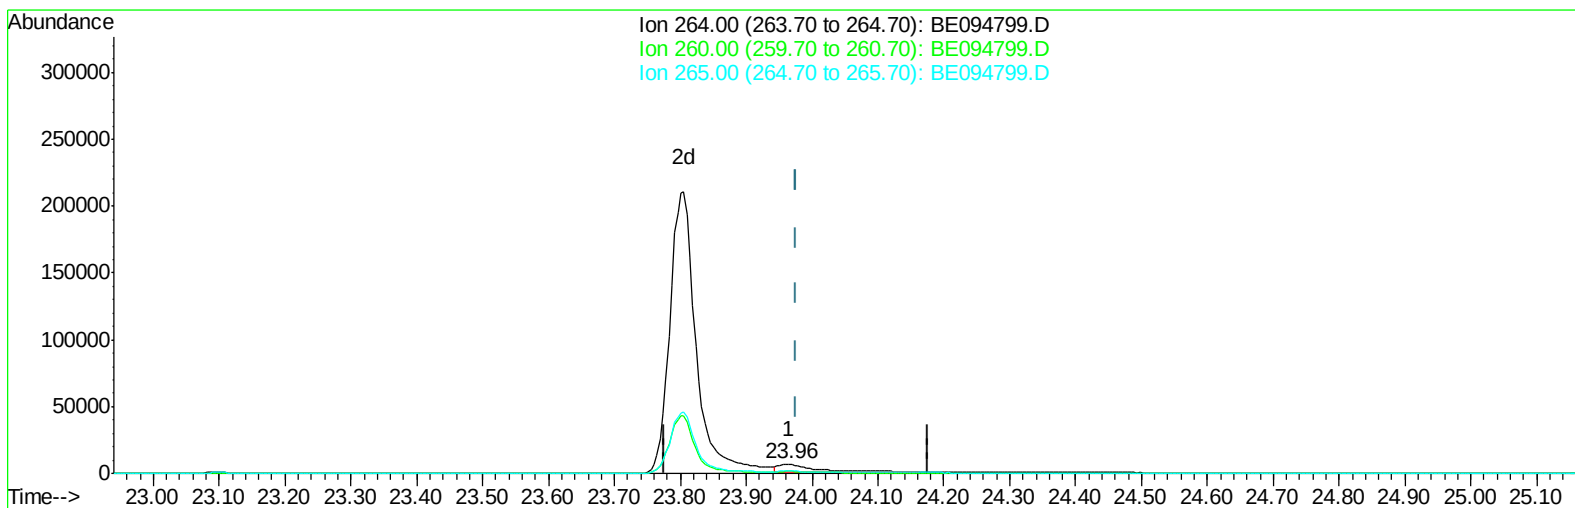

TIC: BE094799.D

(20) Perylene-d12 (I)

23.965min (-0.013) 0.40ng/ul

response 20871

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.59#
265.00	103.50	25.77#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094799.D
Acq On : 9 Nov 2017 11:41
Operator : SJ/JU
Sample : I6120-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-5-102417

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:15 PM

Quant Time: Nov 09 12:50:03 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

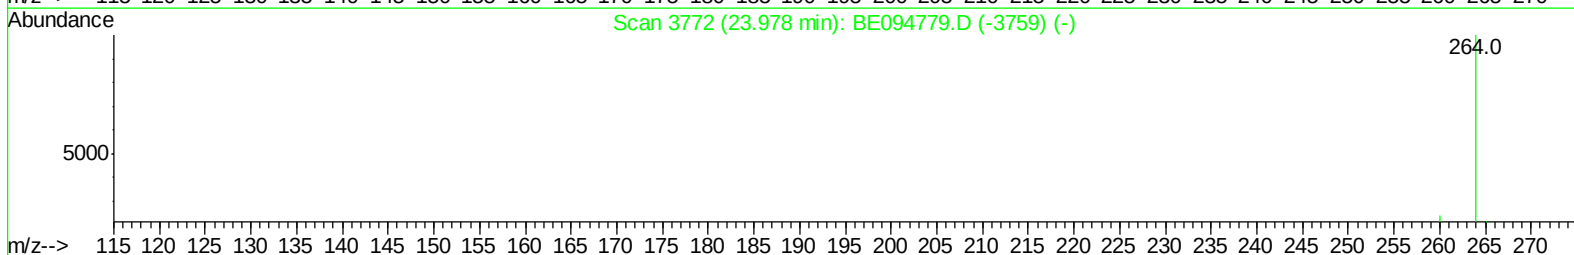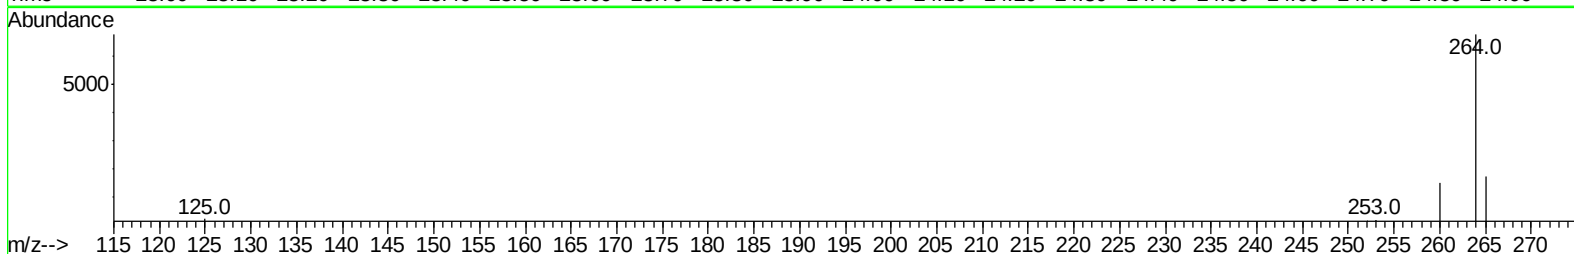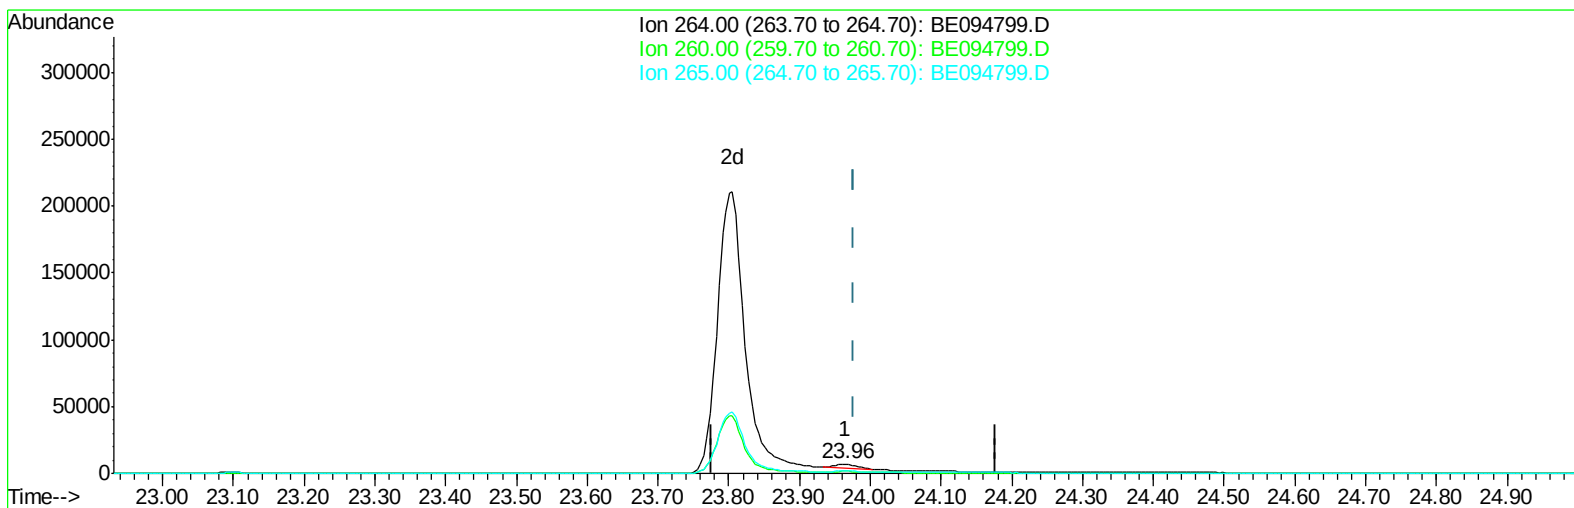

TIC: BE094799.D

(20) Perylene-d12 (I)

23.965min (-0.013) 0.40ng/ul m

response 5837

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.59#
265.00	103.50	25.77#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
 Data File : BE094799.D
 Acq On : 9 Nov 2017 11:41
 Operator : SJ/JU
 Sample : I6120-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EQB-5-102417

Manual Integrations
 APPROVED

Sohil
 11/9/2017 6:35:15 PM

Quant Time: Nov 09 13:13:43 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 01:37:48 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1517	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	9215	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	5303	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.26	188	10960	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	11067	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	5837m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3330	0.22	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	7881	0.24	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE111017\
Data File : BE094799.D
Acq On : 9 Nov 2017 11:41
Operator : SJ/JU
Sample : I6120-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EQB-5-102417

Manual Integrations
APPROVED

Sohil
11/9/2017 6:35:15 PM

Quant Time: Nov 09 13:13:43 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 01:37:48 2017
Response via : Initial Calibration

