

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091117.D
 Acq On : 11 Nov 2015 18:29
 Operator : UM/NP
 Sample : PB86558BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK58

Quant Time: Nov 13 15:20:17 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3285	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	18494	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	10576	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1797664	0.40	ng/ul	0.08
18) Chrysene-d12	20.29	240	27792	0.40	ng/ul	0.00
22) Perylene-d12	22.07	264	2039070	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	23276	9.85	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.08	152	7237	0.29	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	20305	0.00	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Fluorene	14.39	166	2979	0.06	ng/ul#	8
19) Pyrene	18.51	202	13588	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091117.D
Acq On : 11 Nov 2015 18:29
Operator : UM/NP
Sample : PB86558BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK58

Quant Time: Nov 13 15:20:17 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

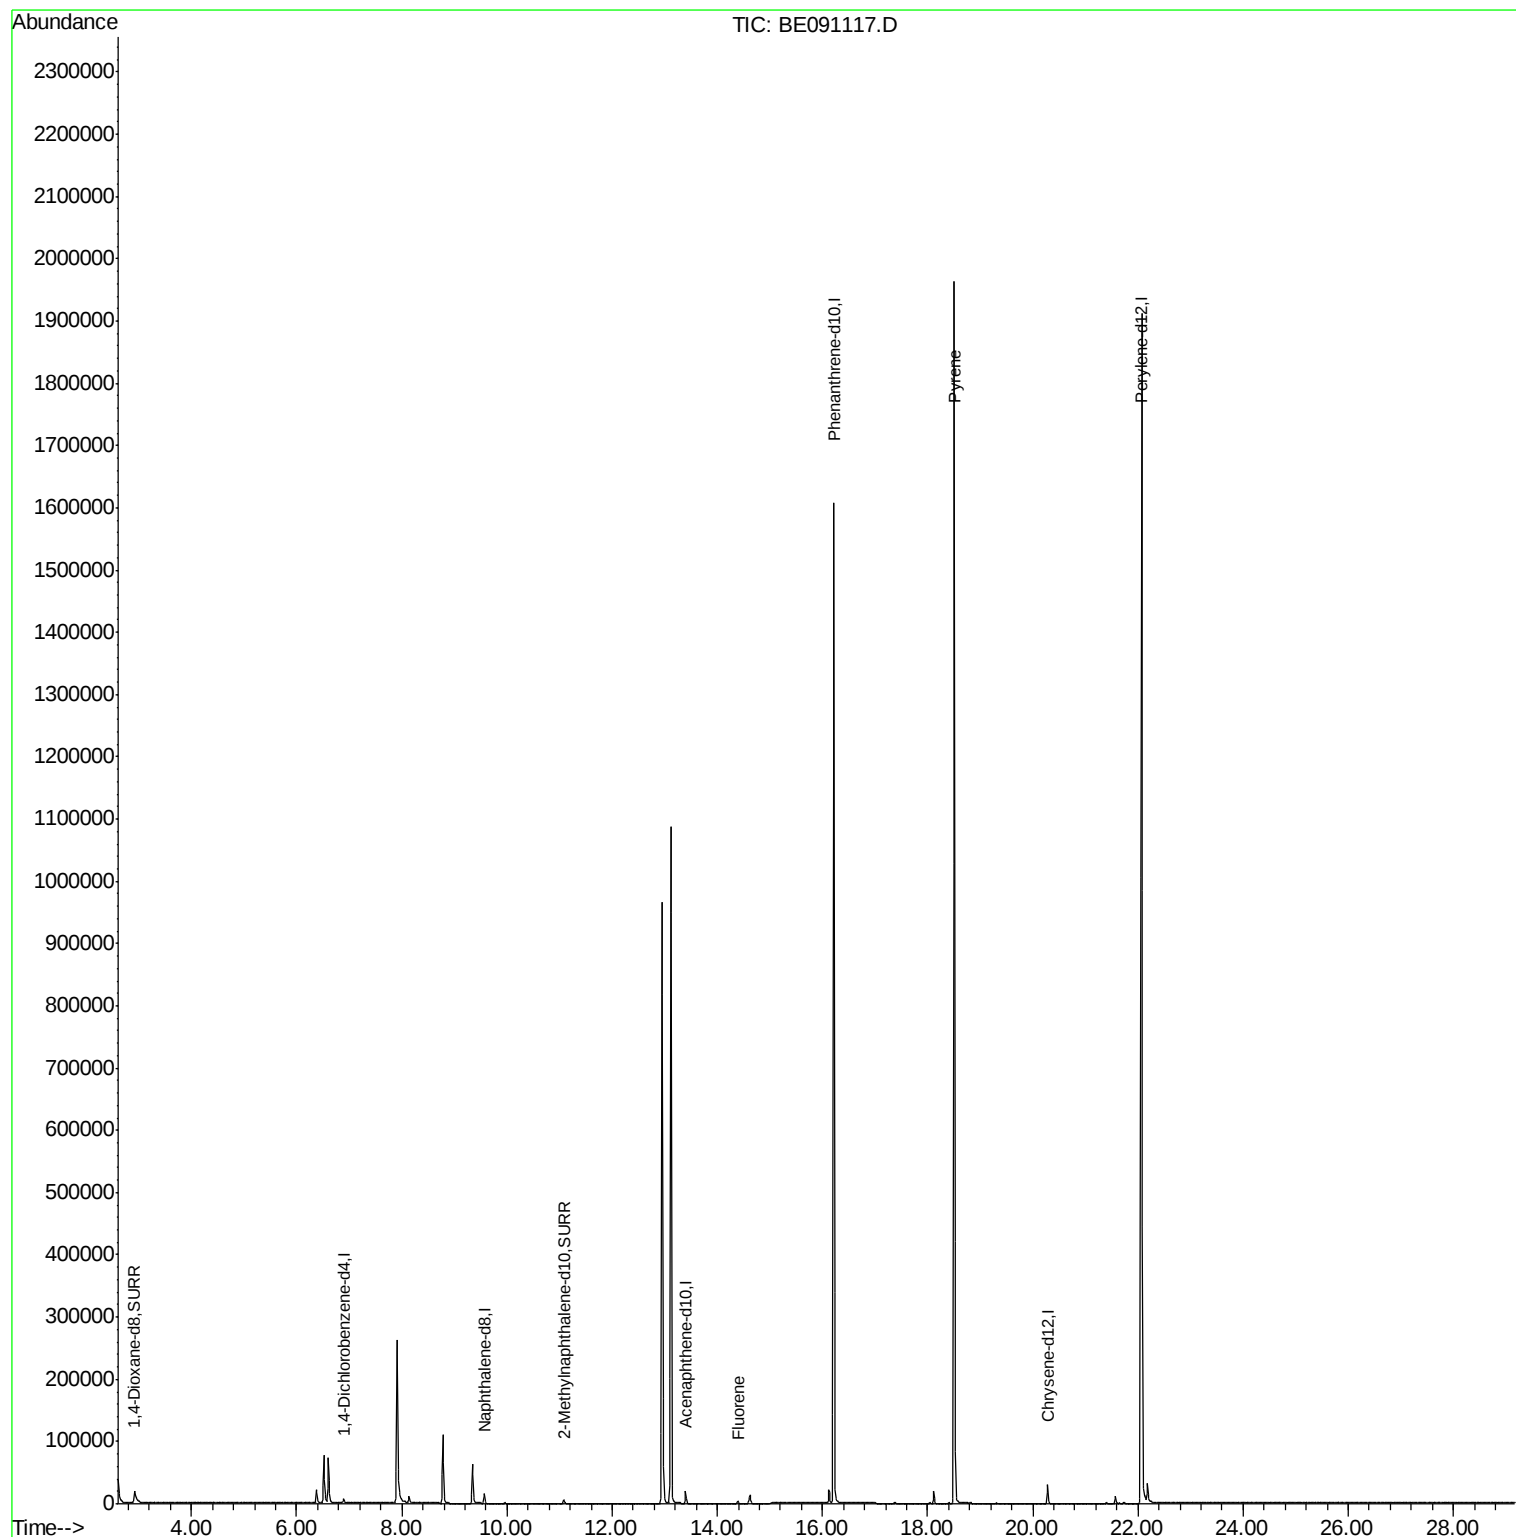

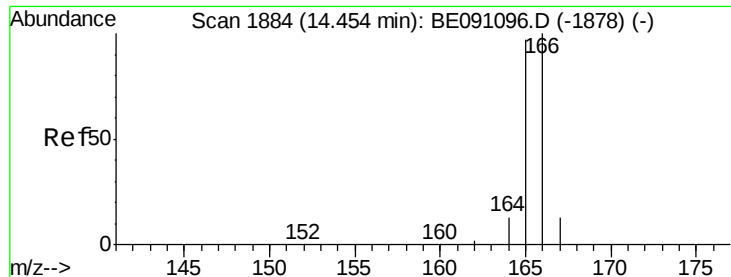

#11

Fluorene

Concen: 0.06 ng/ul

RT: 14.39 min Scan# 1876

Delta R.T. -0.06 min

Lab File: BE091117.D

Acq: 11 Nov 2015 18:29

Instrument :

BNA_E

ClientSampleId :

SBLK58





Tgt Ion:166 Resp: 2979

Ion Ratio Lower Upper

166 100

165 7.5 87.6 131.4#

167 35.4 11.1 16.7#

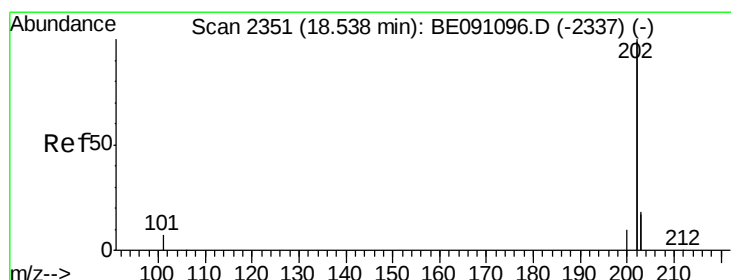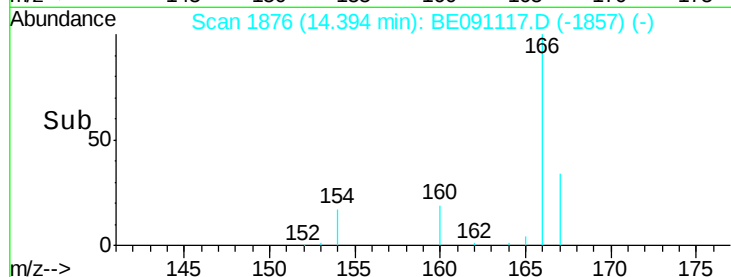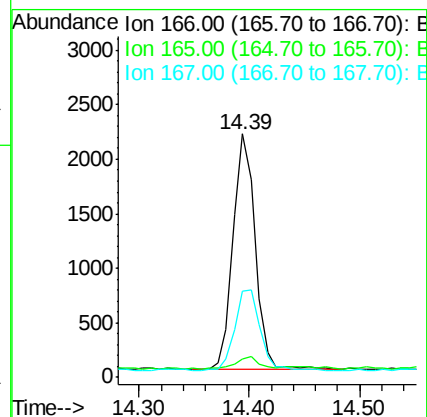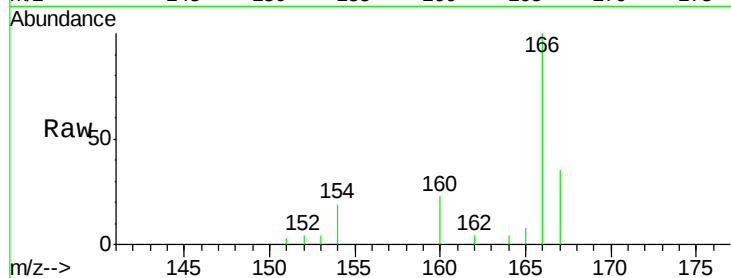

#19

Pyrene

Concen: 0.04 ng/ul

RT: 18.51 min Scan# 2347

Delta R.T. -0.02 min

Lab File: BE091117.D

Acq: 11 Nov 2015 18:29

Tgt Ion:202 Resp: 13588

Ion Ratio Lower Upper

202 100

200 1.6 18.0 27.0#

203 201.1 13.8 20.6#

