

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091119.D
 Acq On : 11 Nov 2015 19:44
 Operator : UM/NP
 Sample : G4308-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KS4

Quant Time: Nov 13 15:20:27 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3742	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	21345	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	12095	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1630776	0.40	ng/ul	0.08
18) Chrysene-d12	20.29	240	39087	0.40	ng/ul	0.00
22) Perylene-d12	22.07	264	1869241	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.95	96	5866	2.18	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.07	152	7196	0.25	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	21108	0.00	ng/ul	0.00
Target Compounds						
3) 1,4-Dioxane	3.03	88	159	0.05	ng/ul#	Qvalue 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091119.D
Acq On : 11 Nov 2015 19:44
Operator : UM/NP
Sample : G4308-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KS4

Quant Time: Nov 13 15:20:27 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

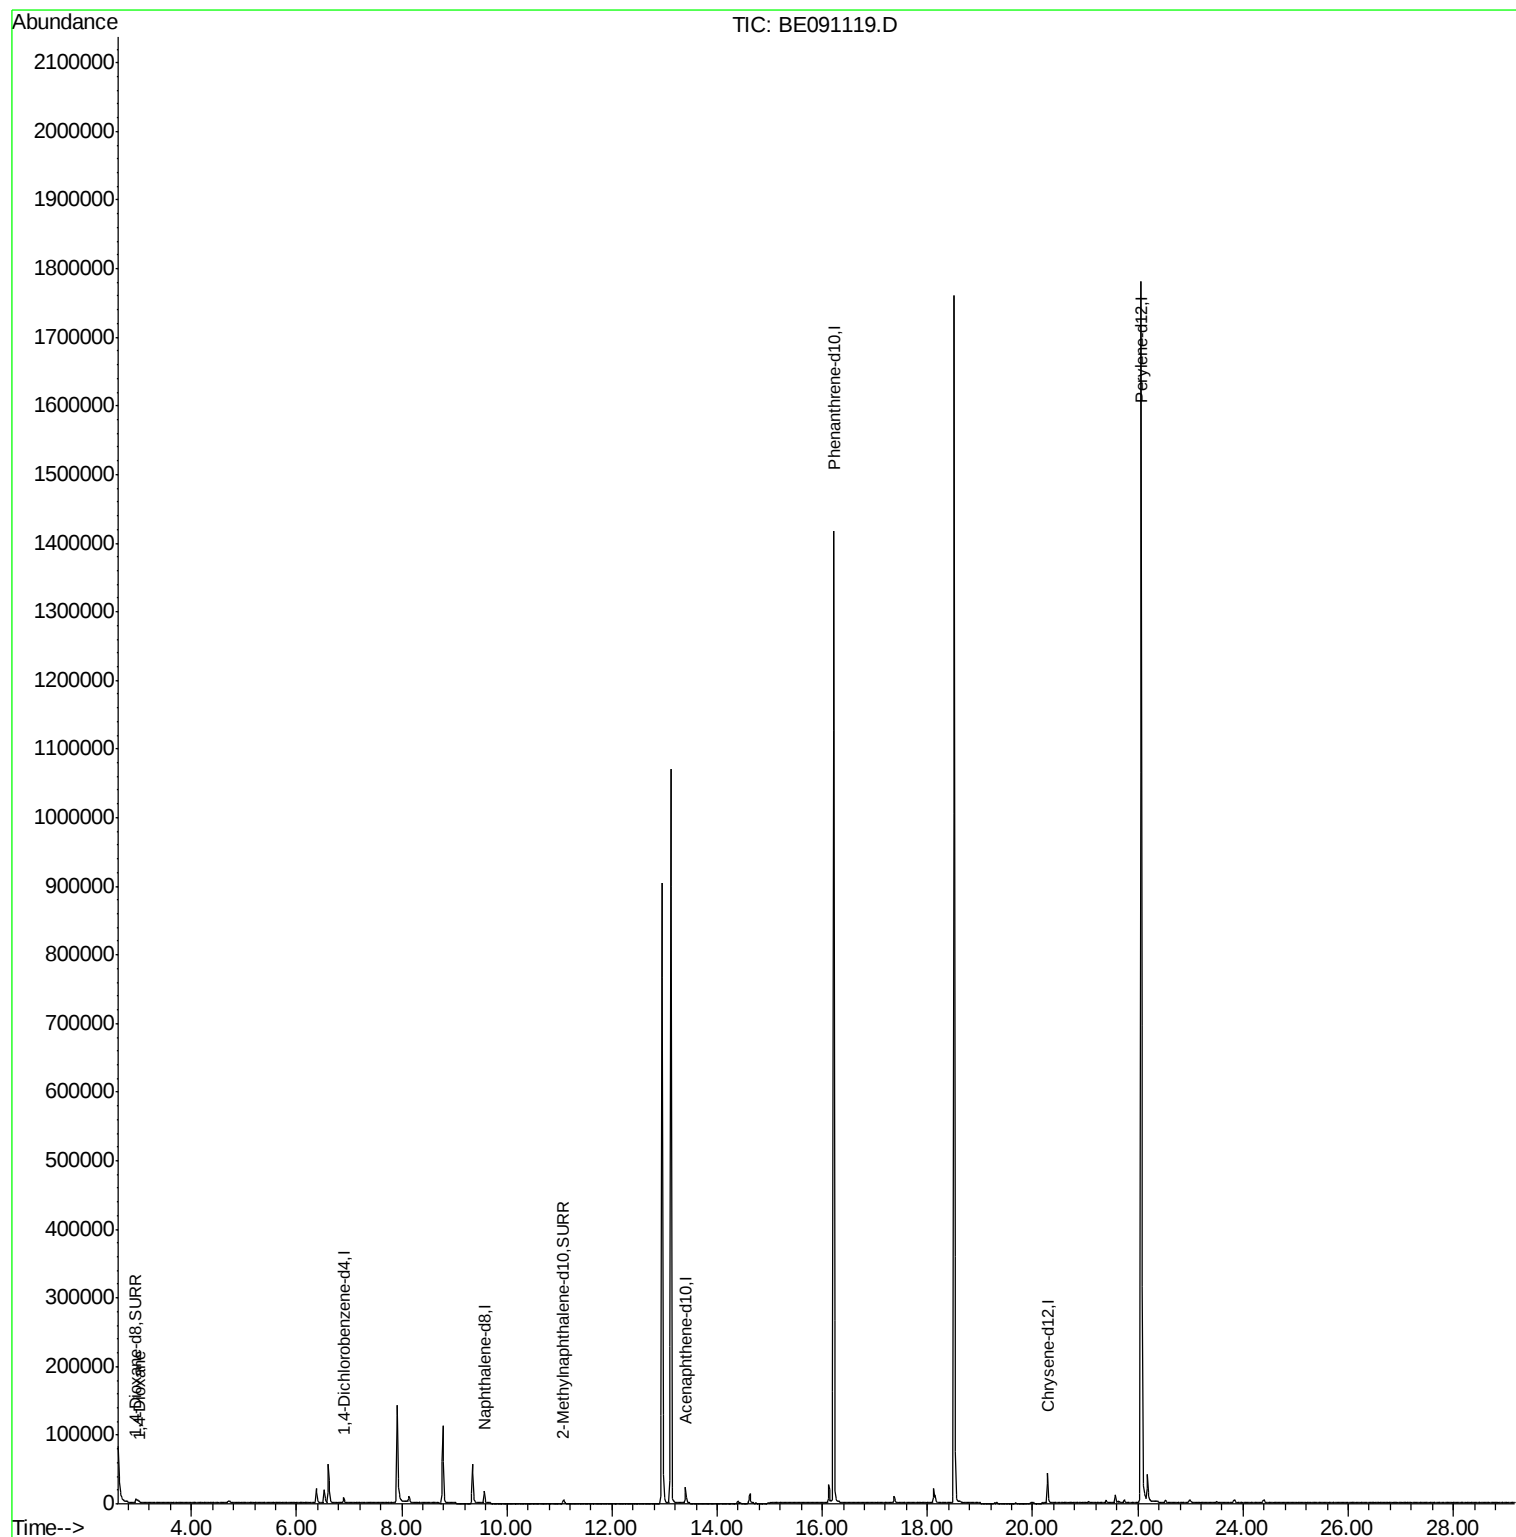

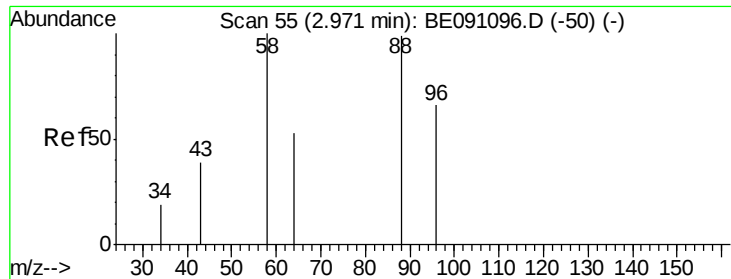

#3

1,4-Dioxane

Concen: 0.05 ng/ul

RT: 3.03 min Scan# 63

Delta R.T. 0.05 min

Lab File: BE091119.D

Acq: 11 Nov 2015 19:44

Instrument :

BNA_E

ClientSampleId :

D9KS4

Tgt Ion: 88 Resp: 159

Ion Ratio Lower Upper

88 100

58 9.4 55.4 83.2#

43 0.0 24.2 36.2#

