

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091124.D
 Acq On : 11 Nov 2015 22:46
 Operator : UM/NP
 Sample : PB86577BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK77

Quant Time: Nov 13 15:20:53 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3354	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	18671	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	11018	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1595367	0.40	ng/ul	0.08
18) Chrysene-d12	20.29	240	31042	0.40	ng/ul	0.00
22) Perylene-d12	22.07	264	1883610	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.91	96	23980	9.94	ng/uL	-0.04
6) 2-Methylnaphthalene-d10	11.08	152	6855	0.27	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	17488	0.00	ng/ul	0.00
Target Compounds						
						Qvalue
11) Fluorene	14.39	166	2804	0.06	ng/ul#	8
19) Pyrene	18.51	202	11580	0.03	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091124.D
Acq On : 11 Nov 2015 22:46
Operator : UM/NP
Sample : PB86577BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK77

Quant Time: Nov 13 15:20:53 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration




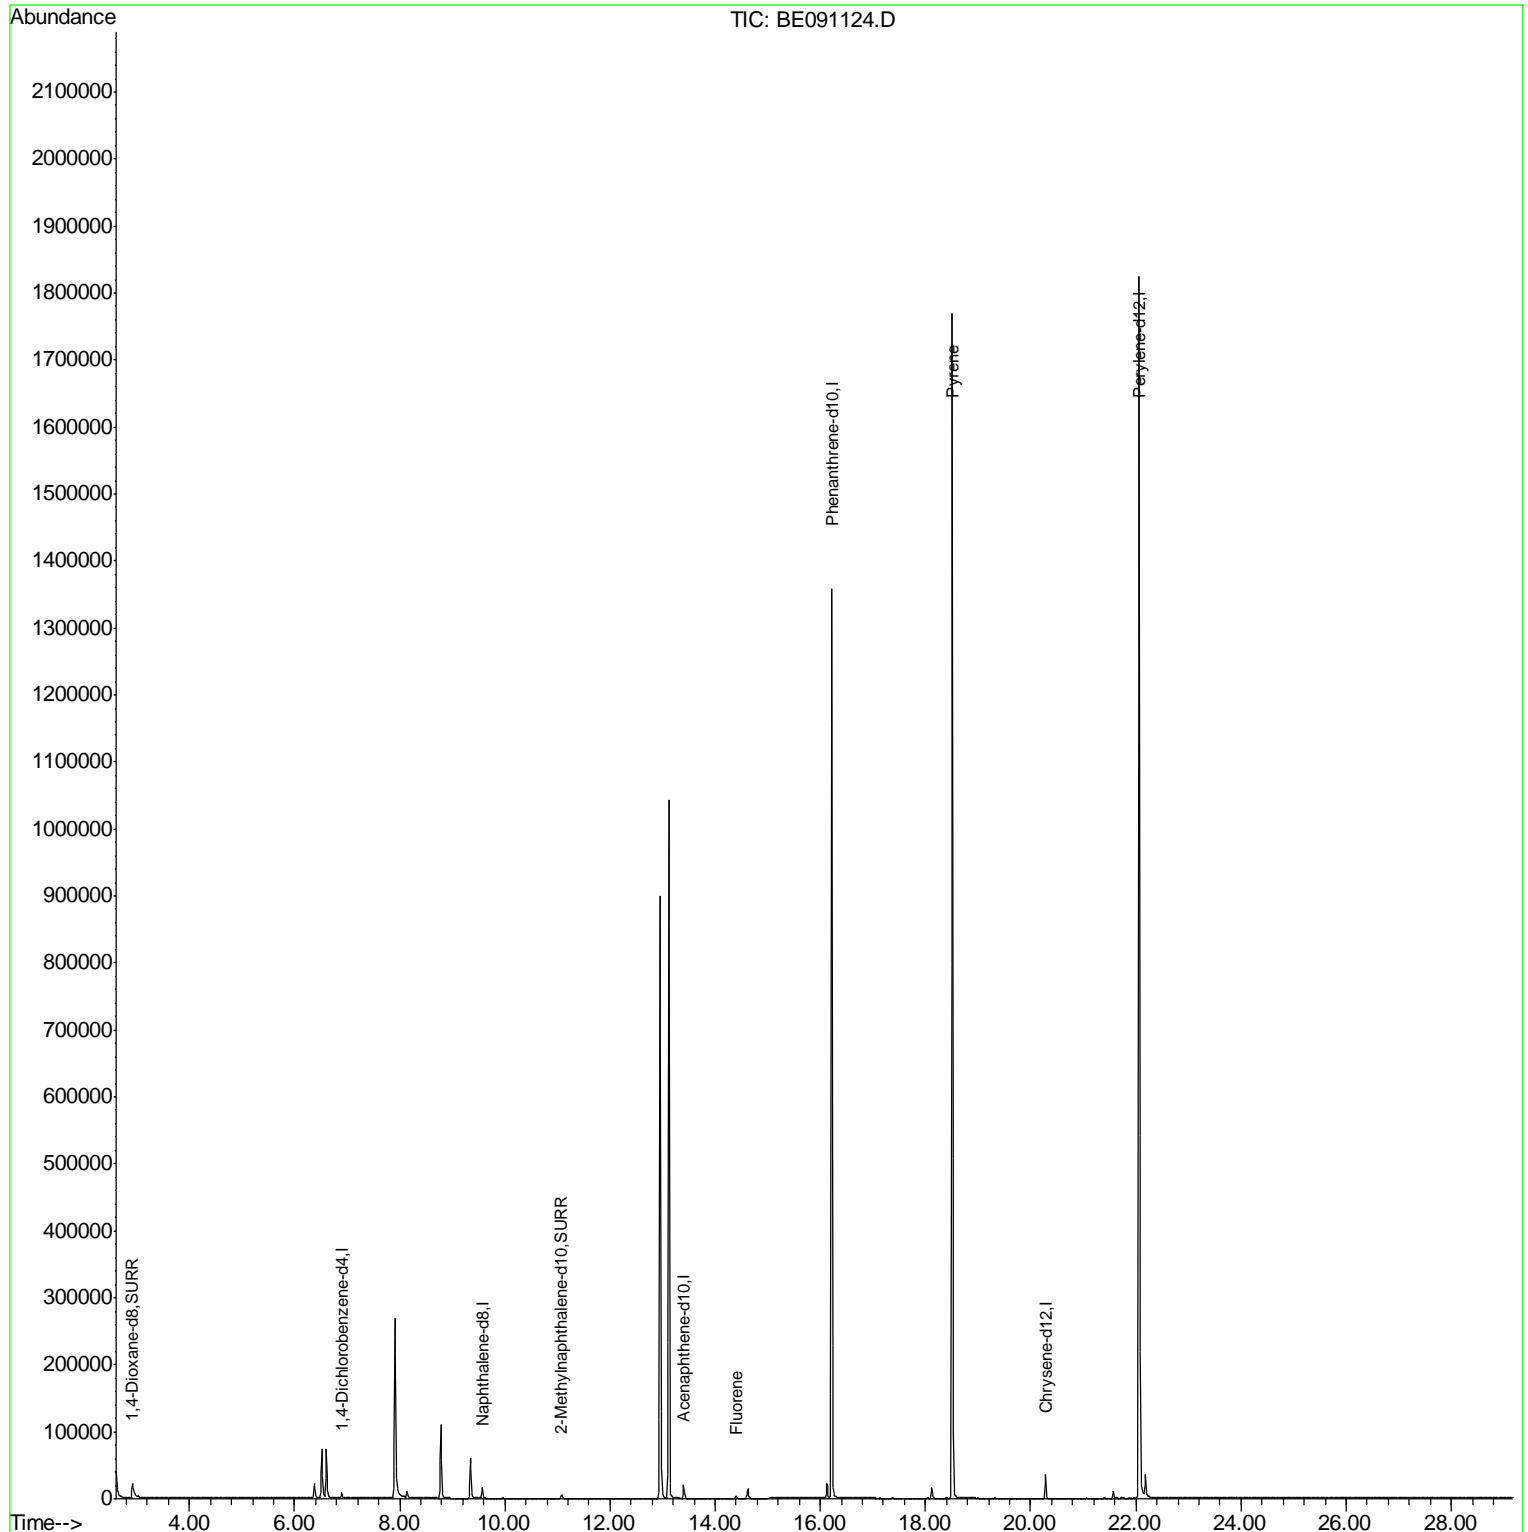


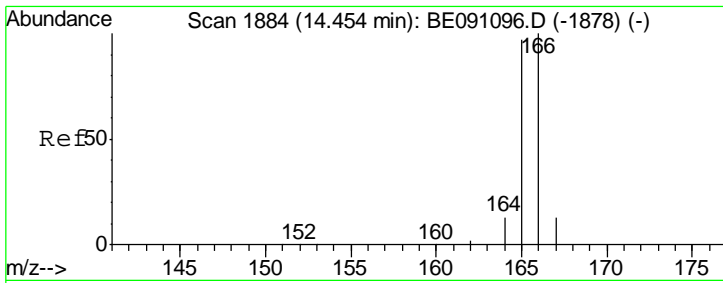

#11
 Fluorene
 Concen: 0.06 ng/ul
 RT: 14.39 min Scan# 1876
 Delta R.T. -0.06 min
 Lab File: BE091124.D
 Acq: 11 Nov 2015 22:46

Instrument :
 BNA_E
 ClientSampled :
 SBLK77

Tgt Ion	Resp	Lower	Upper
166	100		
165	8.3	87.6	131.4#
167	37.0	11.1	16.7#

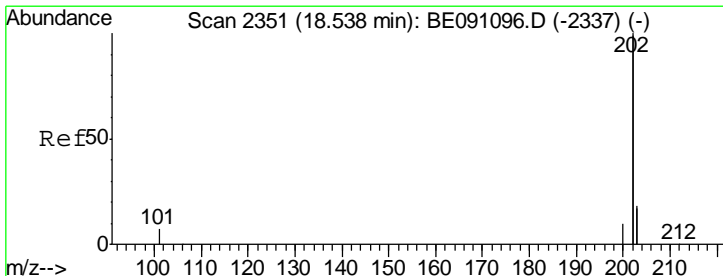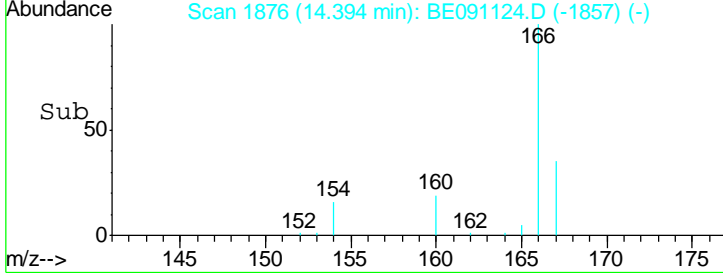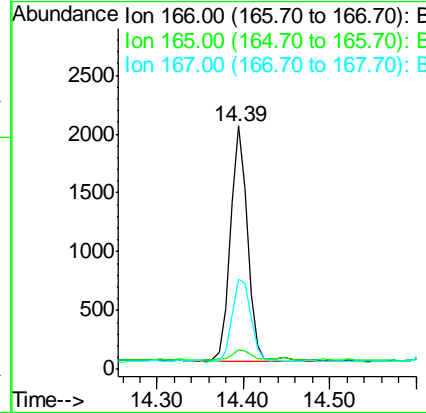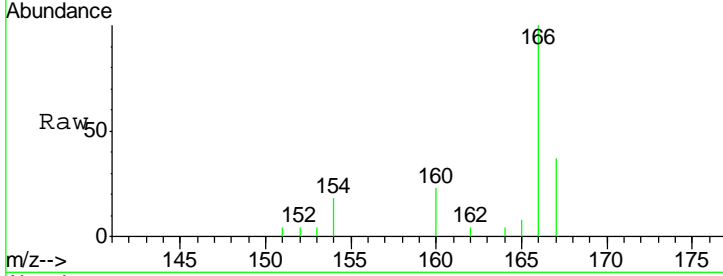

#19
 Pyrene
 Concen: 0.03 ng/ul
 RT: 18.51 min Scan# 2347
 Delta R.T. -0.03 min
 Lab File: BE091124.D
 Acq: 11 Nov 2015 22:46

Tgt Ion	Resp	Lower	Upper
202	100		
200	1.7	18.0	27.0#
203	195.7	13.8	20.6#

