

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091126.D
 Acq On : 11 Nov 2015 23:57
 Operator : UM/NP
 Sample : G4322-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A4HR4

Quant Time: Nov 13 15:21:02 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3400	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	18743	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	10798	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1199839	0.40	ng/ul	0.08
18) Chrysene-d12	20.28	240	33513	0.40	ng/ul	0.00
22) Perylene-d12	22.19	264	42650	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	17548	7.17	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.08	152	5063	0.20	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	13174	0.00	ng/ul	0.00
Target Compounds						
25) Benzo(a)pyrene	22.06	252	5116	0.04	ng/ul#	Qvalue 83




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091126.D
Acq On : 11 Nov 2015 23:57
Operator : UM/NP
Sample : G4322-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A4HR4

Quant Time: Nov 13 15:21:02 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

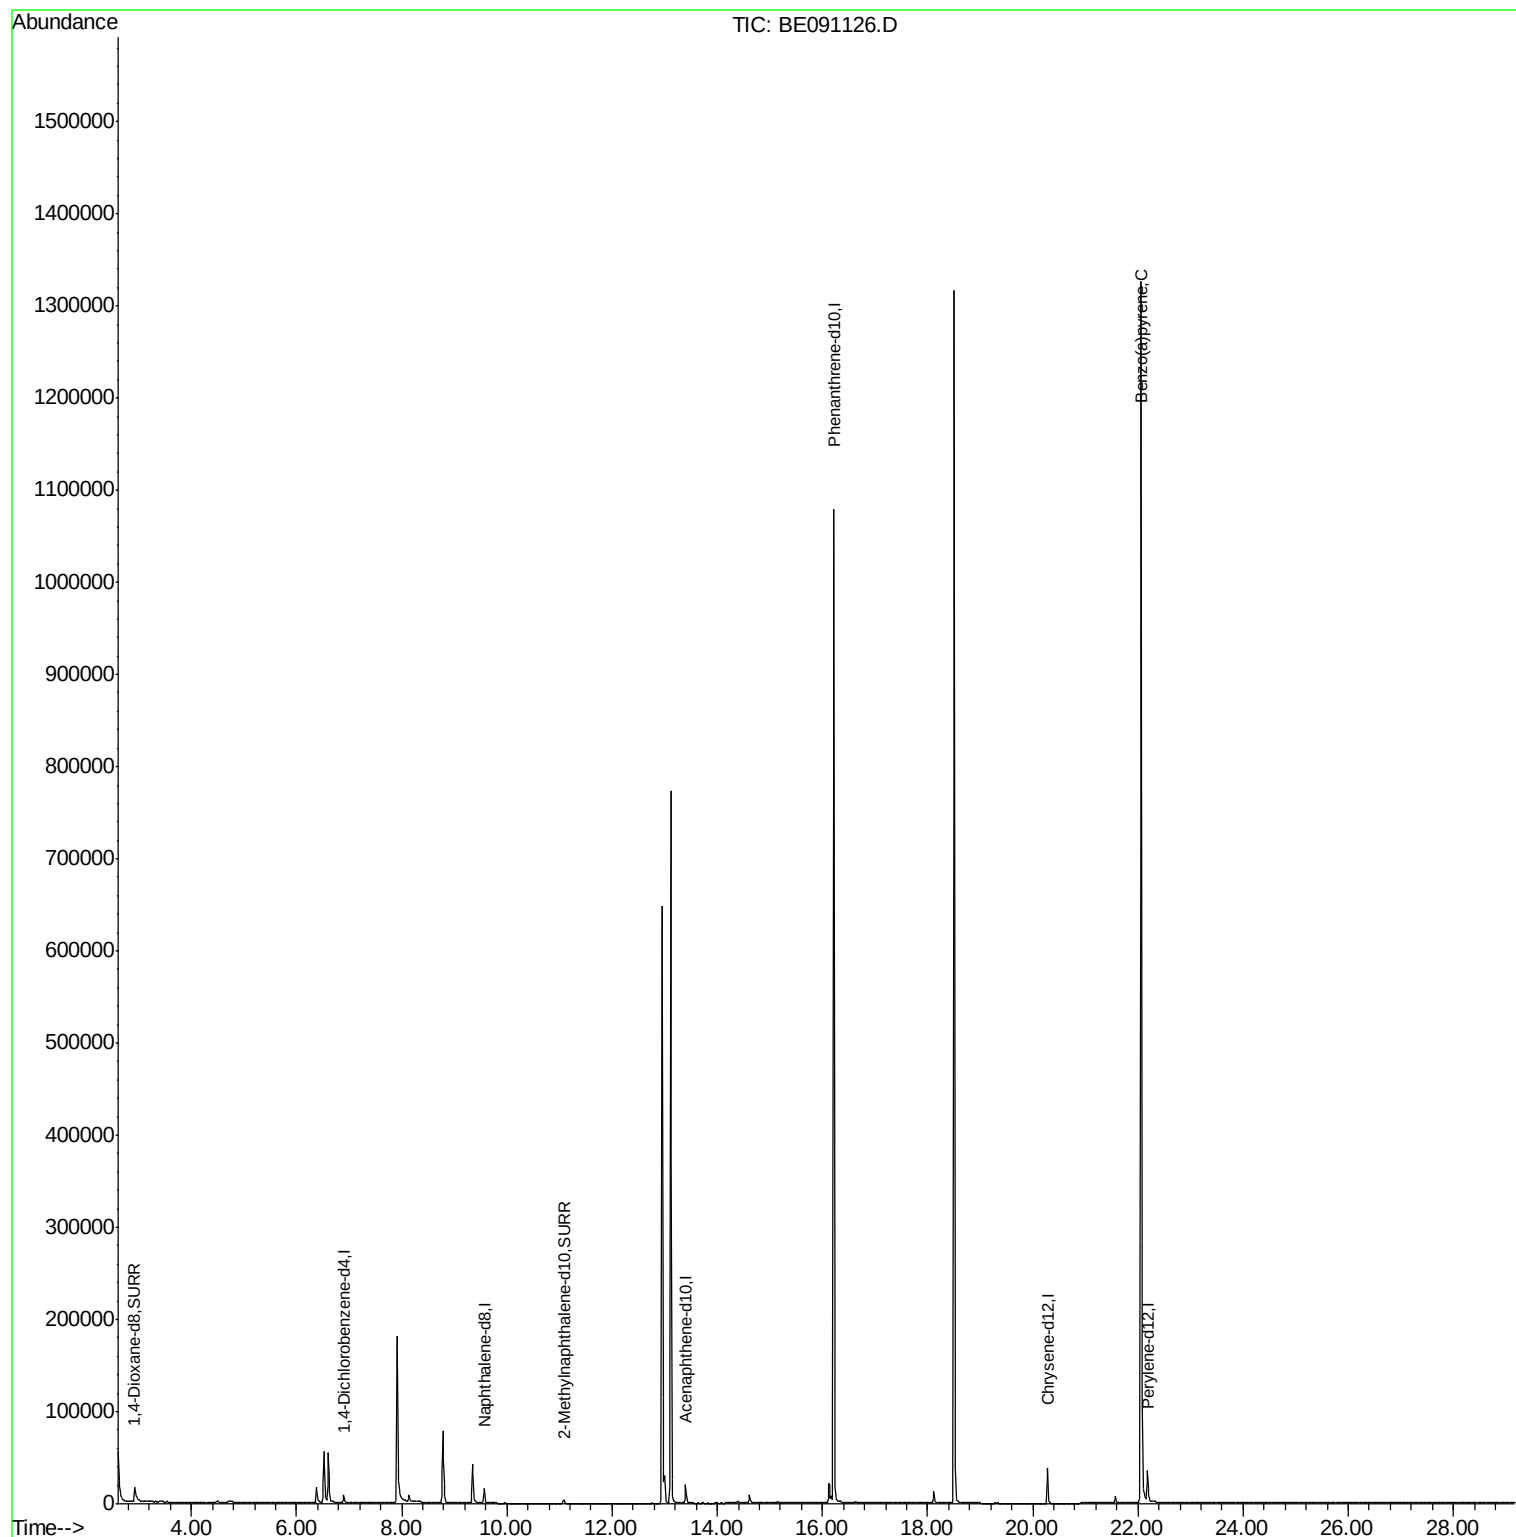

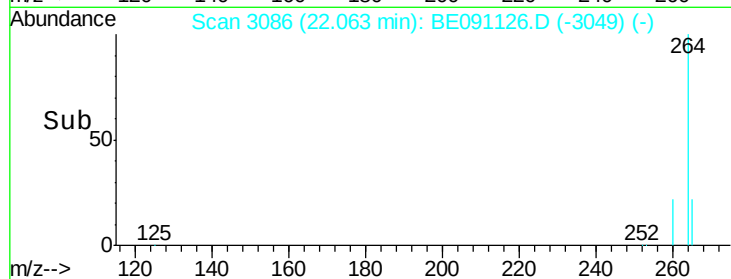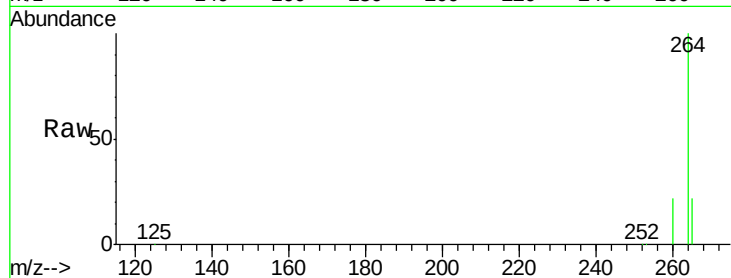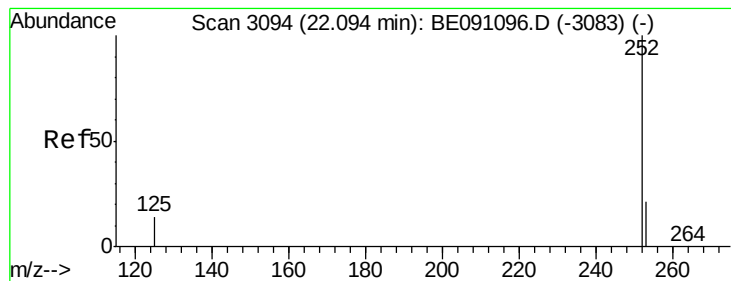

#25

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 22.06 min Scan# 3086

Delta R.T. -0.03 min

Lab File: BE091126.D

Acq: 11 Nov 2015 23:57

Instrument :

BNA_E

ClientSampleId :

A4HR4

Tgt Ion: 252 Resp: 5116

Ion Ratio Lower Upper

252 100

253 33.3 21.8 32.8#

125 29.5 14.5 21.7#

