

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091127.D
 Acq On : 12 Nov 2015 00:33
 Operator : UM/NP
 Sample : G4322-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A4HR6

Quant Time: Nov 13 15:21:08 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3100	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	17326	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	10019	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	1351673	0.40	ng/ul	0.08
18) Chrysene-d12	20.28	240	31770	0.40	ng/ul	0.00
22) Perylene-d12	22.06	264	1587279	0.40	ng/ul	-0.13
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	17258	7.74	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	5349	0.23	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	15284	0.00	ng/ul	0.00
Target Compounds						
					Qvalue	
3) 1,4-Dioxane	2.98	88	169	0.07	ng/ul#	42
5) Naphthalene	9.61	128	1303	0.03	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091127.D
Acq On : 12 Nov 2015 00:33
Operator : UM/NP
Sample : G4322-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A4HR6

Quant Time: Nov 13 15:21:08 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

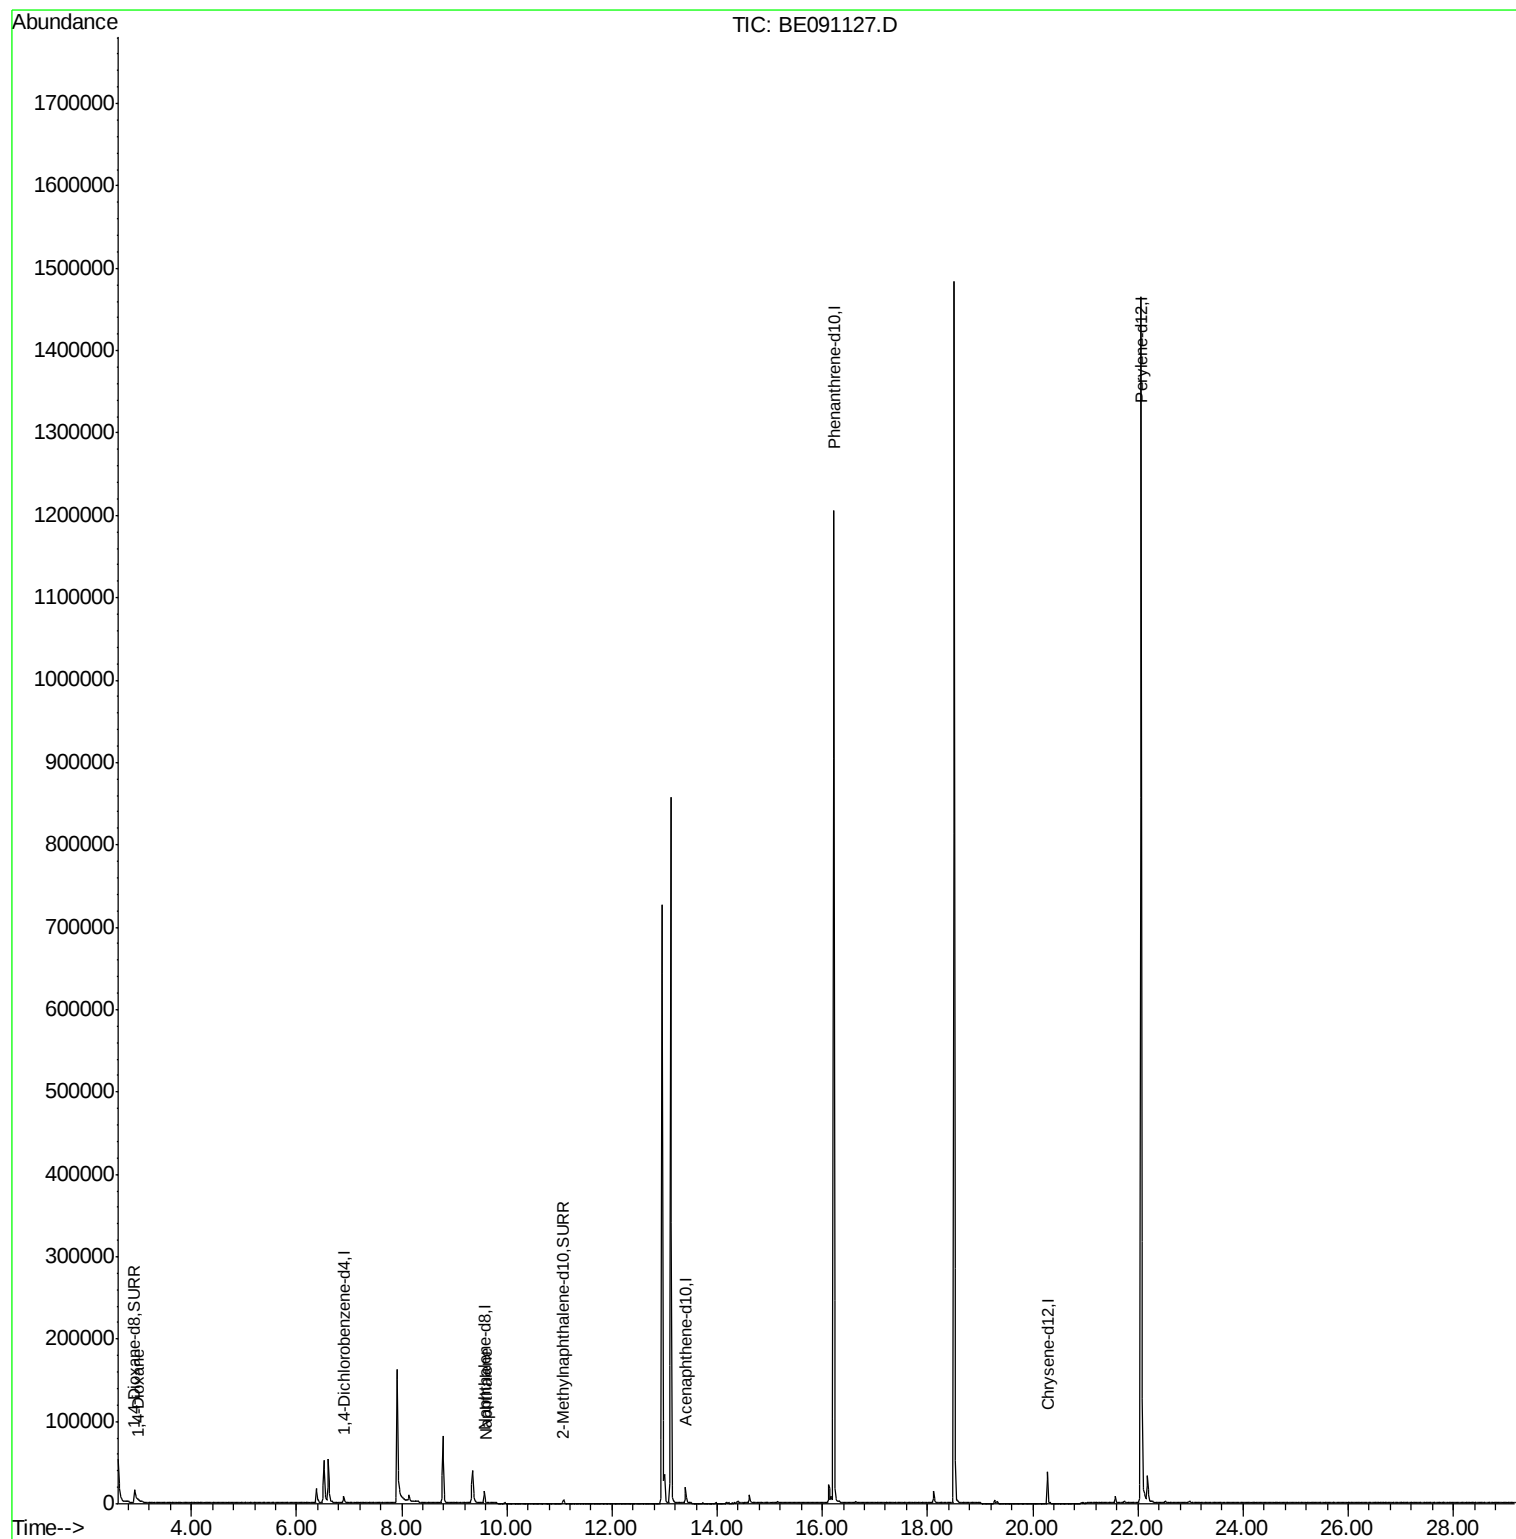

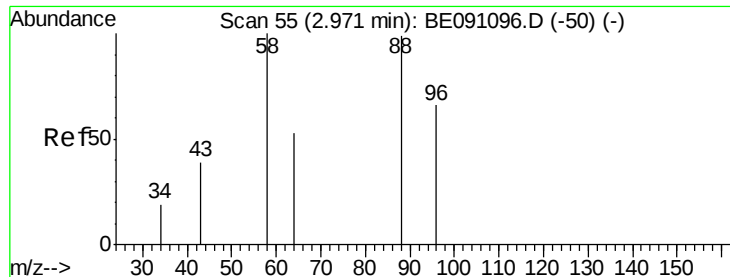

#3

1,4-Dioxane

Concen: 0.07 ng/ul

RT: 2.98 min Scan# 56

Delta R.T. 0.01 min

Lab File: BE091127.D

Acq: 12 Nov 2015 00:33

Instrument :

BNA_E

ClientSampled :

A4HR6


Tgt Ion: 88 Resp: 169

Ion Ratio Lower Upper

88 100

58 21.3 55.4 83.2#




43 0.0 24.2 36.2#

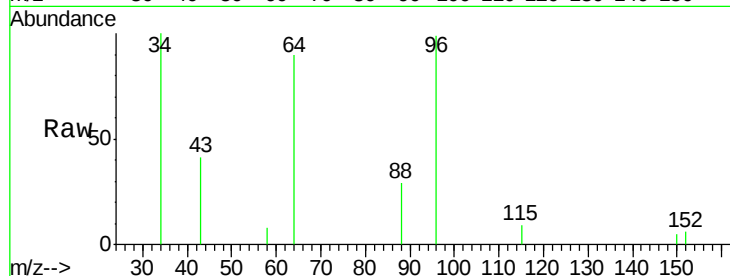

Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

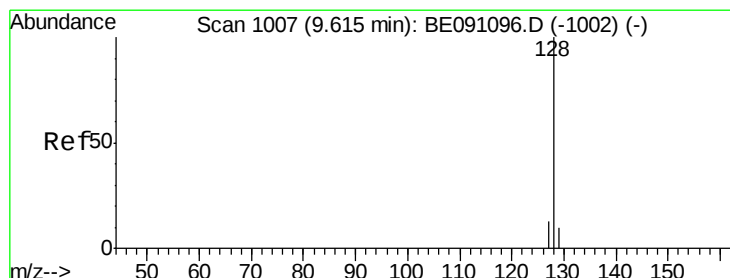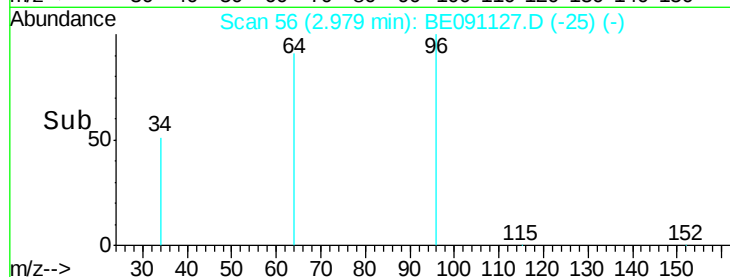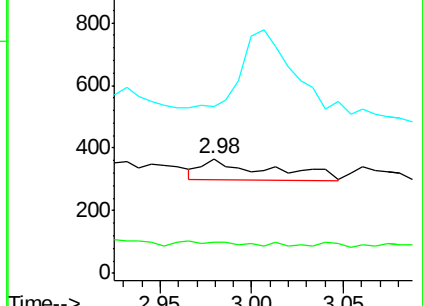

#5

Naphthalene

Concen: 0.03 ng/ul

RT: 9.61 min Scan# 1007

Delta R.T. -0.00 min

Lab File: BE091127.D

Acq: 12 Nov 2015 00:33


Tgt Ion: 128 Resp: 1303

Ion Ratio Lower Upper

128 100

129 24.3 9.8 14.8#

127 18.6 10.7 16.1#

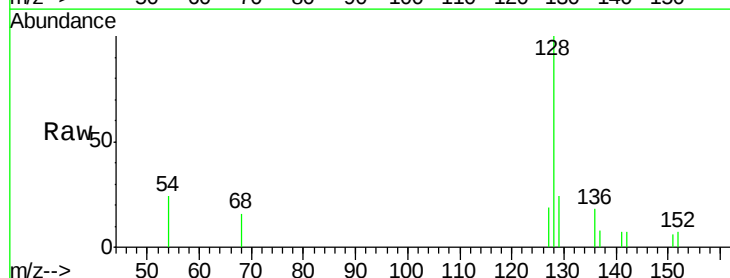

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

