

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091115.D
 Acq On : 11 Nov 2015 17:17
 Operator : UM/NP
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.493

Quant Time: Nov 13 15:31:00 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:54 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3133	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	17223	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	8685	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.14	188	22276	0.40	ng/ul	0.00
18) Chrysene-d12	20.29	240	22558	0.40	ng/ul	0.00
22) Perylene-d12	22.19	264	19947	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.95	96	3864	1.71	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.08	152	8903	0.38	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	21426	0.34	ng/ul	0.00
Target Compounds						
3) 1,4-Dioxane	2.96	88	4340	1.70	ng/ul#	64
5) Naphthalene	9.61	128	15887	0.37	ng/ul	98
7) 2-Methylnaphthalene	11.15	142	10296m	0.37	ng/ul	99
9) Acenaphthylene	13.15	152	17113	0.39	ng/ul	99
10) Acenaphthene	13.46	153	11895	0.40	ng/ul	90
11) Fluorene	14.45	166	14467	0.38	ng/ul	94
13) Pentachlorophenol	15.89	266	535	0.25	ng/ul	98
14) Phenanthrene	16.17	178	97279	0.38	ng/ul	96
15) Anthracene	16.25	178	88193	0.38	ng/ul	98
17) Fluoranthene	18.15	202	105674	0.35	ng/ul	89
19) Pyrene	18.53	202	96838	0.38	ng/ul#	80
20) Benzo(a)anthracene	20.26	228	21442	0.37	ng/ul	98
21) Chrysene	20.32	228	25572	0.38	ng/ul	97
23) Benzo(b)fluoranthene	21.62	252	24005	0.39	ng/ul	94
24) Benzo(k)fluoranthene	21.65	252	23763	0.37	ng/ul	94
25) Benzo(a)pyrene	22.09	252	22044	0.38	ng/ul#	91
26) Indeno(1,2,3-cd)pyrene	23.83	276	91935m	0.38	ng/ul	71
27) Dibenzo(a,h)anthracene	23.79	278	21662	0.38	ng/ul#	93
28) Benzo(g,h,i)perylene	24.39	276	95237	0.38	ng/ul	93

U.M
 11/24/15

U.M
 11/24/15

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091115.D
 Acq On : 11 Nov 2015 17:17
 Operator : UM/NP
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.493

Quant Time: Nov 13 15:20:02 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:54 PM

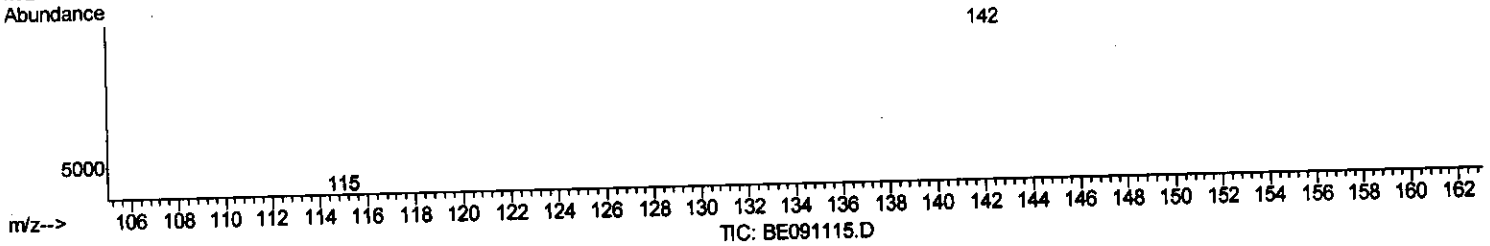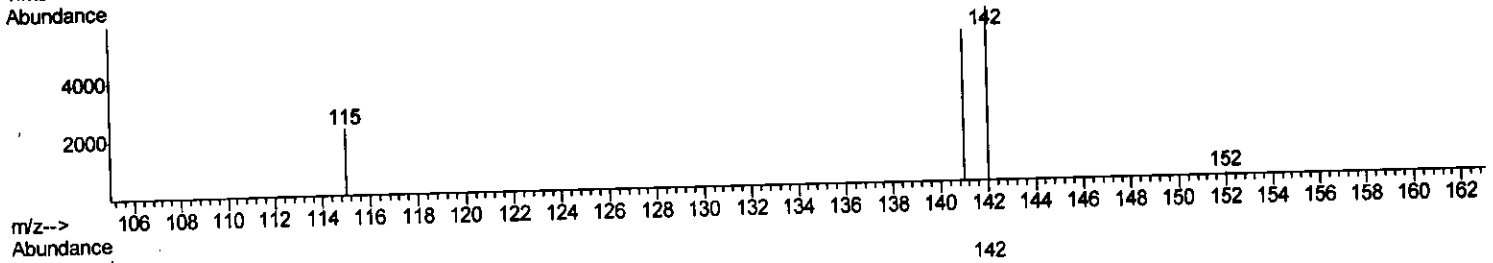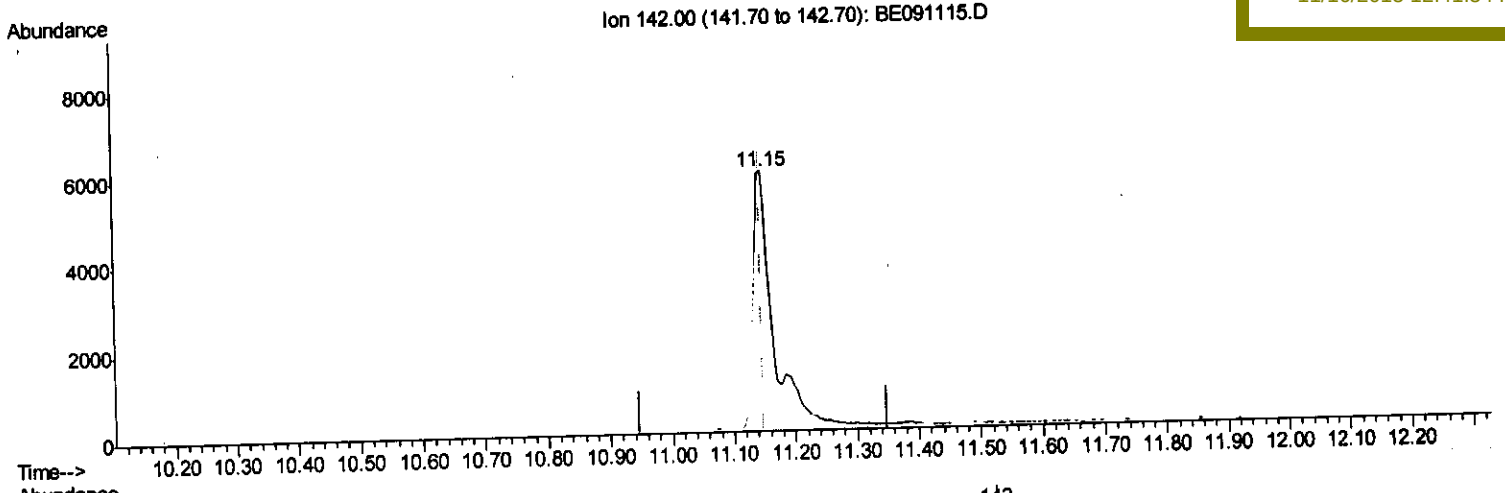

(7) 2-Methylnaphthalene

11.148min (-0.000) 0.48ng/ul

response 13380

Ion	Exp%	Act%
142.00	100	100
141.00	87.90	74.10
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091115.D
 Acq On : 11 Nov 2015 17:17
 Operator : UM/NP
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.493

Quant Time: Nov 13 15:20:02 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:54 PM

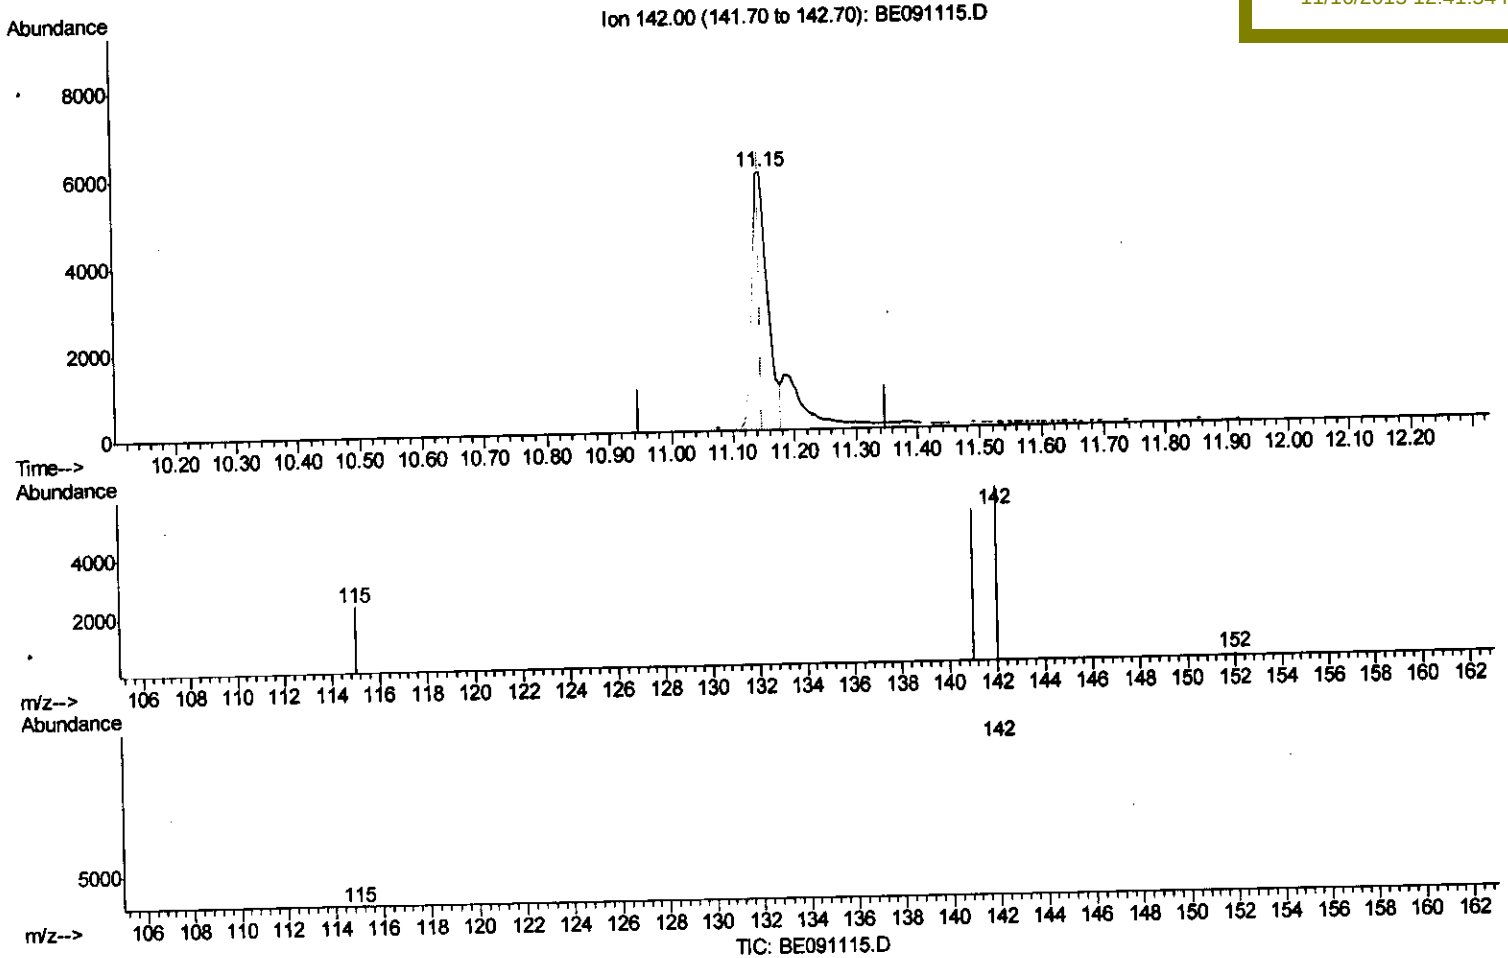

(7) 2-Methylnaphthalene

11.148min (-0.000) 0.37ng/ul m

response 10296

Ion	Exp%	Act%
142.00	100	100
141.00	87.90	96.29
0.00	0.00	0.00
0.00	0.00	0.00

> 6.M
 11/24/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091115.D
 Acq On : 11 Nov 2015 17:17
 Operator : UM/NP
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.493

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:54 PM

Quant Time: Nov 13 15:20:02 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

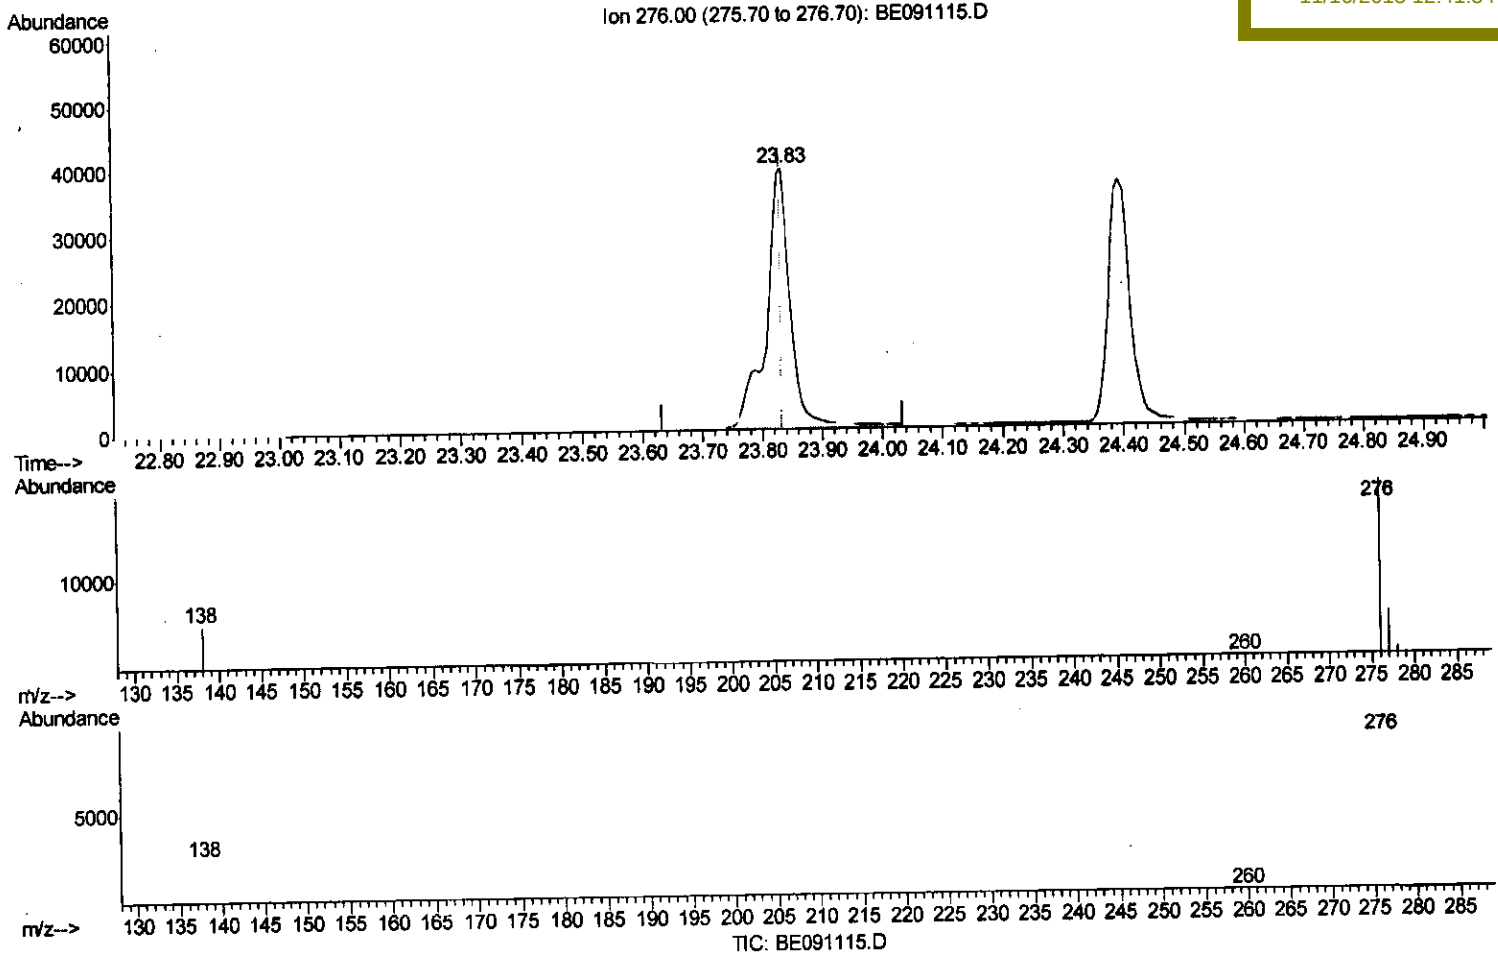

(26) Indeno(1,2,3-cd)pyrene

23.833min (-0.000) 0.45ng/ul

response 109501

Ion	Exp%	Act%
276.00	100	100
138.00	34.40	20.13#
277.00	24.10	19.70
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091115.D
 Acq On : 11 Nov 2015 17:17
 Operator : UM/NP
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 LabSampleId :
 SSTD0.493

Quant Time: Nov 13 15:20:02 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:54 PM

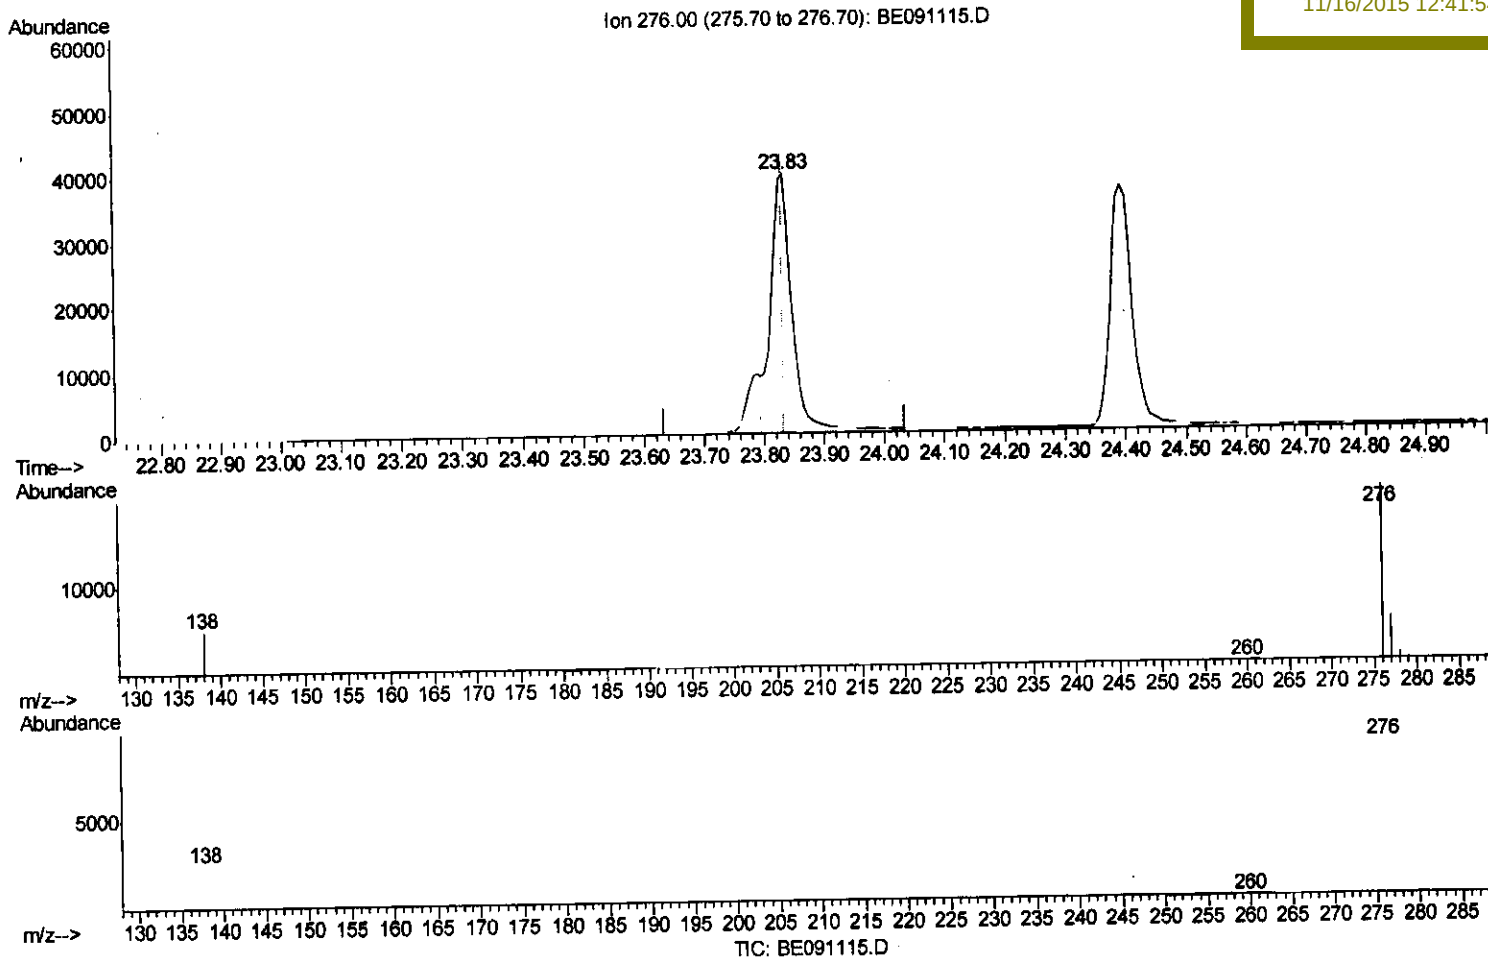

(26) Indeno(1,2,3-cd)pyrene
 23.833min (-0.000) 0.38ng/ui m
 response 91935

> U.M
 11/24/15

Ion	Exp%	Act%
276.00	100	100
138.00	34.40	23.97#
277.00	24.10	23.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091115.D
Acq On : 11 Nov 2015 17:17
Operator : UM/NP
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
LabSampleId :
SSTD0.493

Quant Time: Nov 13 15:31:00 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:41:54 PM

