

Data Path : Z:\HPCHEM1\BNA_E\DATA\BET102715
 Data File : BET102715.D
 Acq On : 13 Nov 2015 17:53
 Operator : UM/NP
 Sample : PB86557BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK57

Quant Time: Nov 13 15:33:06 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant File : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:56 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3132	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	17512	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	10213	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.14	188	24365m	0.40	ng/ul	0.00
18) Chrysene-d12	20.29	240	26394	0.40	ng/ul	0.00
22) Benzo[a]pyrene-d12	22.19	264	24734m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.91	96	27245	11.21	ng/ul	-0.04
6) 2-Methylnaphthalene-d10	11.08	152	7168	0.30	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	17847	0.26	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

6 U.M
 11/24/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111116.D
 Data File : BE091116.D
 Acq On : 11 Nov 2015 17:53
 Operator : CR/NP
 Sample : DB86557BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK57

Quant Time: Nov 13 15:20:12 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:56 PM

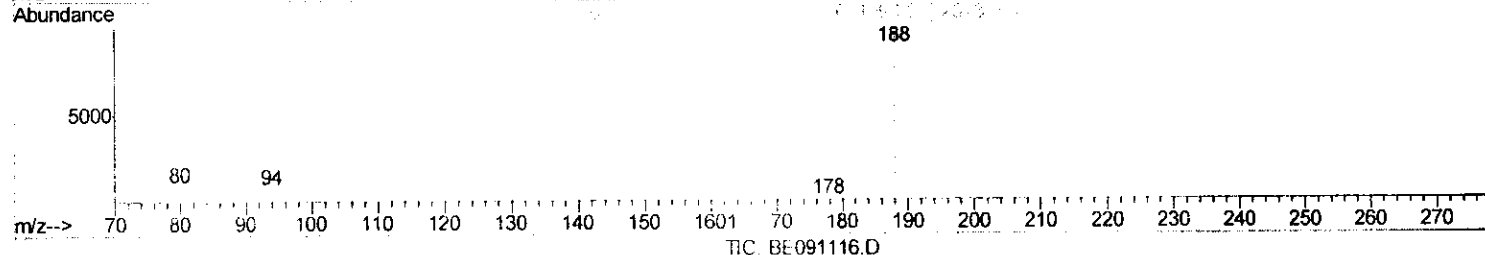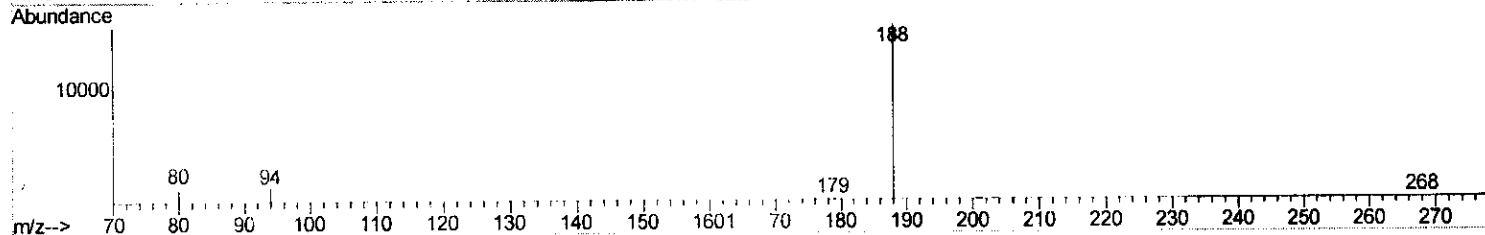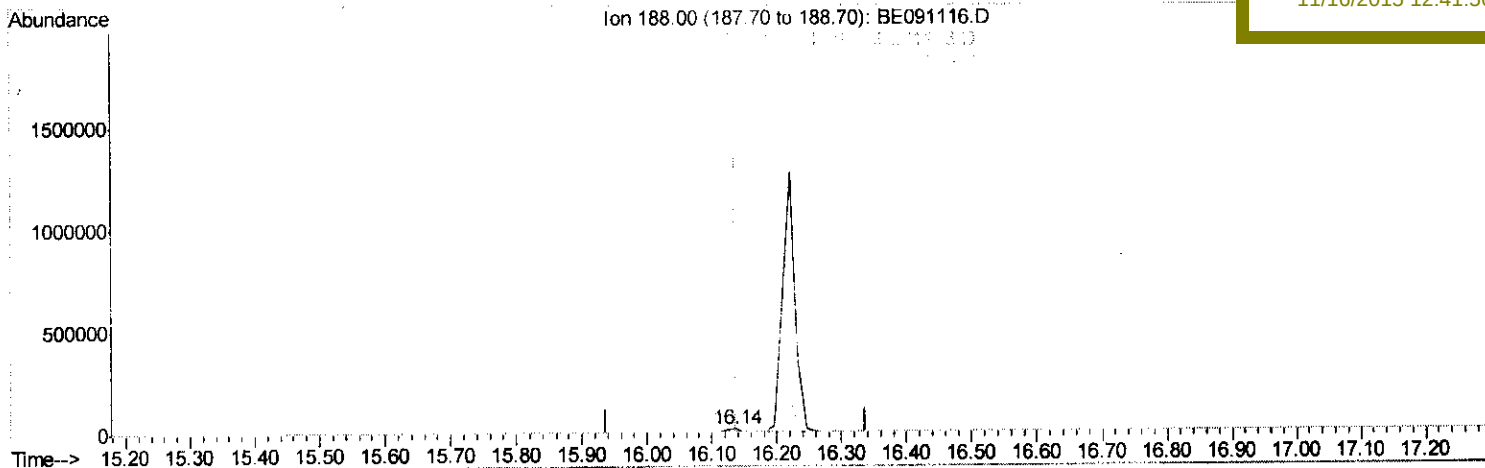

(12) Phenanthrene-d10 (I)

16.136min (-0.001) 0.40ng/ul m

response 24365

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	8.46
80.00	8.90	8.76
0.00	0.00	0.00

> U.M
 11/24/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091116.D
 Acq On : 11 Nov 2015 17:53
 Operator : UM/NP
 Sample : PB86557BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK57

Quant Time: Nov 13 15:20:12 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:56 PM

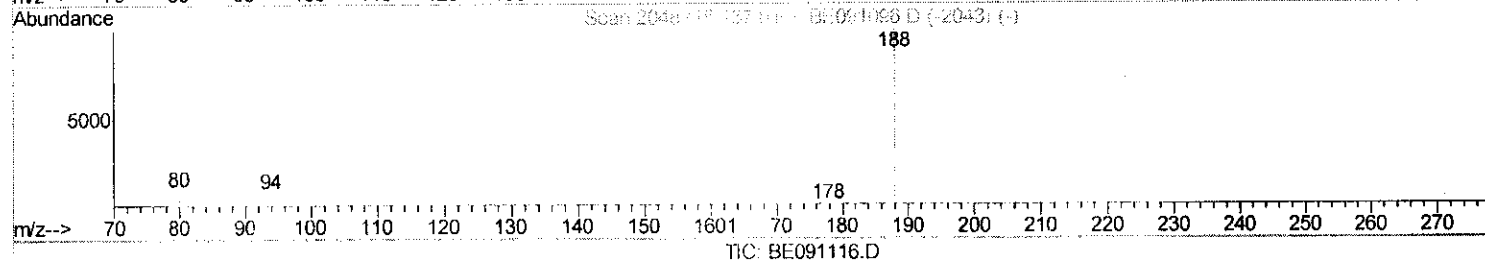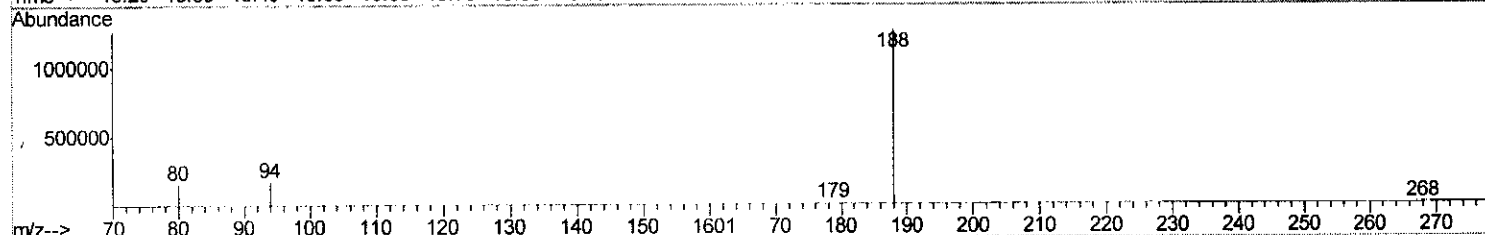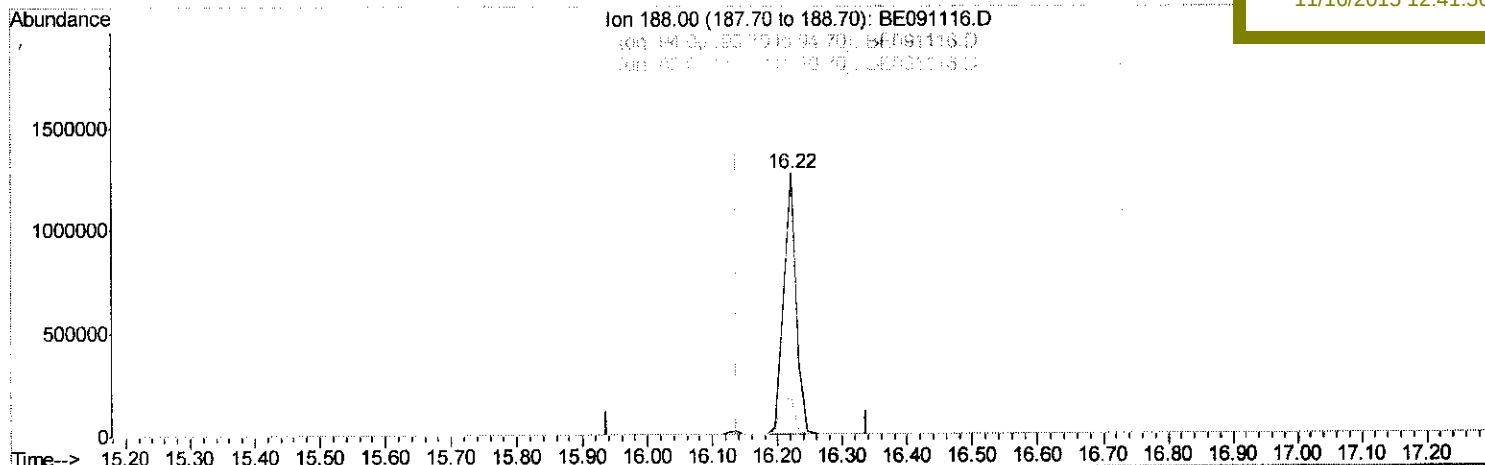

(12) Phenanthrene-d10 (I)

16.221min (+0.083) 0.40ng/ui

response 1672885

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	13.52#
80.00	8.90	12.08#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091116.D
 Acq On : 11 Nov 2015 17:53
 Operator : GM/NP
 Sample : P88655/BLE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK57

Quant Time: Nov 13 15:32:13 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:41:56 PM

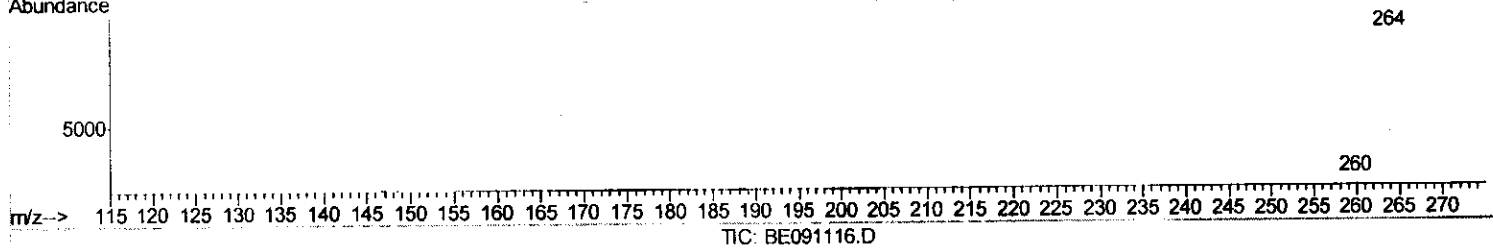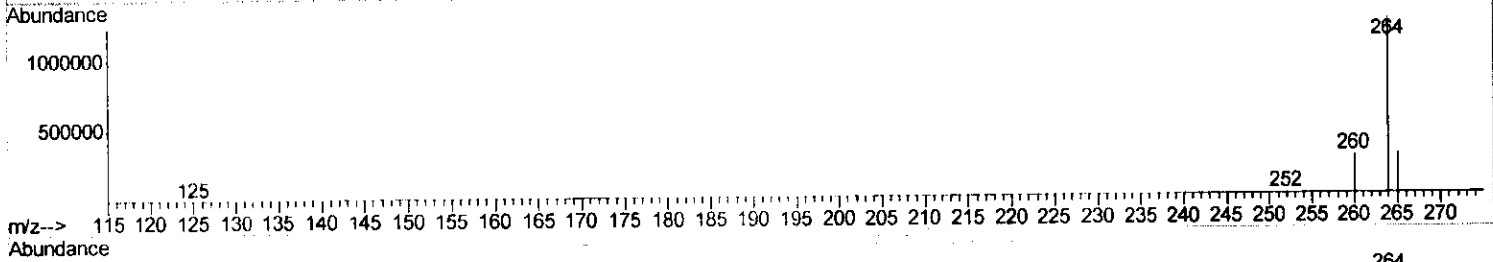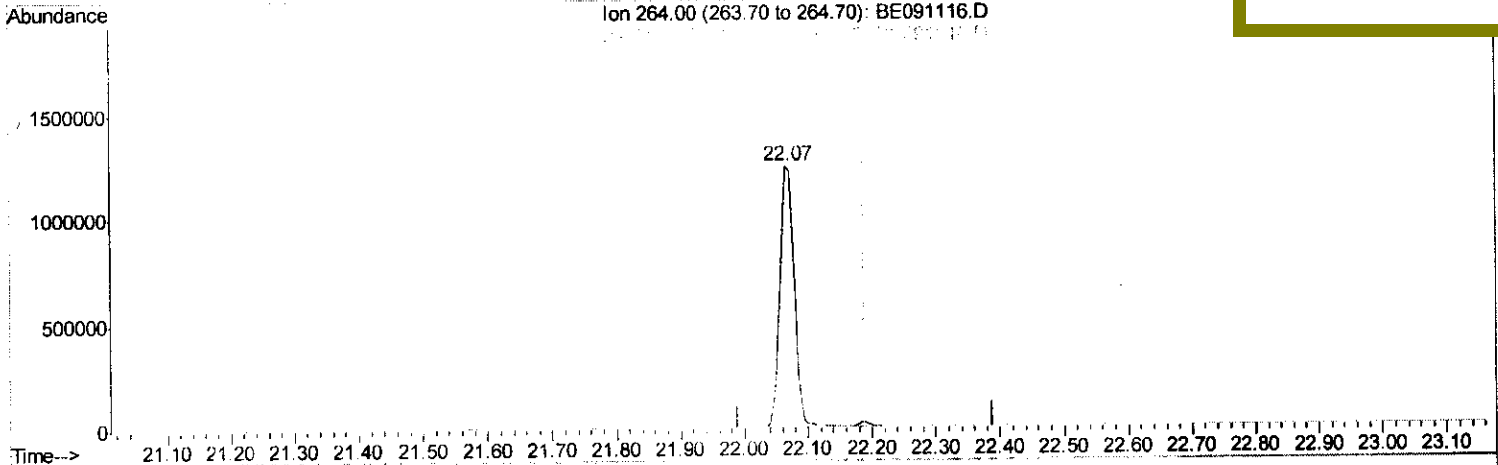

(22) Perylene-d12 (I)

22.067min (-0.122) 0.40ng/ul

response 1957758

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	21.96#
265.00	34.70	22.44#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111116\A
Data File : BE091116.D
Acq On : 11 Nov 2015 17:53
Operator : UM/NP
Sample : PB8655/BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK57

Quant Time: Nov 13 15:32:13 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-BPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:41:56 PM

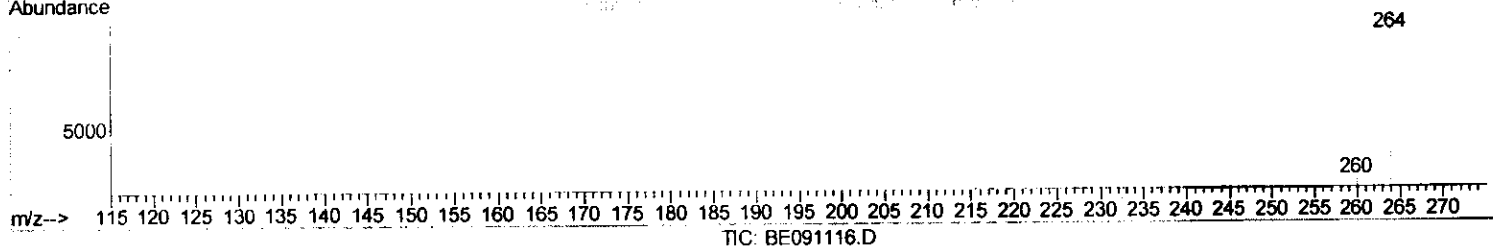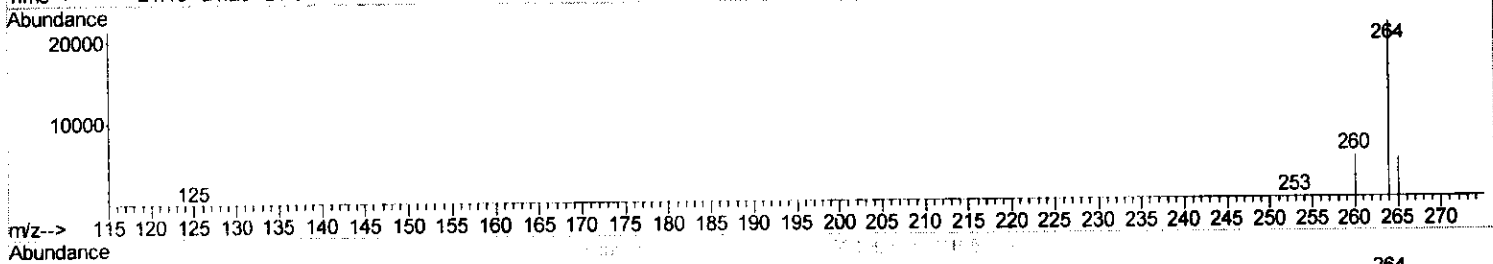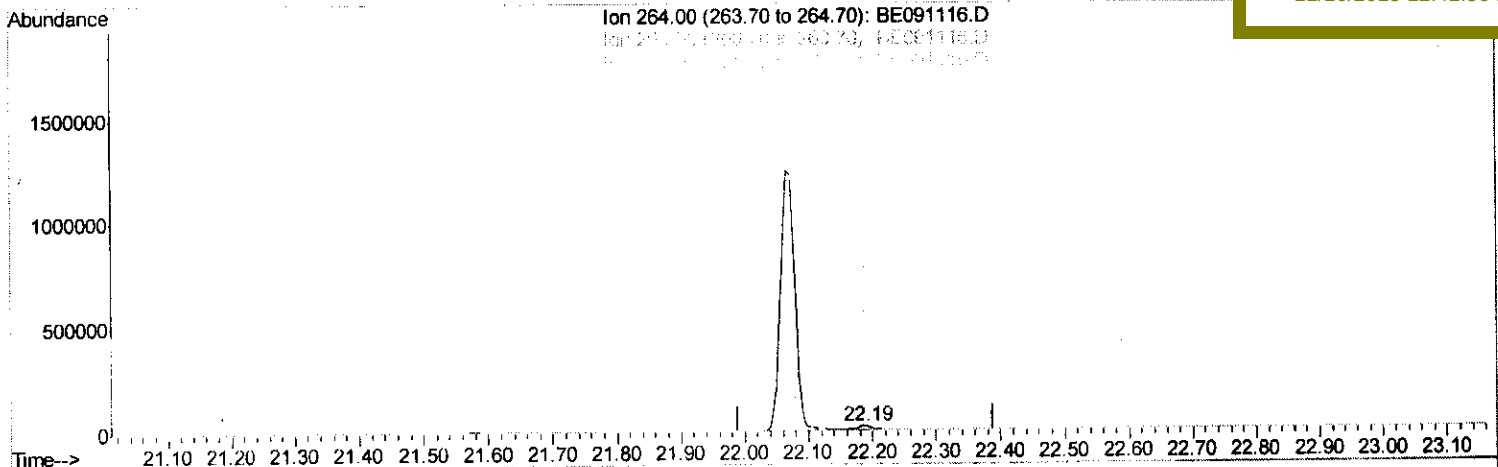

(22) Perylene-d12 (I)

22.190min (+0.001) 0.40ng/ul m

response 24734

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	24.12
265.00	34.70	22.69#
0.00	0.00	0.00

U.M
11/24/15

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091116.D
Acq On : 11 Nov 2015 17:53
Operator : UM/NP
Sample : B886557BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK57

Quant Time: Nov 13 15:33:06 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:41:56 PM

